

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
 Data File : FF003198.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jan 2019 16:25
 Operator : AJ\SJ
 Sample : K1005-01 5X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 11 01:07:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.614	420092	3.160 ug/ml
Target Compounds			
4) N-TETRADECANE	8.217	214485	1.407 ug/ml
7) N-EICOSANE	12.563	889062	5.839 ug/ml
10) N-TETRACOSANE	14.784f	312574	2.098 ug/ml
11) N-HEXACOSANE	15.840	126579	0.860 ug/ml
12) N-OCTACOSANE	16.792	285004	1.958 ug/ml
13) N-TRIACONTANE	17.681	368520	2.580 ug/ml
14) N-DOTRIACONTANE	18.522	471465	3.539 ug/ml
15) N-TETRATRIACONTANE	19.307	133770	1.079 ug/ml
16) N-HEXATRIACONTANE	20.091	1089907	9.662 ug/ml
18) N-TETRACONTANE	21.718	2125075	21.080 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
Data File : FF003198.D
Signal(s) : FID2B.ch
Acq On : 10 Jan 2019 16:25
Operator : AJ\SJ
Sample : K1005-01 5X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 11 01:07:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

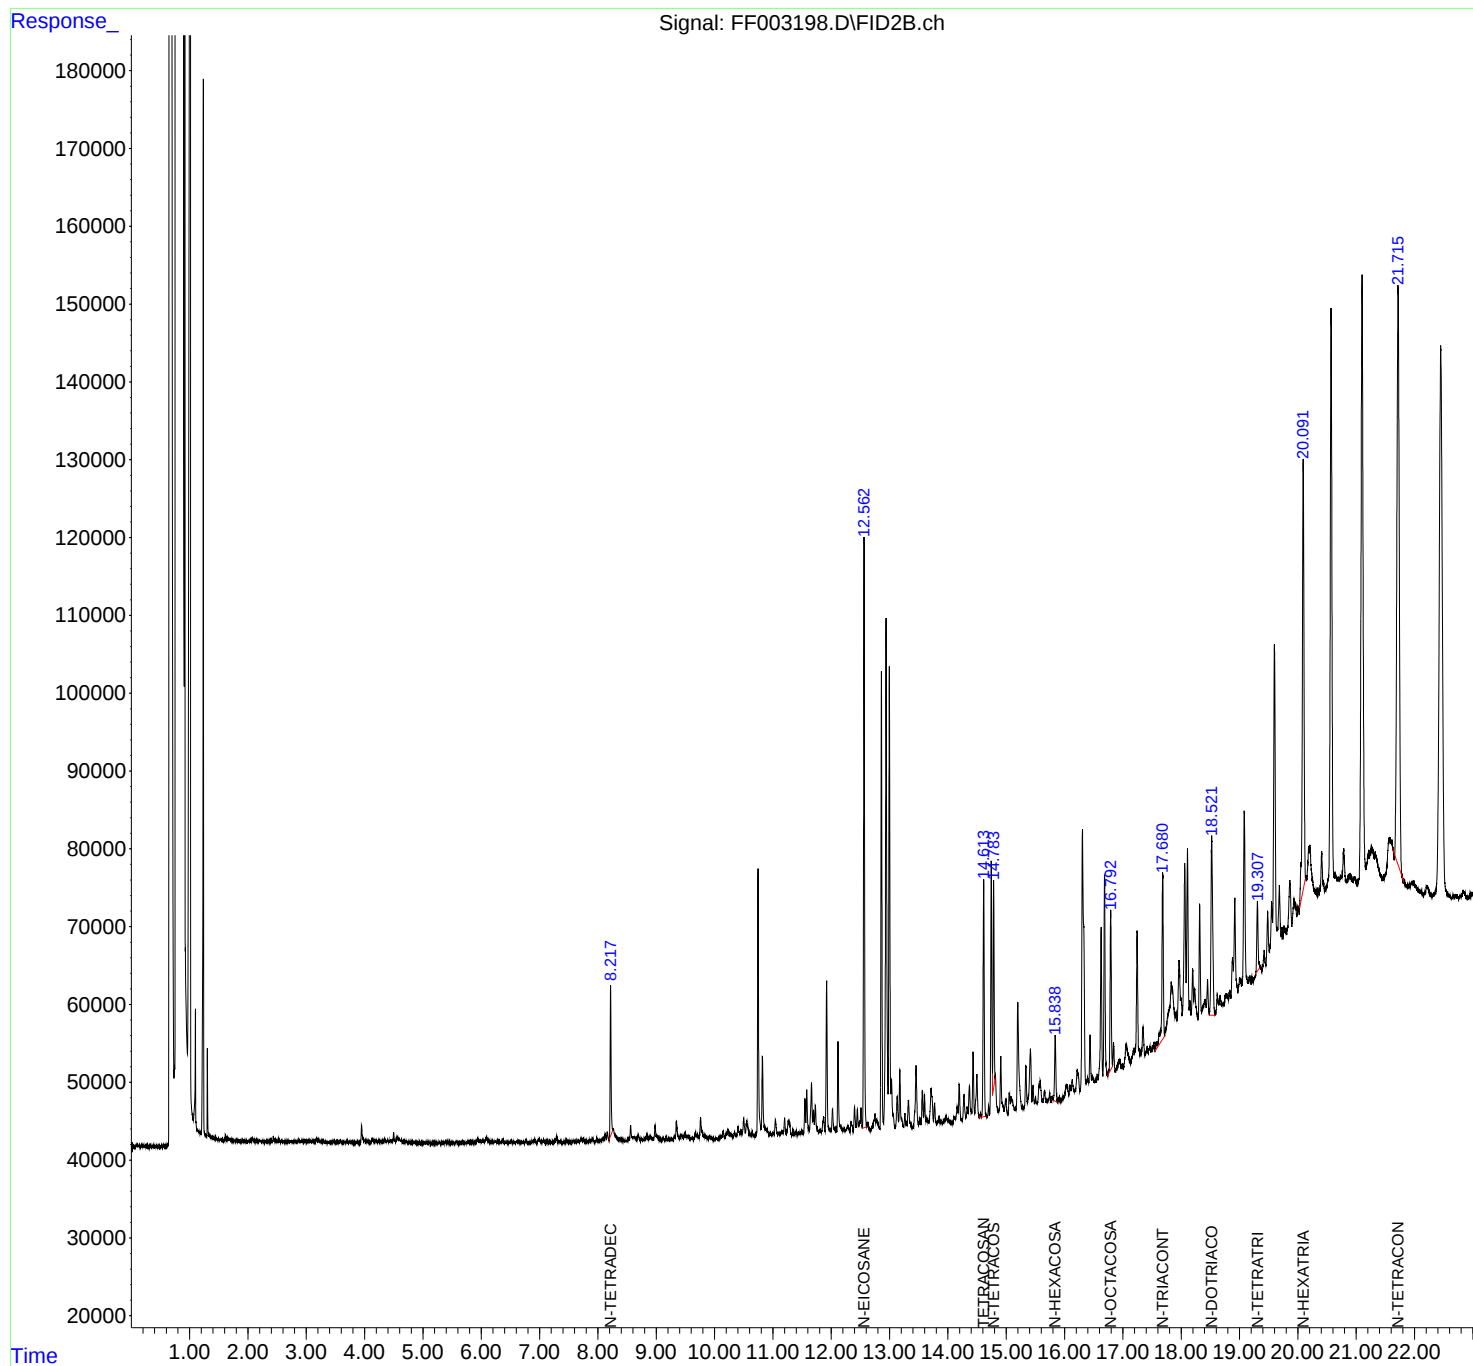


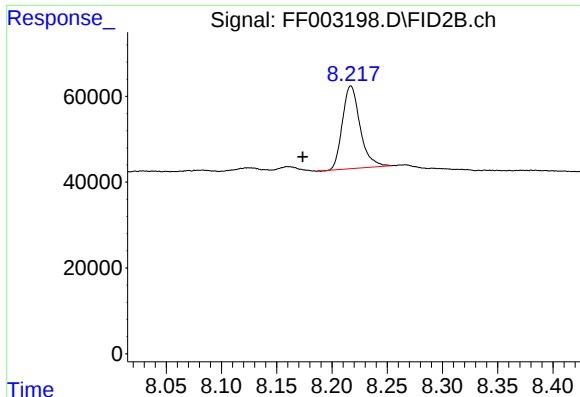

#4 N-TETRADECANE


R.T.: 8.217 min
Delta R.T.: 0.044 min
Response: 214485
Conc: 1.41 ug/ml

Instrument :
FID_F
ClientSampleId :

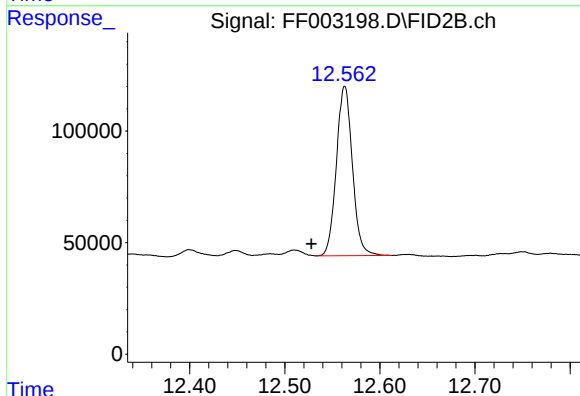


#7 N-EICOSANE

R.T.: 12.563 min
Delta R.T.: 0.035 min
Response: 889062
Conc: 5.84 ug/ml

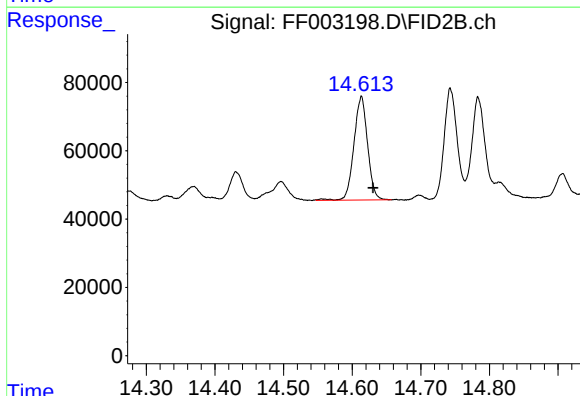


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.614 min
Delta R.T.: -0.017 min
Response: 420092
Conc: 3.16 ug/ml

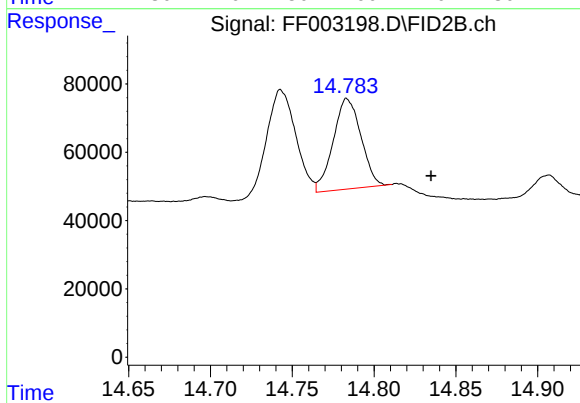

#10 N-TETRACOSANE


R.T.: 14.784 min
Delta R.T.: -0.051 min
Response: 312574
Conc: 2.10 ug/ml

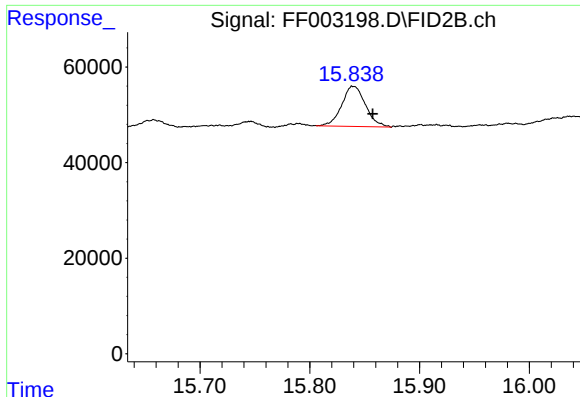

#11 N-HEXACOSANE


R.T.: 15.840 min
Delta R.T.: -0.018 min
Response: 126579
Conc: 0.86 ug/ml

Instrument :
FID_F
ClientSampleId :

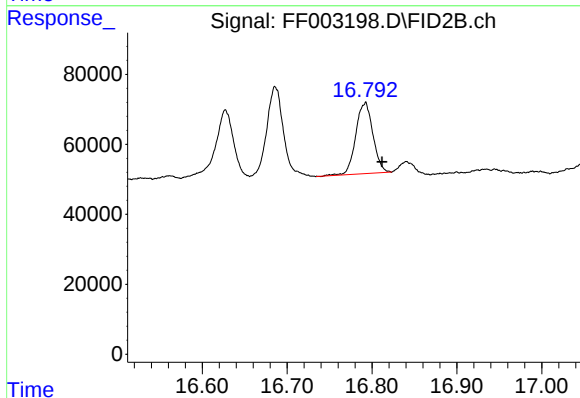


#12 N-OCTACOSANE

R.T.: 16.792 min
Delta R.T.: -0.020 min
Response: 285004
Conc: 1.96 ug/ml

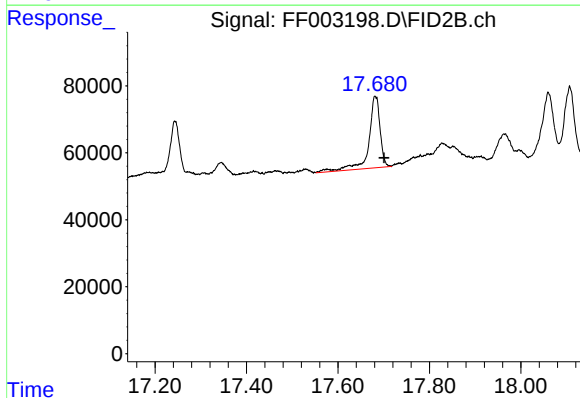


#13 N-TRIACONTANE

R.T.: 17.681 min
Delta R.T.: -0.020 min
Response: 368520
Conc: 2.58 ug/ml

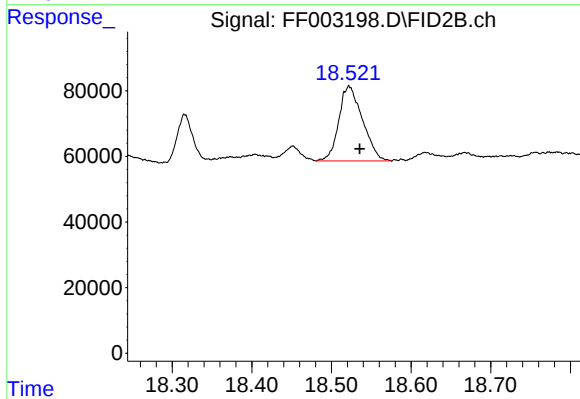

#14 N-DOTRIACONTANE


R.T.: 18.522 min
Delta R.T.: -0.013 min
Response: 471465
Conc: 3.54 ug/ml

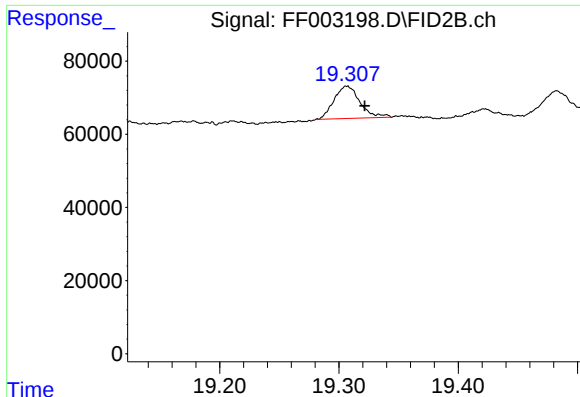

#15 N-TETRATRIACONTANE


R.T.: 19.307 min
Delta R.T.: -0.015 min
Response: 133770
Conc: 1.08 ug/ml

Instrument :
FID_F
ClientSampleId :

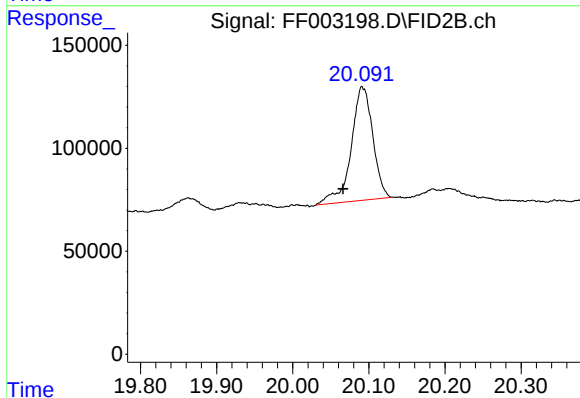

#16 N-HEXATRIACONTANE

R.T.: 20.091 min
Delta R.T.: 0.025 min
Response: 1089907
Conc: 9.66 ug/ml

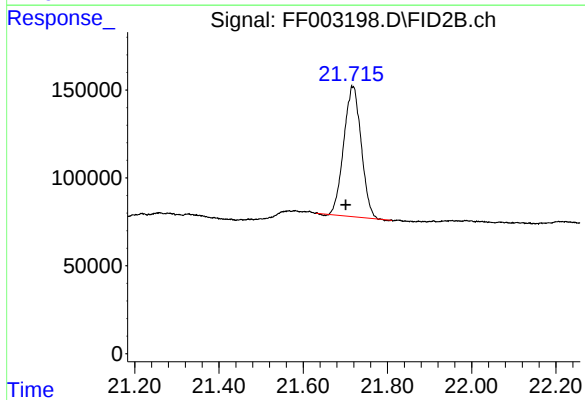

#18 N-TETRACONTANE

R.T.: 21.718 min
Delta R.T.: 0.016 min
Response: 2125075
Conc: 21.08 ug/ml