

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
 Data File : FF003199.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jan 2019 16:55
 Operator : AJ\SJ
 Sample : K1005-05 5X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 11 01:07:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.611	352418	2.651 ug/ml
Target Compounds			
2) N-DECANE	4.351	996042	6.633 ug/ml
3) N-DODECANE	6.369	1234728	8.159 ug/ml
4) N-TETRADECANE	8.160	797387	5.230 ug/ml
5) N-HEXADECANE	9.758	159929	1.043 ug/ml
11) N-HEXACOSANE	15.840	106825	0.726 ug/ml
12) N-OCTACOSANE	16.793	184956	1.271 ug/ml
13) N-TRIACONTANE	17.682	539058	3.774 ug/ml
14) N-DOTRIACONTANE	18.520	499733	3.751 ug/ml
15) N-TETRATRIACONTANE	19.309	439119	3.543 ug/ml
16) N-HEXATRIACONTANE	20.056	191054	1.694 ug/ml
17) N-OCTATRIACONTANE	20.791	231550	2.311 ug/ml
18) N-TETRACONTANE	21.719	743243	7.373 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
Data File : FF003199.D
Signal(s) : FID2B.ch
Acq On : 10 Jan 2019 16:55
Operator : AJ\SJ
Sample : K1005-05 5X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 11 01:07:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

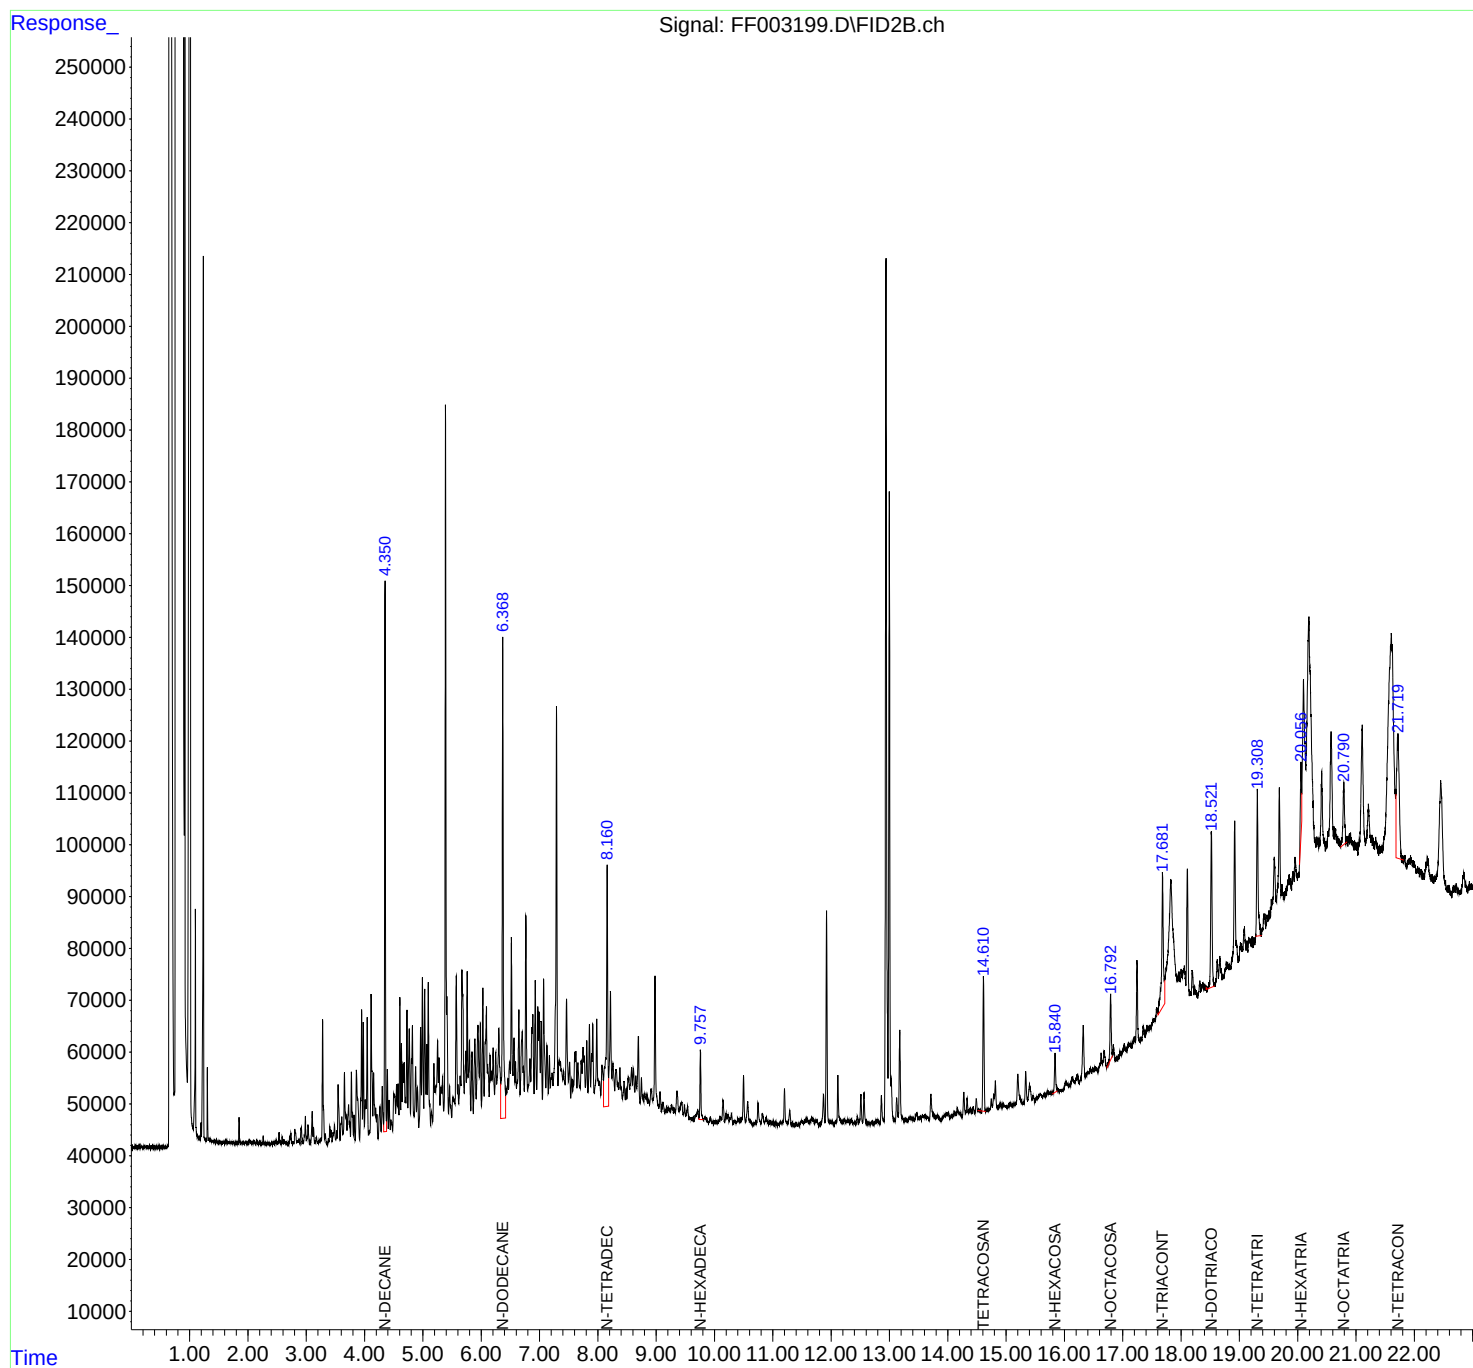


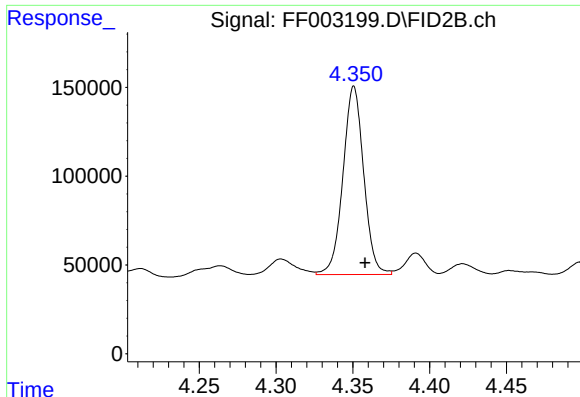

#2 N-DECANE


R.T.: 4.351 min
Delta R.T.: -0.007 min
Response: 996042
Conc: 6.63 ug/ml

Instrument :
FID_F
ClientSampleId :

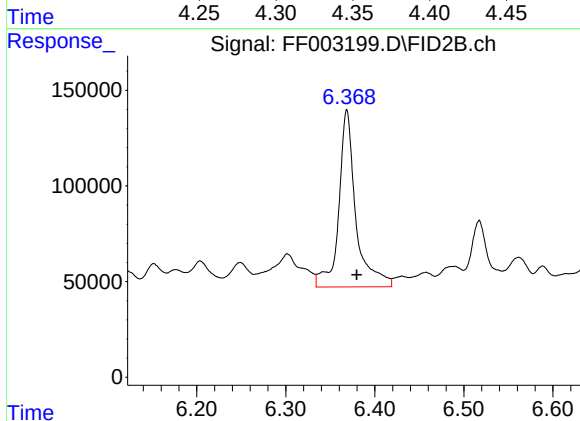


#3 N-DODECANE

R.T.: 6.369 min
Delta R.T.: -0.011 min
Response: 1234728
Conc: 8.16 ug/ml

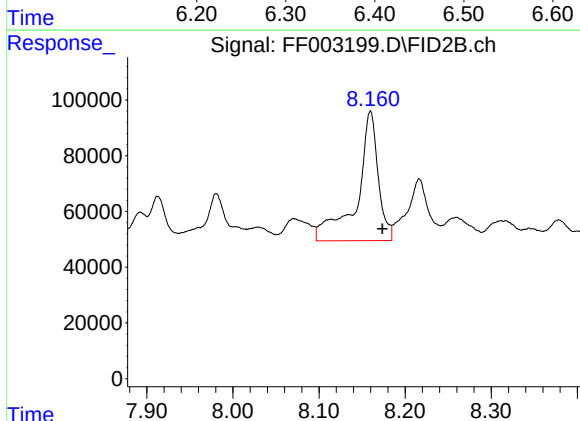


#4 N-TETRADECANE

R.T.: 8.160 min
Delta R.T.: -0.014 min
Response: 797387
Conc: 5.23 ug/ml

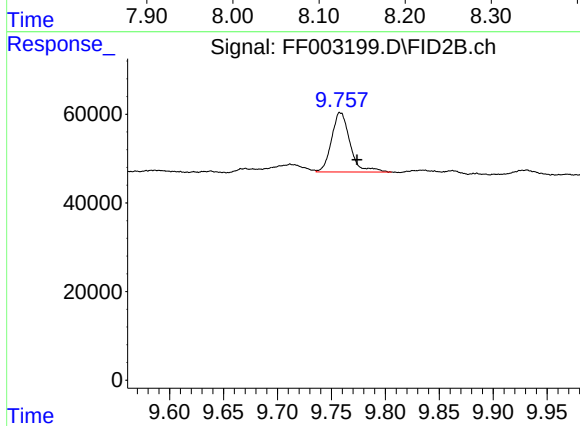

#5 N-HEXADECANE


R.T.: 9.758 min
Delta R.T.: -0.015 min
Response: 159929
Conc: 1.04 ug/ml

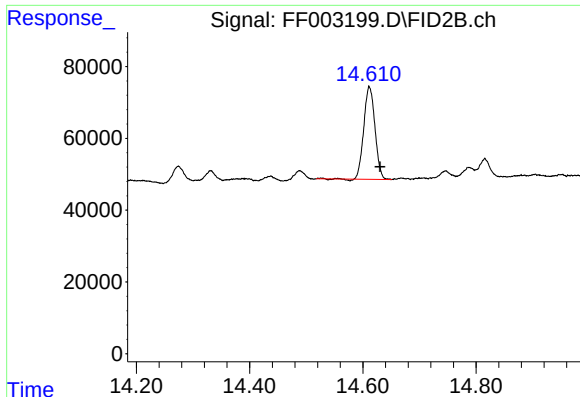

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.611 min
Delta R.T.: -0.019 min
Response: 352418
Conc: 2.65 ug/ml

Instrument :
FID_F
ClientSampleId :

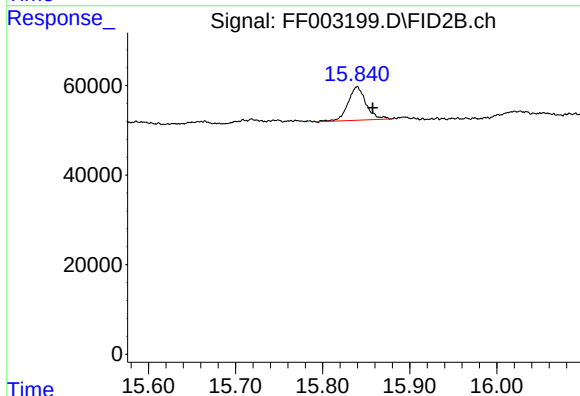


#11 N-HEXACOSANE

R.T.: 15.840 min
Delta R.T.: -0.018 min
Response: 106825
Conc: 0.73 ug/ml

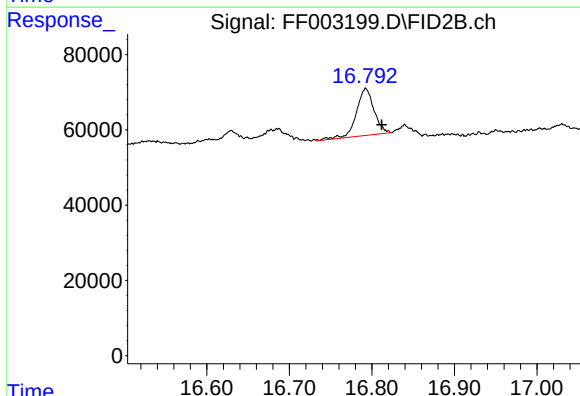


#12 N-OCTACOSANE

R.T.: 16.793 min
Delta R.T.: -0.019 min
Response: 184956
Conc: 1.27 ug/ml

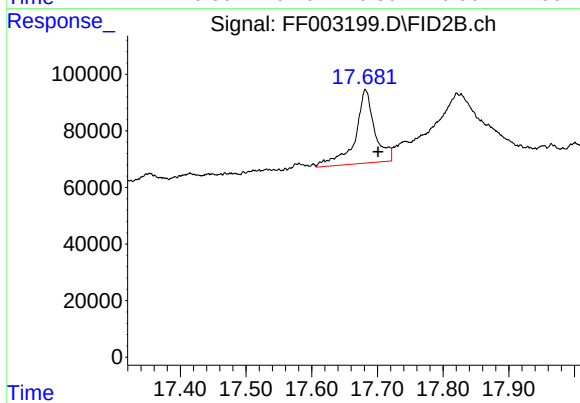

#13 N-TRIACONTANE


R.T.: 17.682 min
Delta R.T.: -0.019 min
Response: 539058
Conc: 3.77 ug/ml

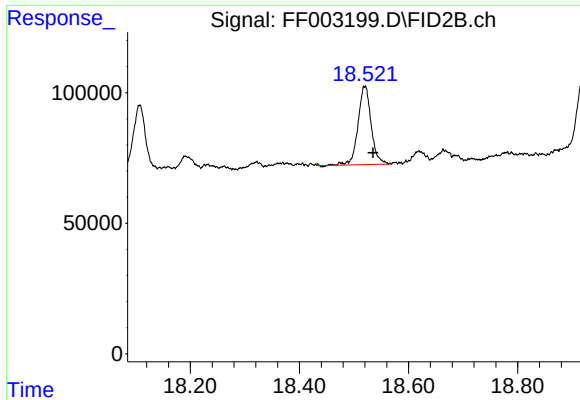

#14 N-DOTRIACONTANE


R.T.: 18.520 min
Delta R.T.: -0.015 min
Response: 499733
Conc: 3.75 ug/ml

Instrument :
FID_F
ClientSampleId :

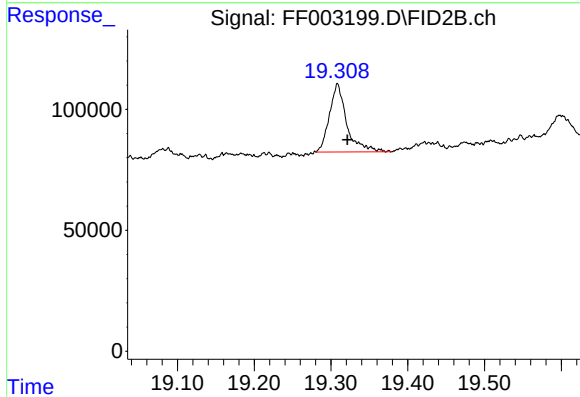


#15 N-TETRATRIACONTANE

R.T.: 19.309 min
Delta R.T.: -0.013 min
Response: 439119
Conc: 3.54 ug/ml

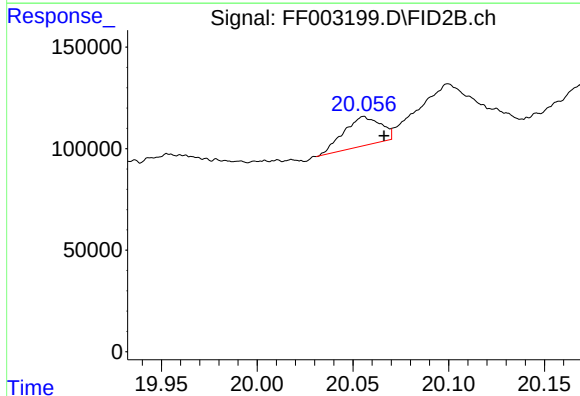


#16 N-HEXATRIACONTANE

R.T.: 20.056 min
Delta R.T.: -0.011 min
Response: 191054
Conc: 1.69 ug/ml

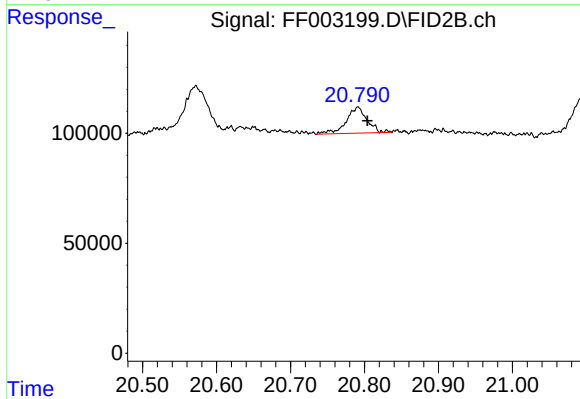

#17 N-OCTATRIACONTANE

R.T.: 20.791 min
Delta R.T.: -0.013 min
Response: 231550
Conc: 2.31 ug/ml

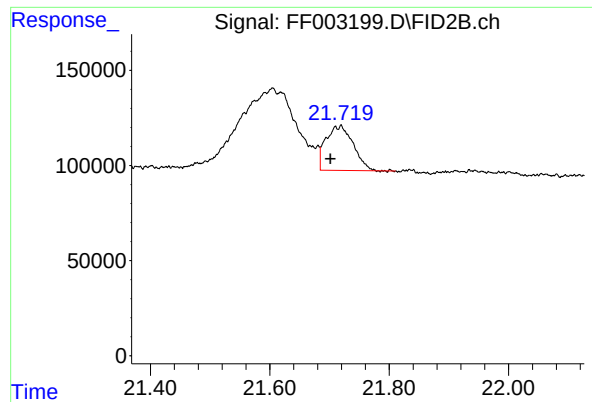

#18 N-TETRACONTANE

R.T.: 21.719 min
Delta R.T.: 0.018 min
Response: 743243
Conc: 7.37 ug/ml

Instrument :
FID_F
ClientSampleId :