

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
 Data File : FF003205.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jan 2019 19:55
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 11 01:09:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.615	2158130	16.233 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.684	140880	0.986 ug/ml
14) N-DOTRIACONTANE	18.518	190706	1.431 ug/ml
16) N-HEXATRIACONTANE	20.058	53119	0.471 ug/ml
17) N-OCTATRIACONTANE	20.819	25570	0.255 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
Data File : FF003205.D
Signal(s) : FID2B.ch
Acq On : 10 Jan 2019 19:55
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 11 01:09:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

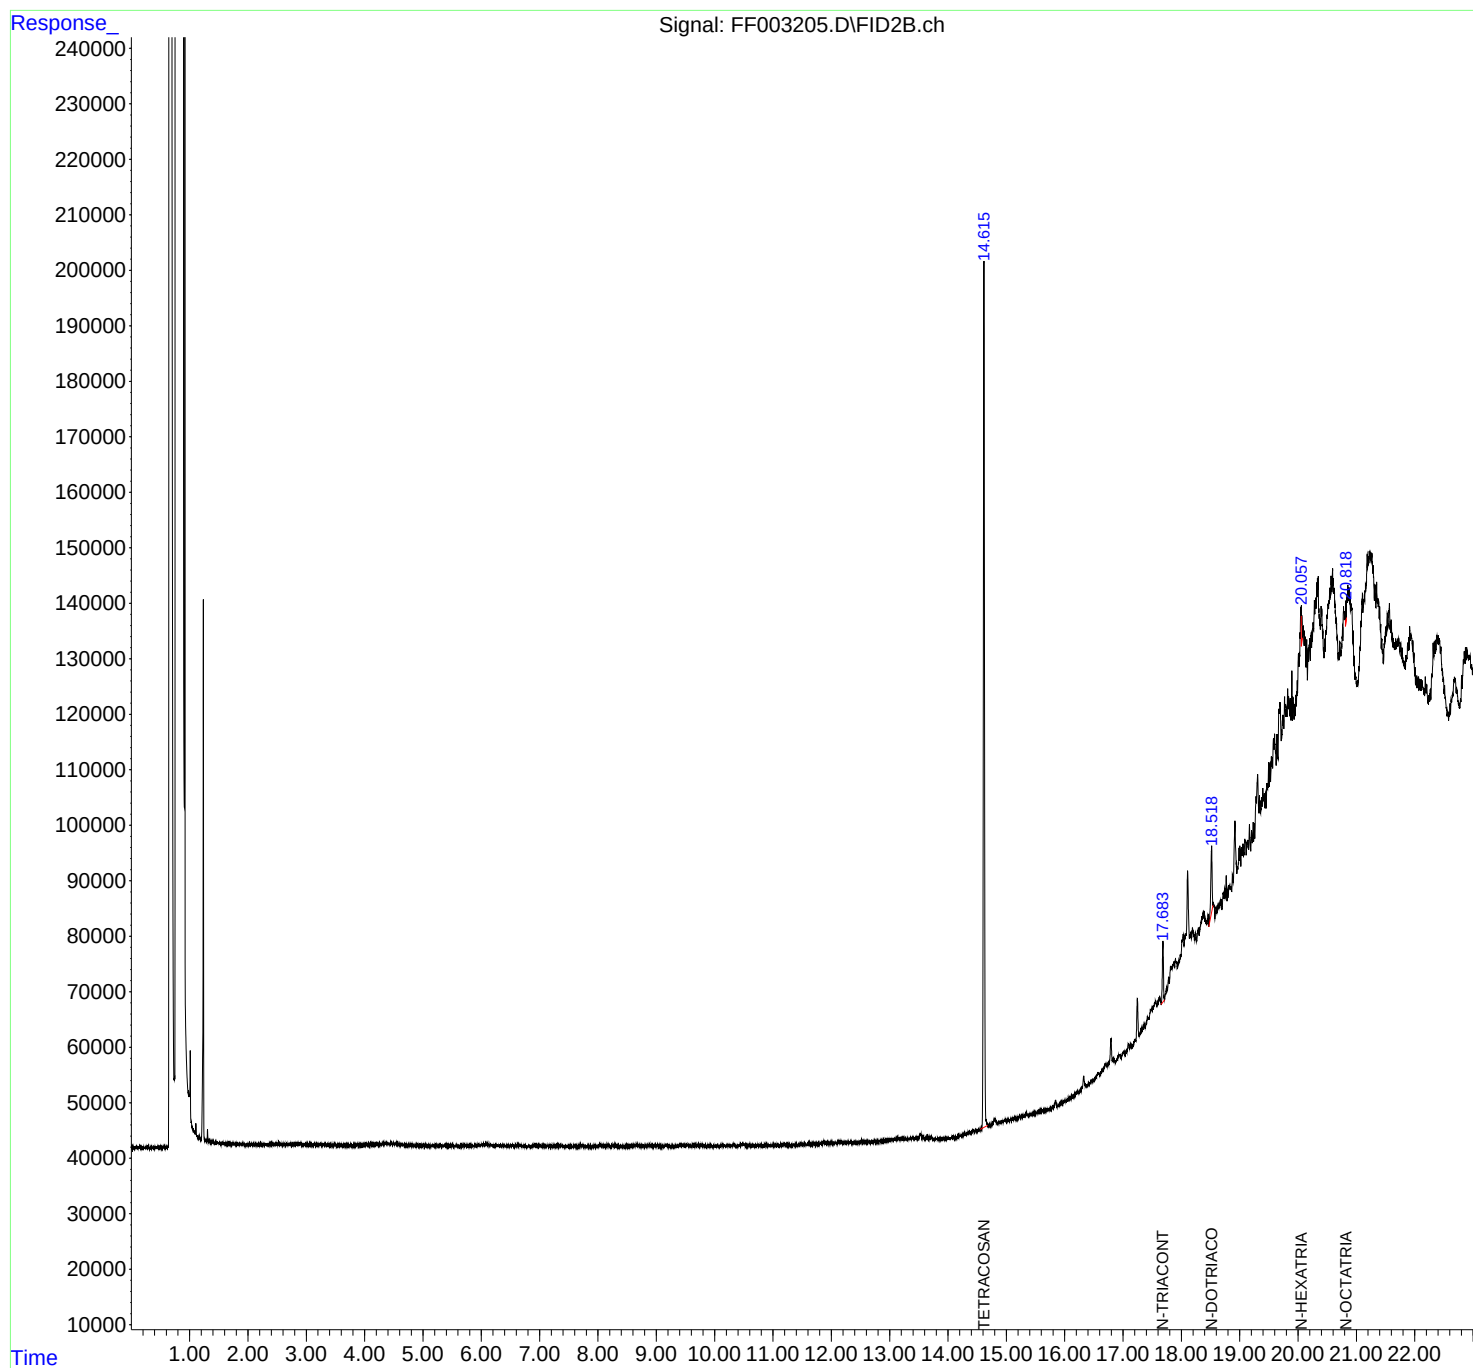


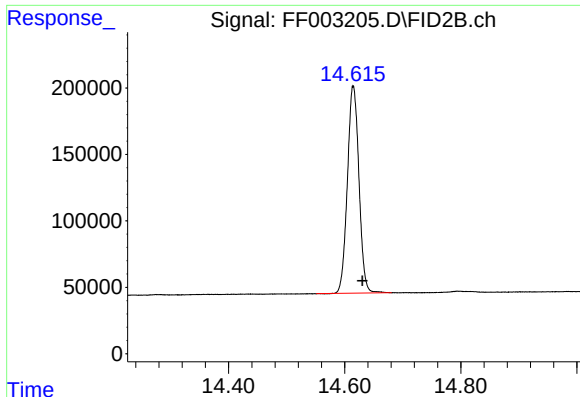

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.615 min
Delta R.T.: -0.016 min
Response: 2158130
Conc: 16.23 ug/ml

Instrument :
FID_F
ClientSampleId :

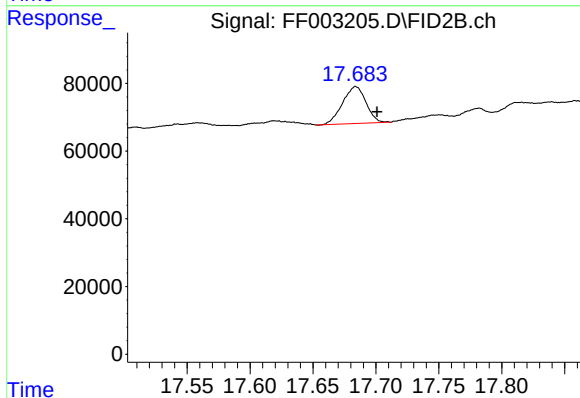


#13 N-TRIACONTANE

R.T.: 17.684 min
Delta R.T.: -0.017 min
Response: 140880
Conc: 0.99 ug/ml

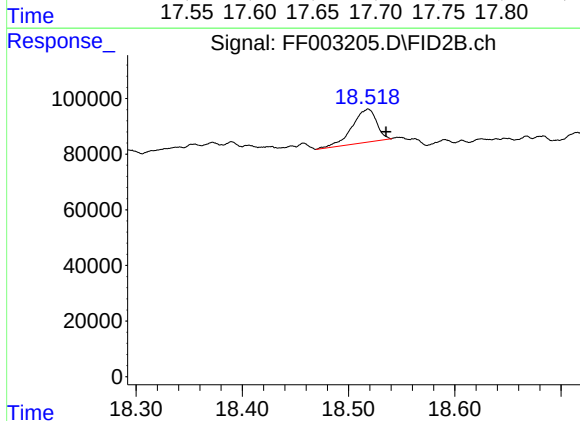


#14 N-DOTRIACONTANE

R.T.: 18.518 min
Delta R.T.: -0.017 min
Response: 190706
Conc: 1.43 ug/ml

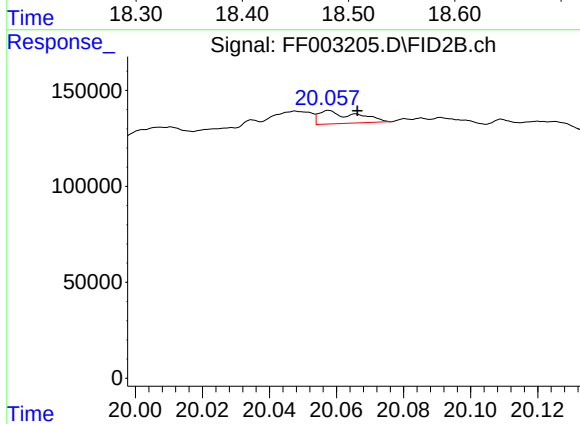

#16 N-HEXATRIACONTANE

R.T.: 20.058 min
Delta R.T.: -0.009 min
Response: 53119
Conc: 0.47 ug/ml

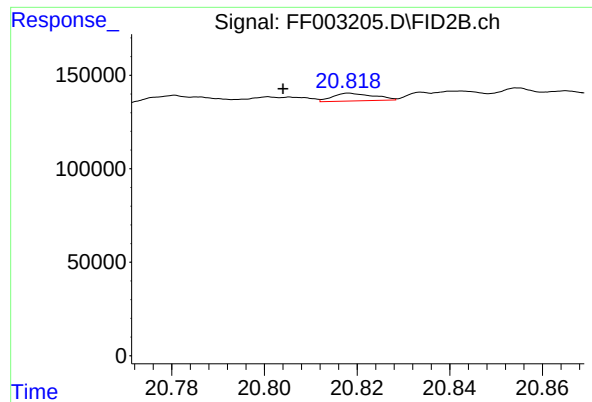

#17 N-OCTATRIACONTANE

R.T.: 20.819 min
Delta R.T.: 0.015 min
Response: 25570
Conc: 0.26 ug/ml

Instrument :
FID_F
ClientSampleId :