

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
 Data File : FF003208.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jan 2019 21:25
 Operator : AJ\SJ
 Sample : K1100-03
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 11 01:10:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.612	1928269	14.504 ug/ml
Target Compounds			
4) N-TETRADECANE	8.218	1601774	10.507 ug/ml
8) N-DOCOSANE	13.710	88217	0.585 ug/ml
10) N-TETRACOSANE	14.816	249239	1.673 ug/ml
11) N-HEXACOSANE	15.840	281868	1.916 ug/ml
12) N-OCTACOSANE	16.792	336935	2.315 ug/ml
13) N-TRIACONTANE	17.682	374270	2.621 ug/ml
14) N-DOTRIACONTANE	18.518	271054	2.034 ug/ml
15) N-TETRATRIACONTANE	19.306	97956	0.790 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
Data File : FF003208.D
Signal(s) : FID2B.ch
Acq On : 10 Jan 2019 21:25
Operator : AJ\SJ
Sample : K1100-03
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 11 01:10:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

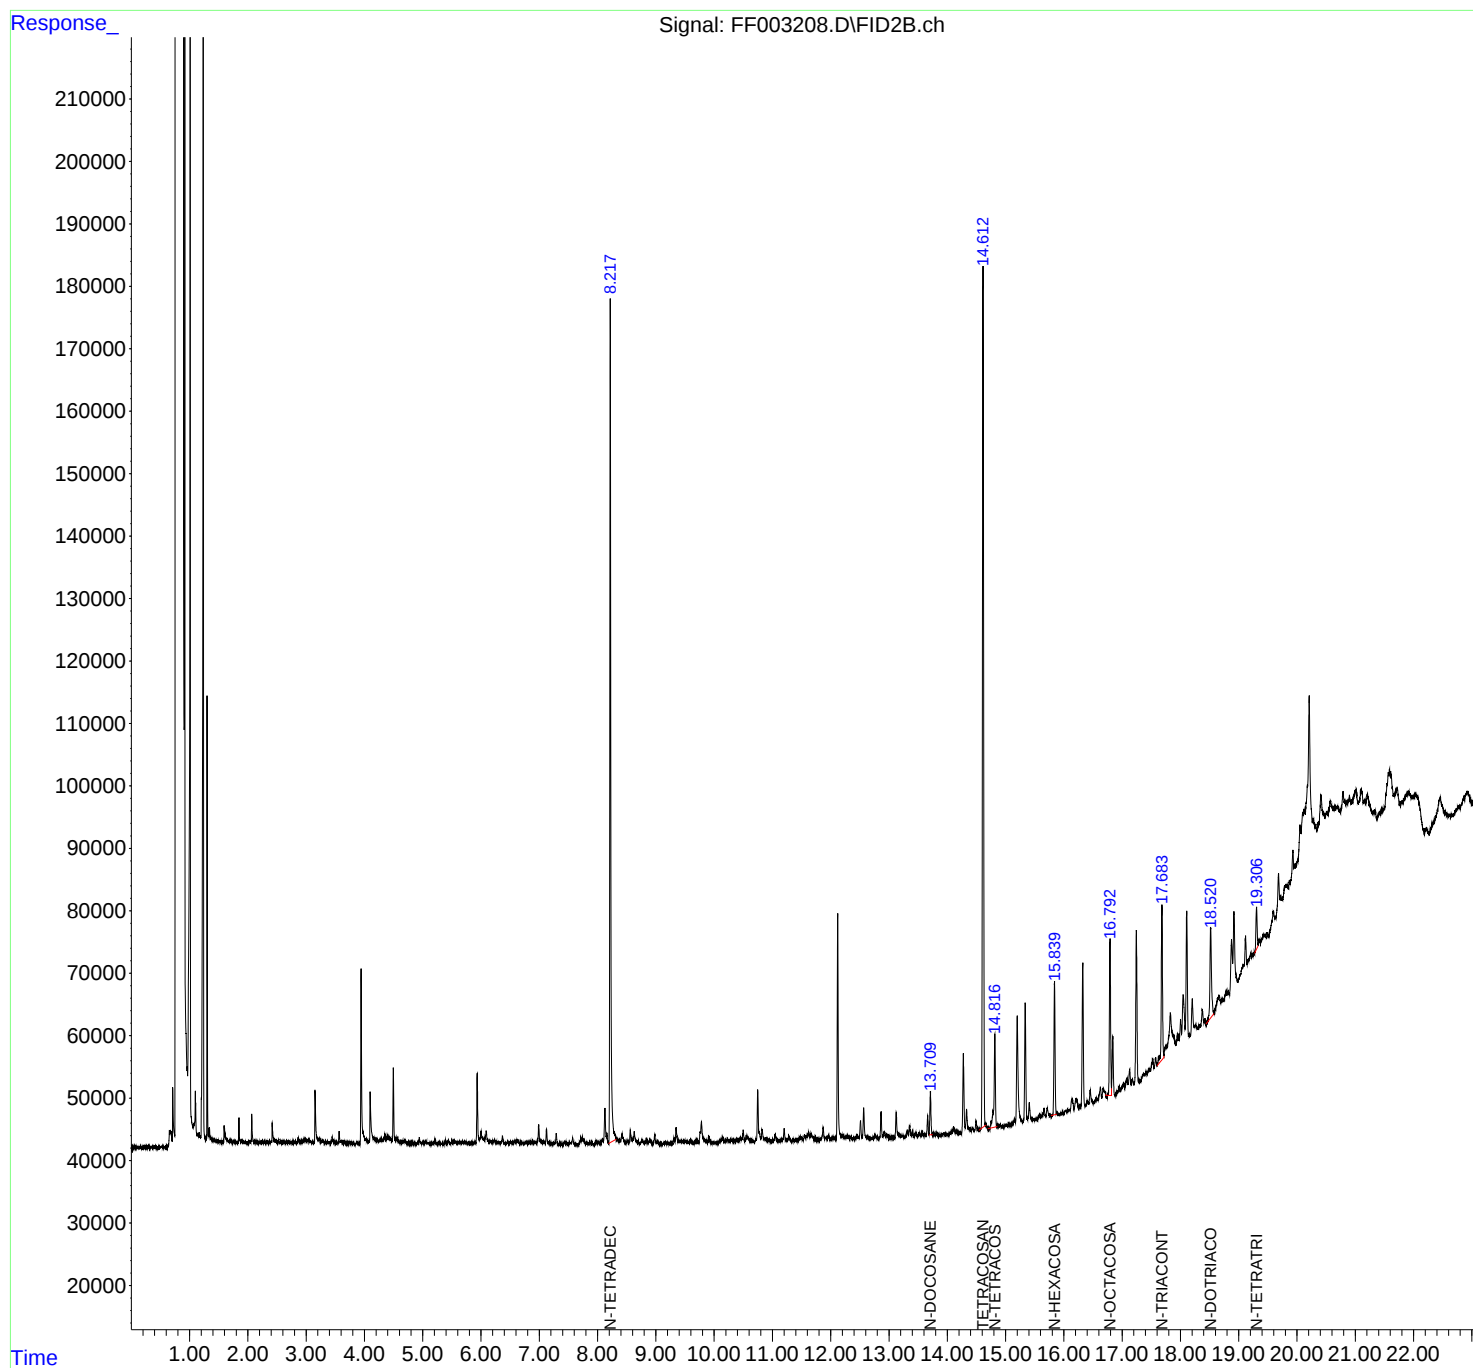


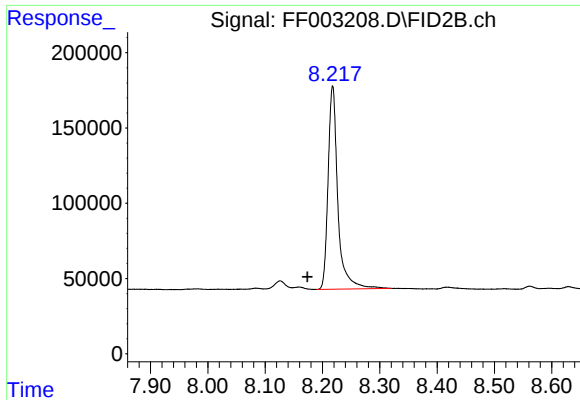

#4 N-TETRADECANE


R.T.: 8.218 min
Delta R.T.: 0.044 min
Response: 1601774
Conc: 10.51 ug/ml

Instrument :
FID_F
ClientSampleId :

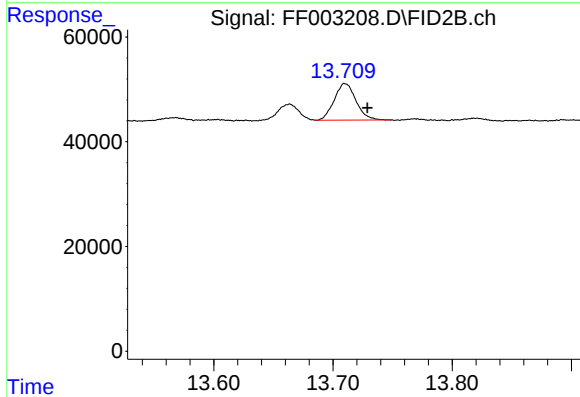


#8 N-DOCOSANE

R.T.: 13.710 min
Delta R.T.: -0.019 min
Response: 88217
Conc: 0.59 ug/ml

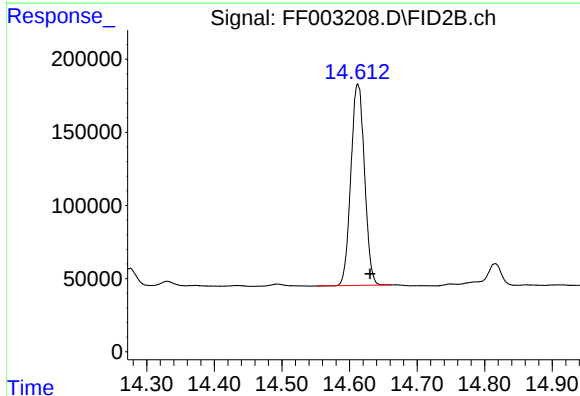


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.612 min
Delta R.T.: -0.018 min
Response: 1928269
Conc: 14.50 ug/ml

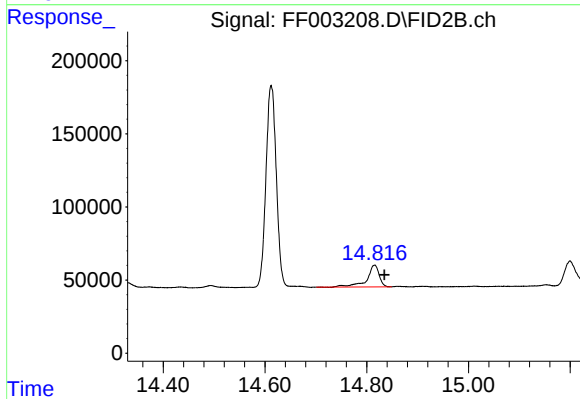

#10 N-TETRACOSANE


R.T.: 14.816 min
Delta R.T.: -0.019 min
Response: 249239
Conc: 1.67 ug/ml

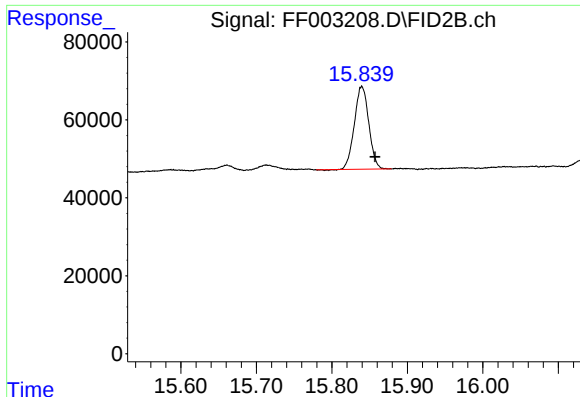

#11 N-HEXACOSANE


R.T.: 15.840 min
Delta R.T.: -0.018 min
Response: 281868
Conc: 1.92 ug/ml

Instrument :
FID_F
ClientSampleId :

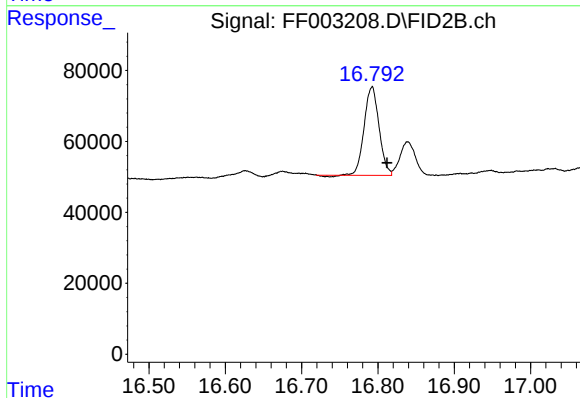


#12 N-OCTACOSANE

R.T.: 16.792 min
Delta R.T.: -0.020 min
Response: 336935
Conc: 2.32 ug/ml

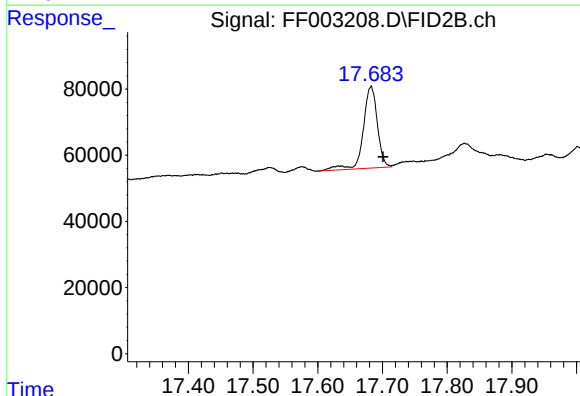


#13 N-TRIACONTANE

R.T.: 17.682 min
Delta R.T.: -0.019 min
Response: 374270
Conc: 2.62 ug/ml

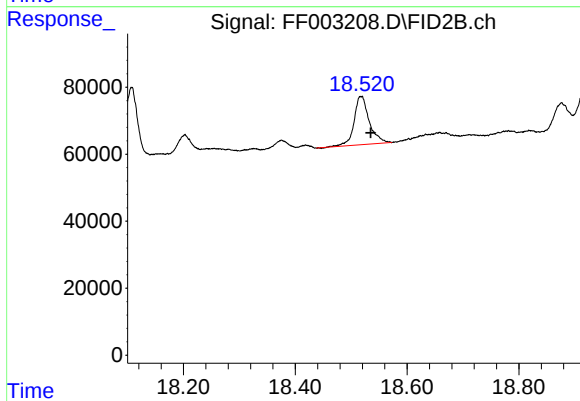

#14 N-DOTRIACONTANE

R.T.: 18.518 min
Delta R.T.: -0.018 min
Response: 271054
Conc: 2.03 ug/ml

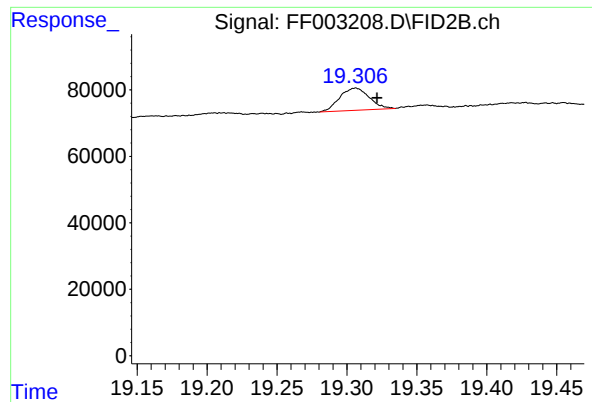

#15 N-TETRATRIACONTANE

R.T.: 19.306 min
Delta R.T.: -0.015 min
Response: 97956
Conc: 0.79 ug/ml

Instrument :
FID_F
ClientSampleId :