

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
 Data File : FF003209.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jan 2019 21:54
 Operator : AJ\SJ
 Sample : K1100-07
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 11 01:10:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.612	1340152	10.080 ug/ml
Target Compounds			
4) N-TETRADECANE	8.217	951366	6.240 ug/ml
8) N-DOCOSANE	13.710	100007	0.663 ug/ml
10) N-TETRACOSANE	14.815	287257	1.928 ug/ml
11) N-HEXACOSANE	15.838	409498	2.783 ug/ml
12) N-OCTACOSANE	16.791	532889	3.662 ug/ml
13) N-TRIACONTANE	17.680	523760	3.667 ug/ml
14) N-DOTRIACONTANE	18.516	363689	2.730 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
Data File : FF003209.D
Signal(s) : FID2B.ch
Acq On : 10 Jan 2019 21:54
Operator : AJ\SJ
Sample : K1100-07
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 11 01:10:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

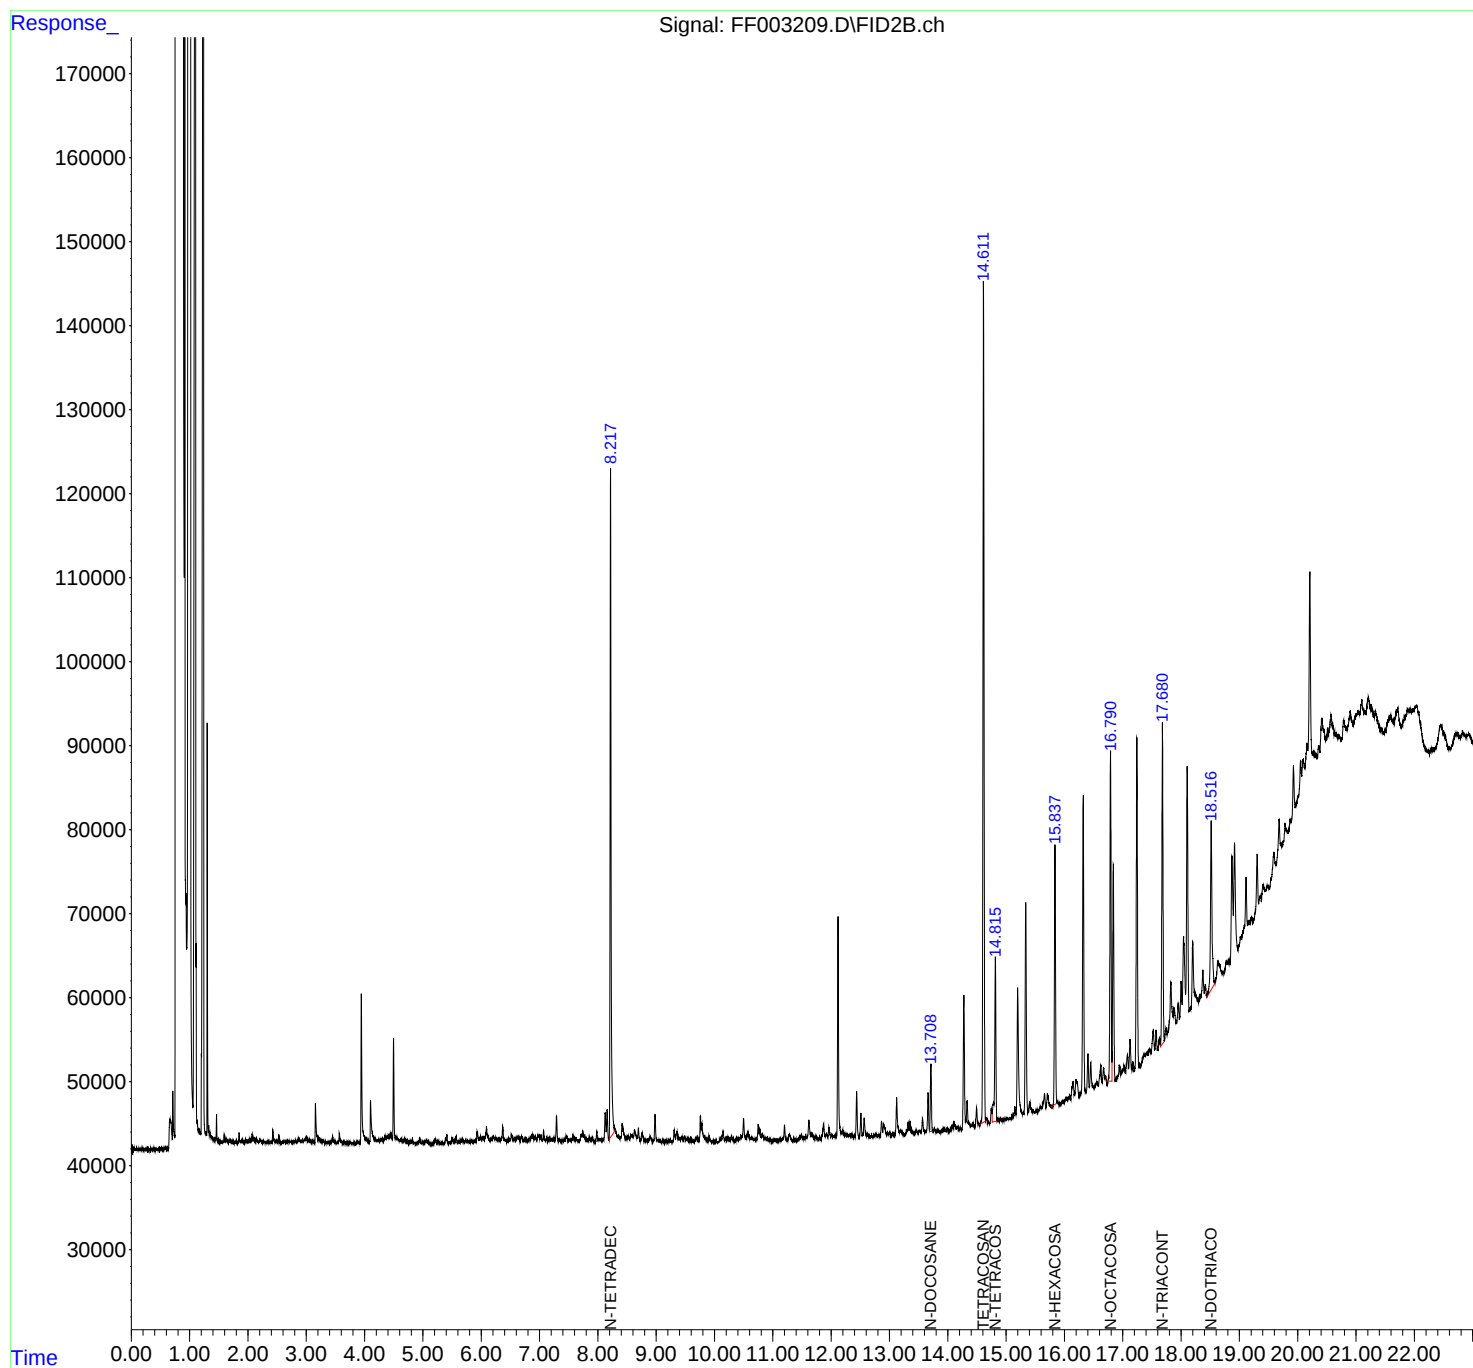


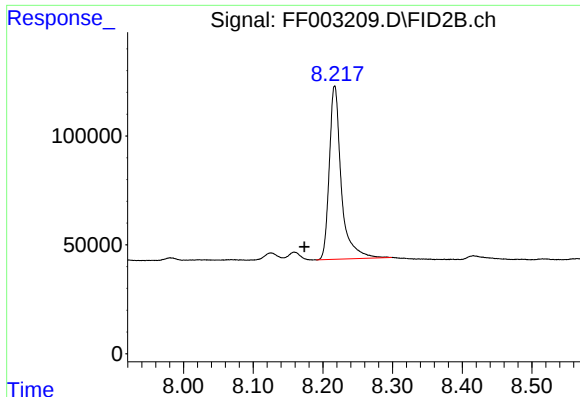

#4 N-TETRADECANE


R.T.: 8.217 min
Delta R.T.: 0.043 min
Response: 951366
Conc: 6.24 ug/ml

Instrument :
FID_F
ClientSampleId :

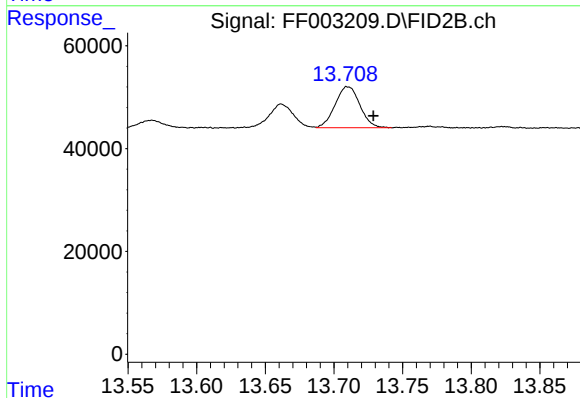


#8 N-DOCOSANE

R.T.: 13.710 min
Delta R.T.: -0.019 min
Response: 100007
Conc: 0.66 ug/ml

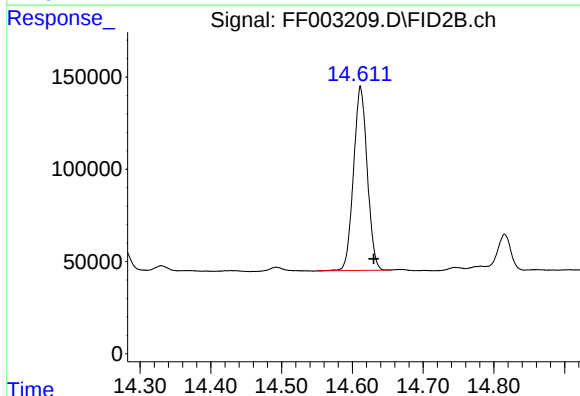


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.612 min
Delta R.T.: -0.019 min
Response: 1340152
Conc: 10.08 ug/ml

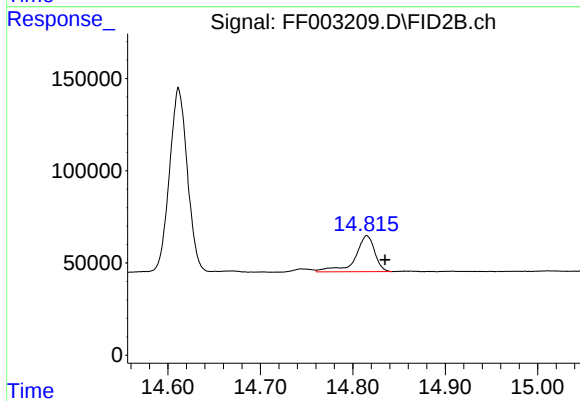

#10 N-TETRACOSANE


R.T.: 14.815 min
Delta R.T.: -0.020 min
Response: 287257
Conc: 1.93 ug/ml

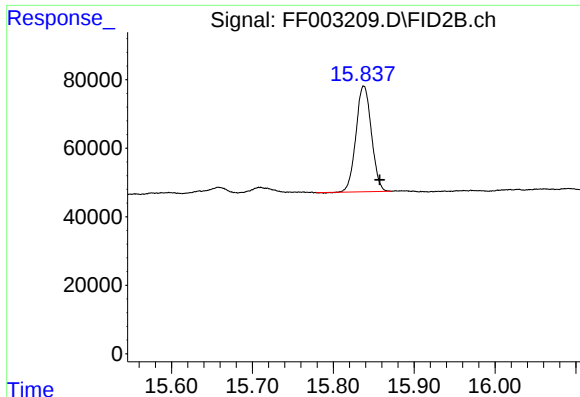

#11 N-HEXACOSANE


R.T.: 15.838 min
Delta R.T.: -0.019 min
Response: 409498
Conc: 2.78 ug/ml

Instrument :
FID_F
ClientSampleId :

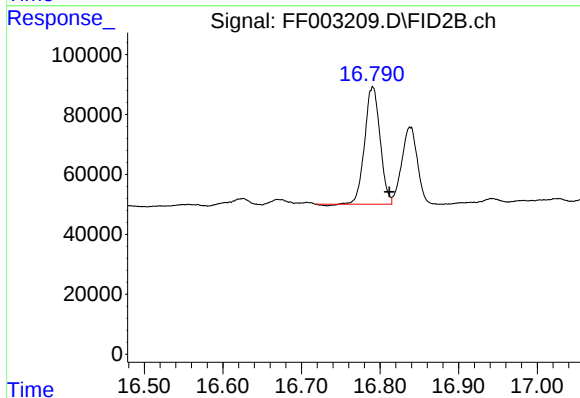


#12 N-OCTACOSANE

R.T.: 16.791 min
Delta R.T.: -0.021 min
Response: 532889
Conc: 3.66 ug/ml

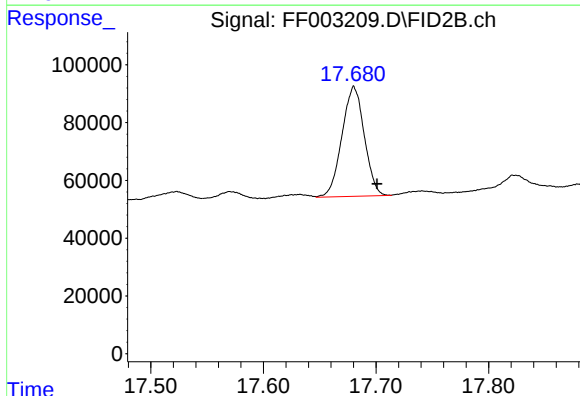

#13 N-TRIACONTANE

R.T.: 17.680 min
Delta R.T.: -0.020 min
Response: 523760
Conc: 3.67 ug/ml

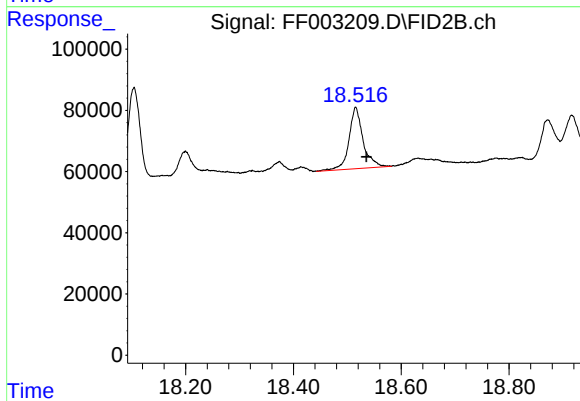

#14 N-DOTRIACONTANE

R.T.: 18.516 min
Delta R.T.: -0.020 min
Response: 363689
Conc: 2.73 ug/ml