

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
 Data File : FF003210.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jan 2019 22:25
 Operator : AJ\SJ
 Sample : K1100-05
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 11 01:10:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.612	1338549	10.068 ug/ml
Target Compounds			
4) N-TETRADECANE	8.217	1071168	7.026 ug/ml
10) N-TETRACOSANE	14.815	170788	1.146 ug/ml
11) N-HEXACOSANE	15.837	241535	1.642 ug/ml
12) N-OCTACOSANE	16.790	335745	2.307 ug/ml
13) N-TRIACONTANE	17.681	360849	2.527 ug/ml
14) N-DOTRIACONTANE	18.517	352488	2.646 ug/ml
15) N-TETRATRIACONTANE	19.305	88518	0.714 ug/ml
16) N-HEXATRIACONTANE	20.088	501418	4.445 ug/ml
18) N-TETRACONTANE	21.710	1074420	10.658 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
Data File : FF003210.D
Signal(s) : FID2B.ch
Acq On : 10 Jan 2019 22:25
Operator : AJ\SJ
Sample : K1100-05
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 11 01:10:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

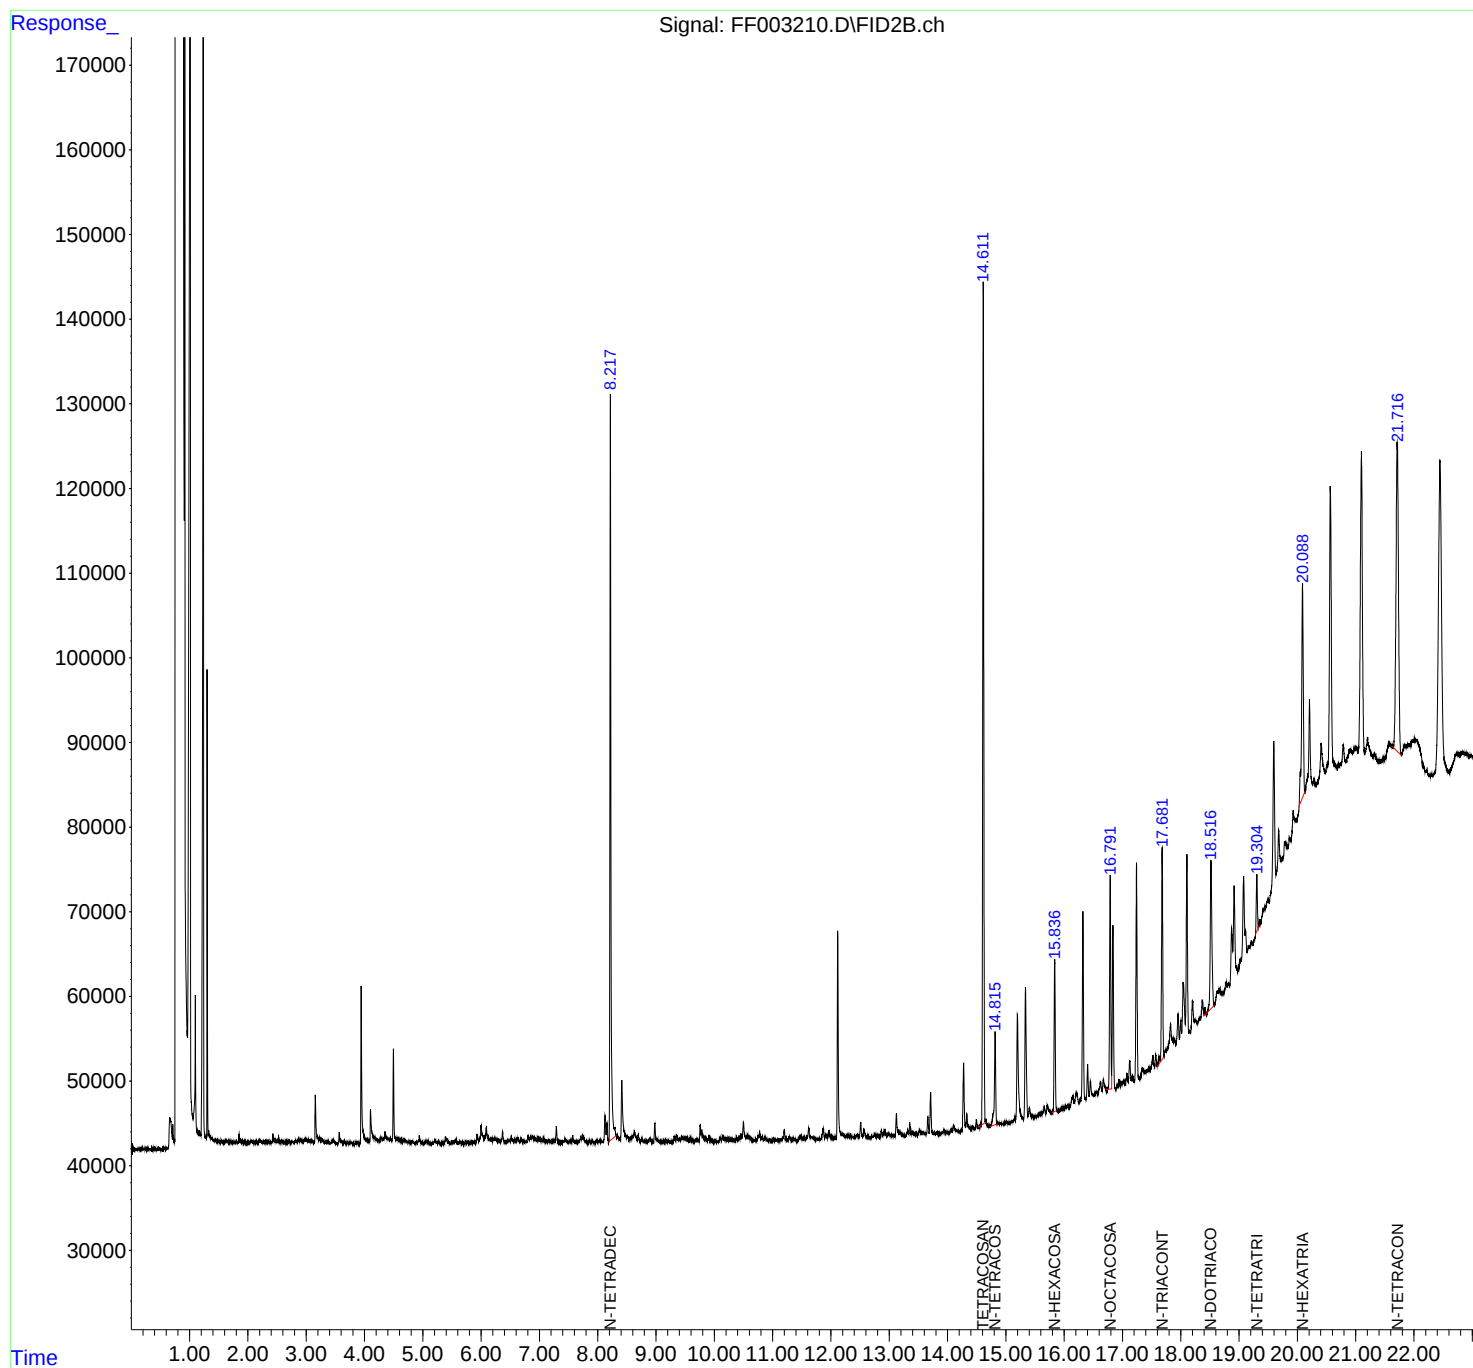


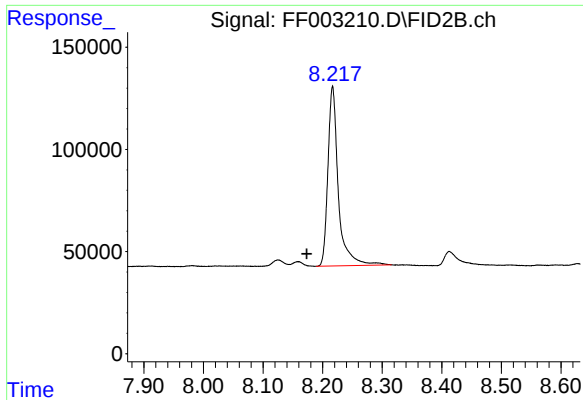

#4 N-TETRADECANE


R.T.: 8.217 min
Delta R.T.: 0.043 min
Response: 1071168
Conc: 7.03 ug/ml

Instrument :
FID_F
ClientSampleId :

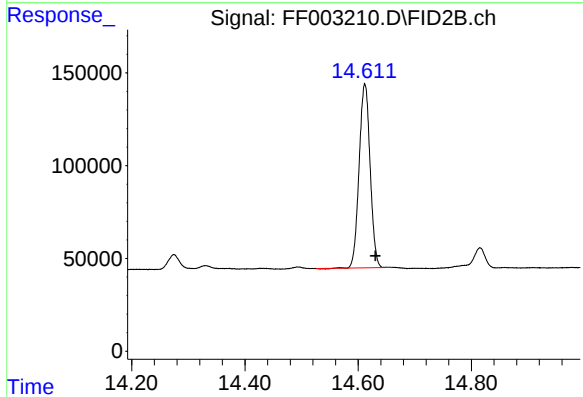


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.612 min
Delta R.T.: -0.018 min
Response: 1338549
Conc: 10.07 ug/ml

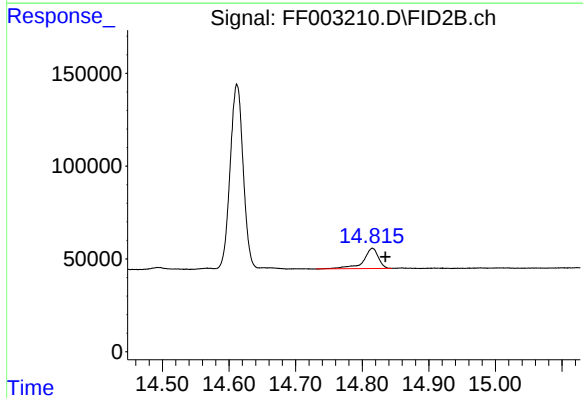


#10 N-TETRACOSANE

R.T.: 14.815 min
Delta R.T.: -0.019 min
Response: 170788
Conc: 1.15 ug/ml

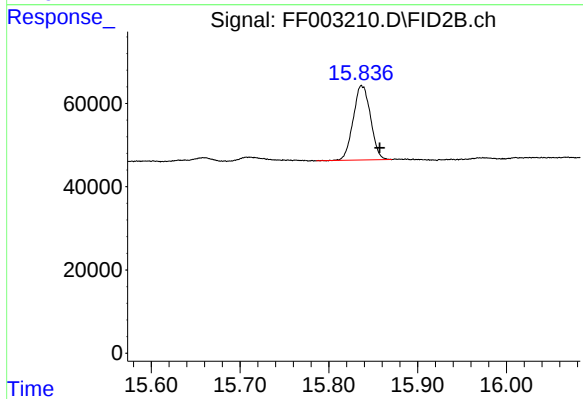

#11 N-HEXACOSANE


R.T.: 15.837 min
Delta R.T.: -0.020 min
Response: 241535
Conc: 1.64 ug/ml

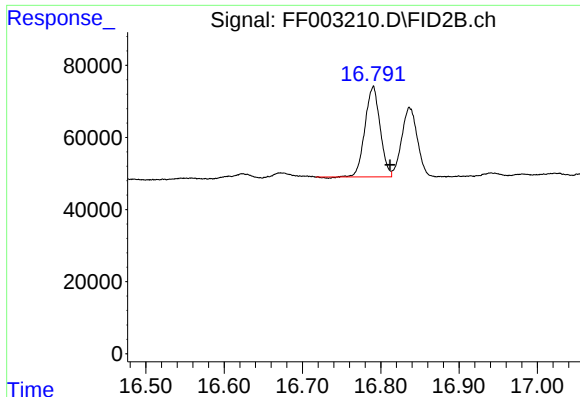

#12 N-OCTACOSANE


R.T.: 16.790 min
Delta R.T.: -0.022 min
Response: 335745
Conc: 2.31 ug/ml

Instrument :
FID_F
ClientSampleId :

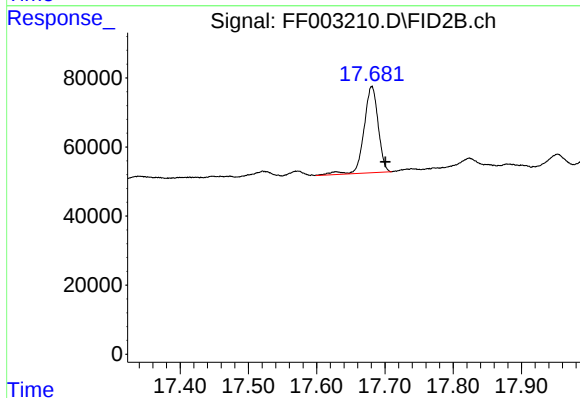


#13 N-TRIACONTANE

R.T.: 17.681 min
Delta R.T.: -0.020 min
Response: 360849
Conc: 2.53 ug/ml

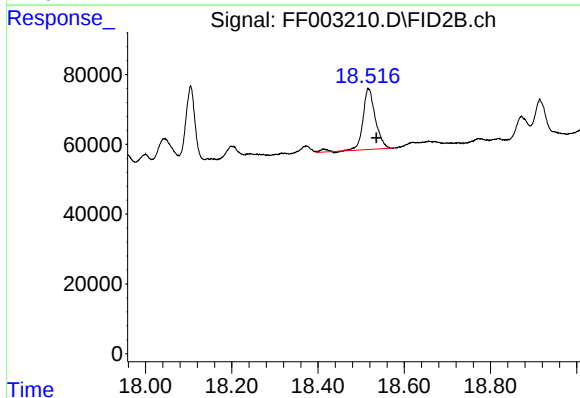


#14 N-DOTRIACONTANE

R.T.: 18.517 min
Delta R.T.: -0.019 min
Response: 352488
Conc: 2.65 ug/ml

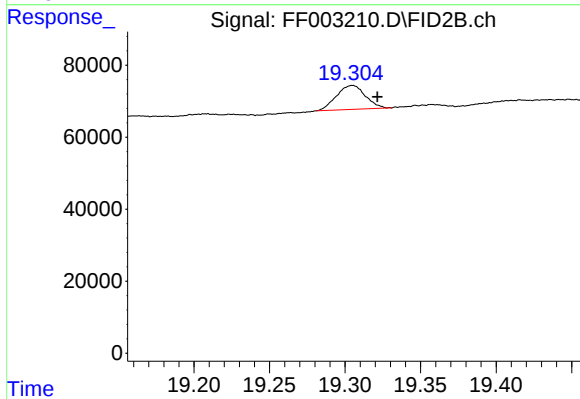

#15 N-TETRATRIACONTANE


R.T.: 19.305 min
Delta R.T.: -0.017 min
Response: 88518
Conc: 0.71 ug/ml

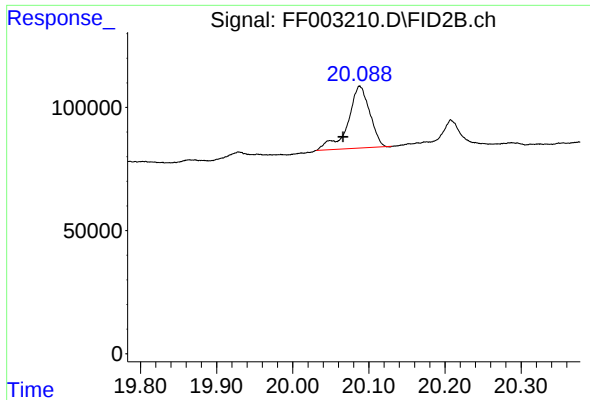

#16 N-HEXATRIACONTANE

R.T.: 20.088 min
Delta R.T.: 0.022 min
Response: 501418
Conc: 4.45 ug/ml

Instrument :
FID_F
ClientSampleId :

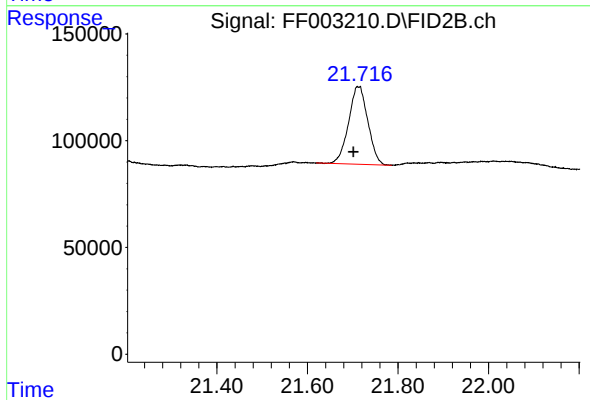

#18 N-TETRACONTANE

R.T.: 21.710 min
Delta R.T.: 0.009 min
Response: 1074420
Conc: 10.66 ug/ml