

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
 Data File : FF003211.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jan 2019 22:54
 Operator : AJ\SJ
 Sample : K1085-01
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 11 01:10:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.612	1734042	13.043 ug/ml
Target Compounds			
11) N-HEXACOSANE	15.838	89712	0.610 ug/ml
12) N-OCTACOSANE	16.790	296230	2.035 ug/ml
13) N-TRIACONTANE	17.681	429344	3.006 ug/ml
14) N-DOTRIACONTANE	18.515	312582	2.346 ug/ml
16) N-HEXATRIACONTANE	20.106	199292	1.767 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
Data File : FF003211.D
Signal(s) : FID2B.ch
Acq On : 10 Jan 2019 22:54
Operator : AJ\SJ
Sample : K1085-01
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 11 01:10:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

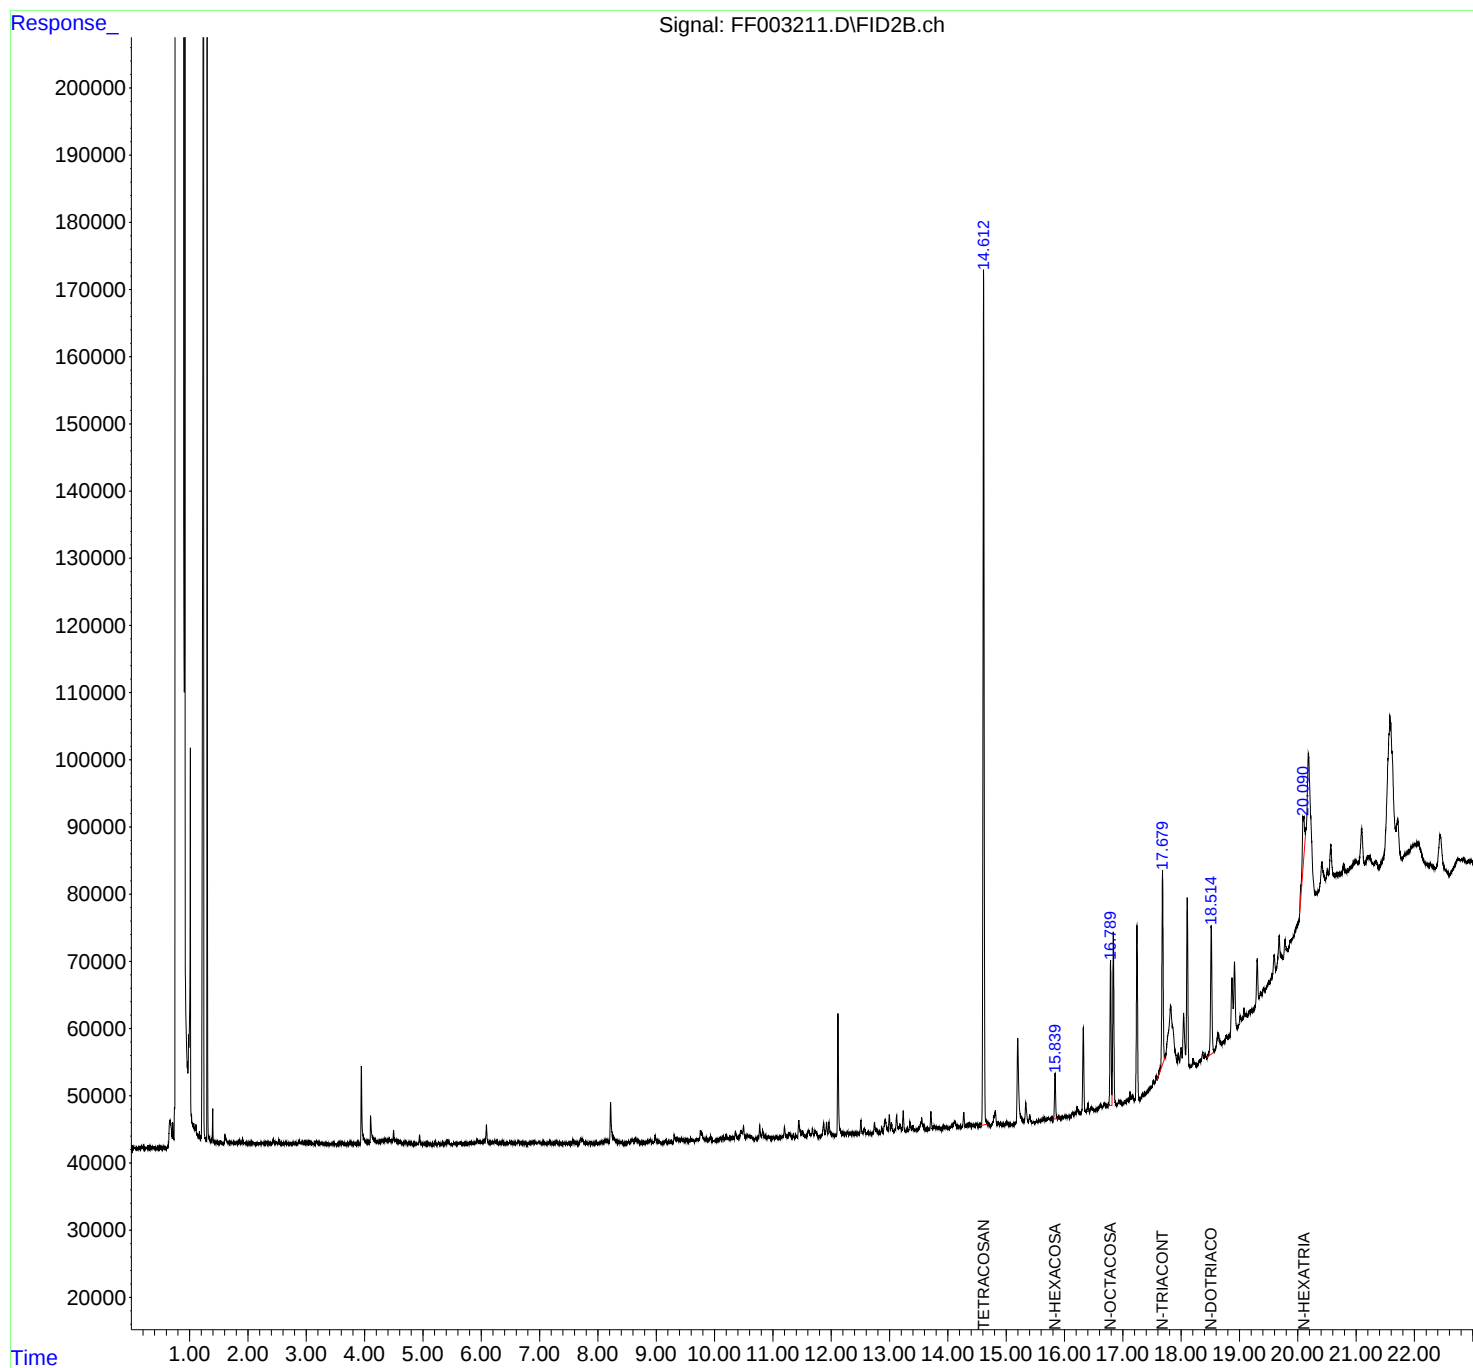


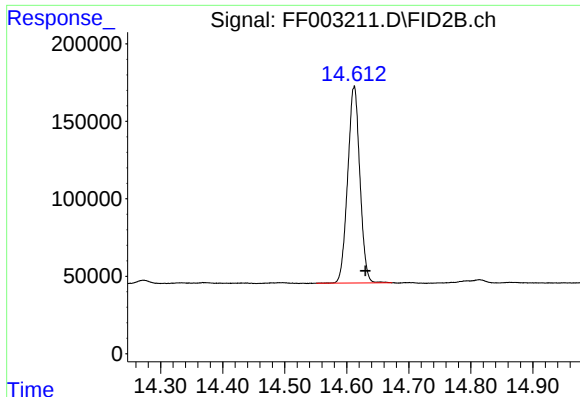

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.612 min
Delta R.T.: -0.018 min
Response: 1734042
Conc: 13.04 ug/ml

Instrument :
FID_F
ClientSampleId :

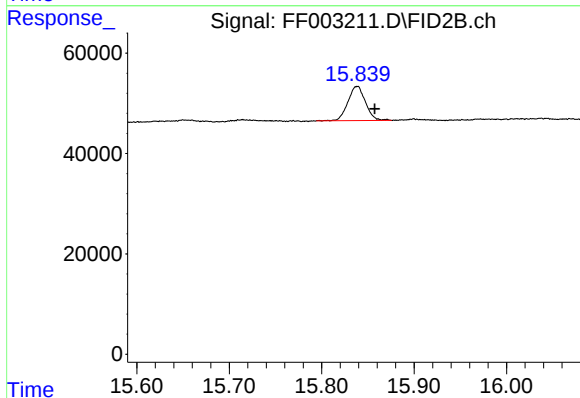


#11 N-HEXACOSANE

R.T.: 15.838 min
Delta R.T.: -0.019 min
Response: 89712
Conc: 0.61 ug/ml

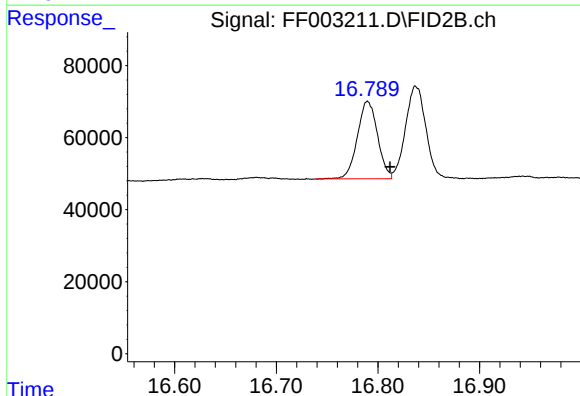


#12 N-OCTACOSANE

R.T.: 16.790 min
Delta R.T.: -0.022 min
Response: 296230
Conc: 2.04 ug/ml

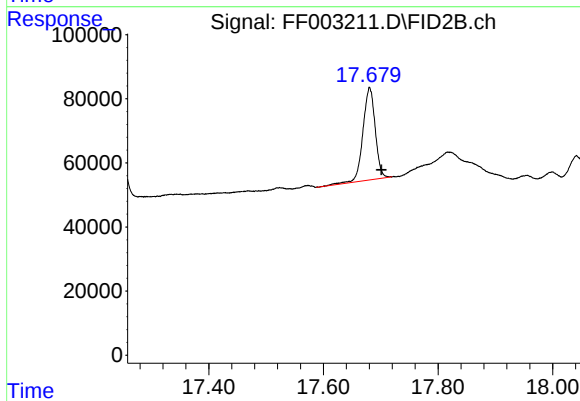

#13 N-TRIACONTANE


R.T.: 17.681 min
Delta R.T.: -0.020 min
Response: 429344
Conc: 3.01 ug/ml

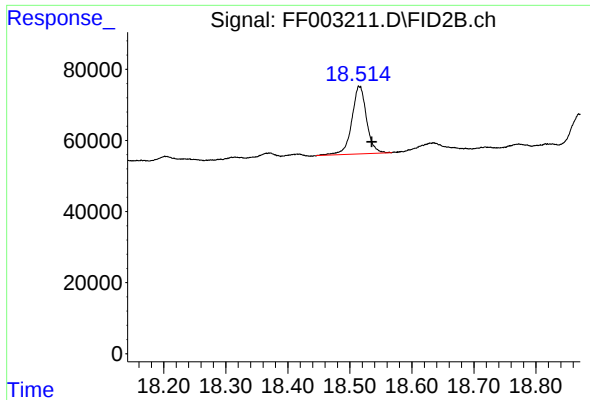

#14 N-DOTRIACONTANE

R.T.: 18.515 min
Delta R.T.: -0.020 min
Response: 312582
Conc: 2.35 ug/ml

Instrument :
FID_F
ClientSampleId :

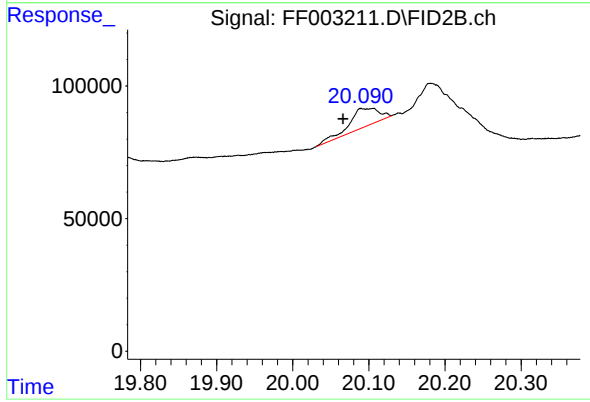

#16 N-HEXATRIACONTANE

R.T.: 20.106 min
Delta R.T.: 0.039 min
Response: 199292
Conc: 1.77 ug/ml