

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
 Data File : FF003206.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jan 2019 20:25
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Jan 11 01:09:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.617	6048213	45.494 ug/ml
Target Compounds			
2) N-DECANE	4.353	8152841	54.292 ug/ml
3) N-DODECANE	6.373	8029142	53.055 ug/ml
4) N-TETRADECANE	8.164	7846139	51.466 ug/ml
5) N-HEXADECANE	9.764	7675241	50.066 ug/ml
6) N-OCTADECANE	11.206	7471835	48.579 ug/ml
7) N-EICOSANE	12.517	7188576	47.209 ug/ml
8) N-DOCOSANE	13.716	6937410	46.017 ug/ml
10) N-TETRACOSANE	14.822	6754845	45.334 ug/ml
11) N-HEXACOSANE	15.844	6665099	45.301 ug/ml
12) N-OCTACOSANE	16.796	6741926	46.324 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
Data File : FF003206.D
Signal(s) : FID2B.ch
Acq On : 10 Jan 2019 20:25
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Jan 11 01:09:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

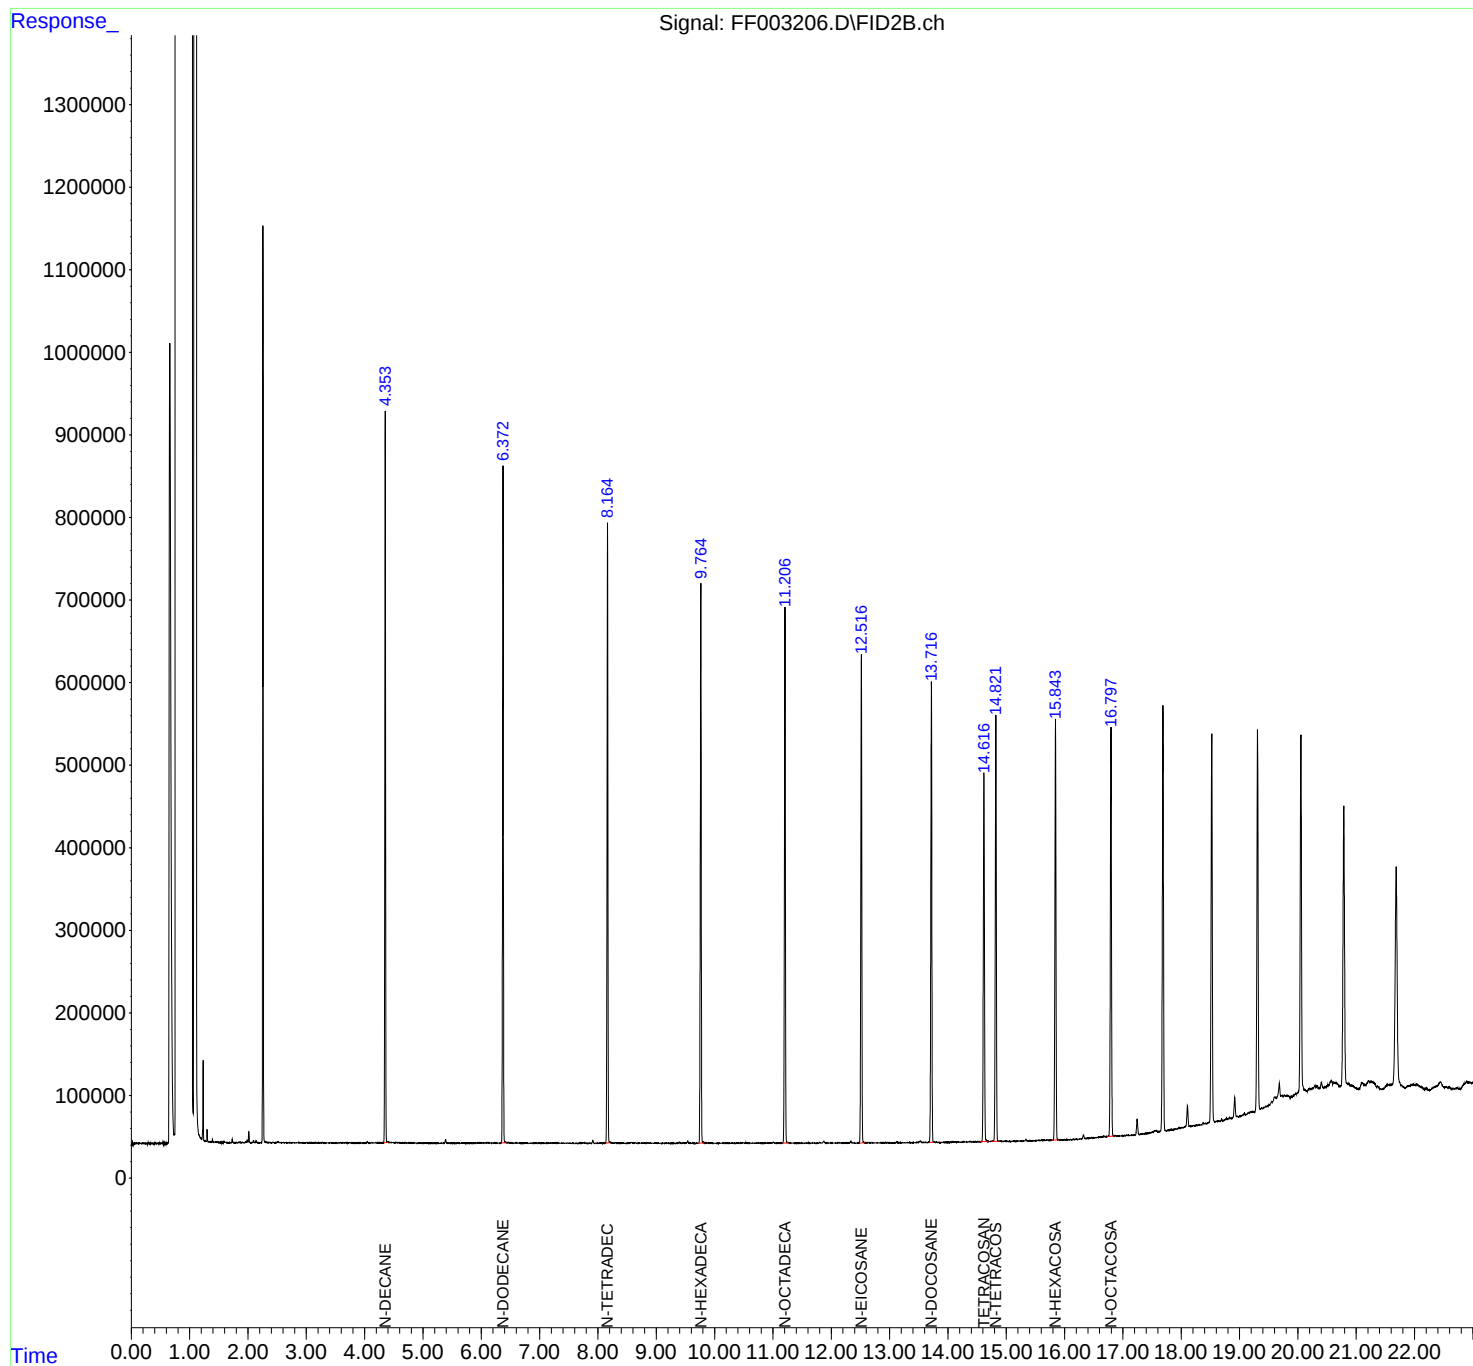


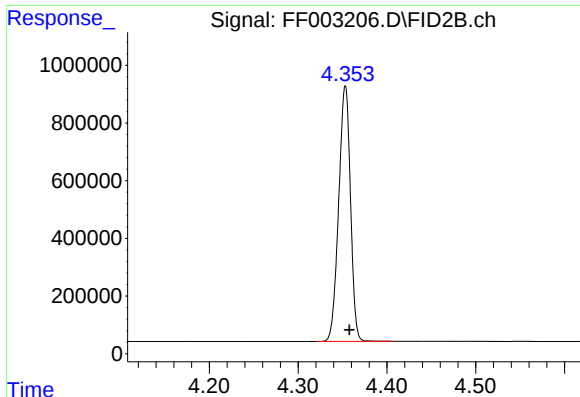

#2 N-DECANE


R.T.: 4.353 min
Delta R.T.: -0.005 min
Response: 8152841
Conc: 54.29 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

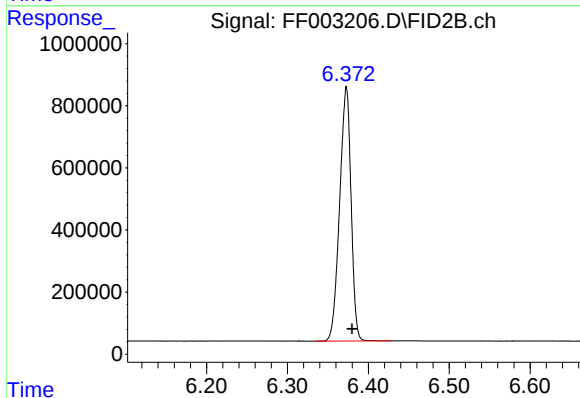


#3 N-DODECANE

R.T.: 6.373 min
Delta R.T.: -0.007 min
Response: 8029142
Conc: 53.05 ug/ml

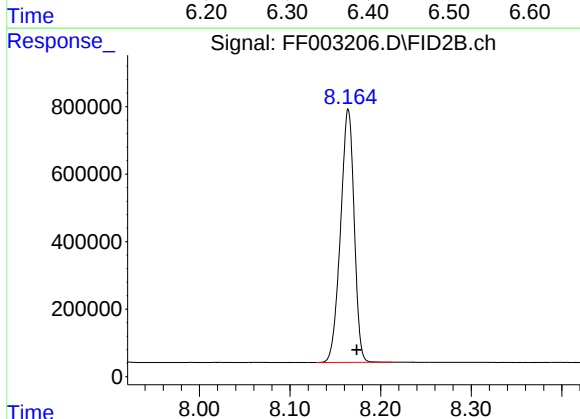


#4 N-TETRADECANE

R.T.: 8.164 min
Delta R.T.: -0.009 min
Response: 7846139
Conc: 51.47 ug/ml

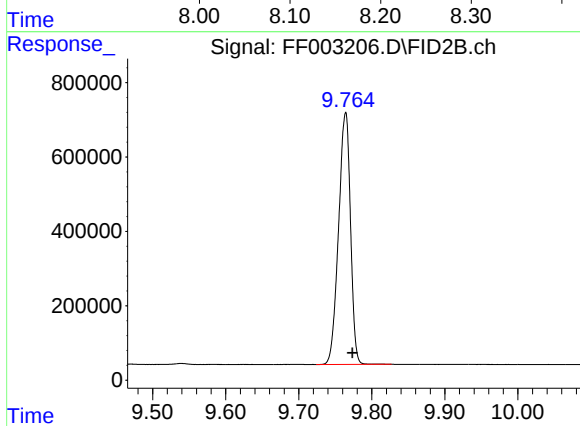

#5 N-HEXADECANE


R.T.: 9.764 min
Delta R.T.: -0.009 min
Response: 7675241
Conc: 50.07 ug/ml

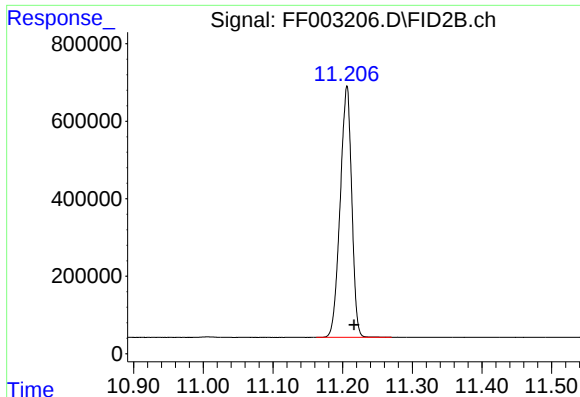

#6 N-OCTADECANE


R.T.: 11.206 min
Delta R.T.: -0.010 min
Response: 7471835
Conc: 48.58 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

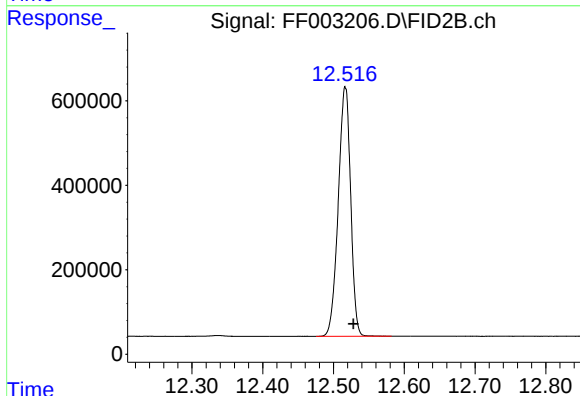


#7 N-EICOSANE

R.T.: 12.517 min
Delta R.T.: -0.011 min
Response: 7188576
Conc: 47.21 ug/ml

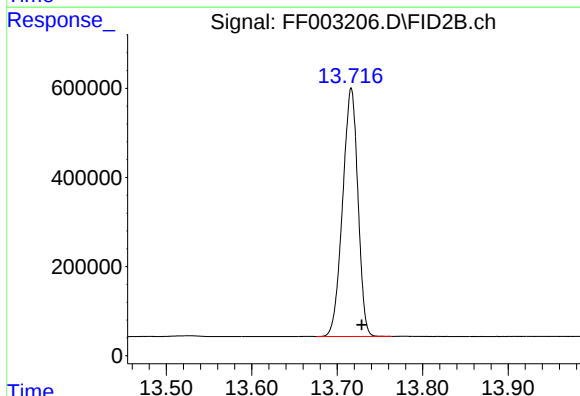


#8 N-DOCOSANE

R.T.: 13.716 min
Delta R.T.: -0.012 min
Response: 6937410
Conc: 46.02 ug/ml

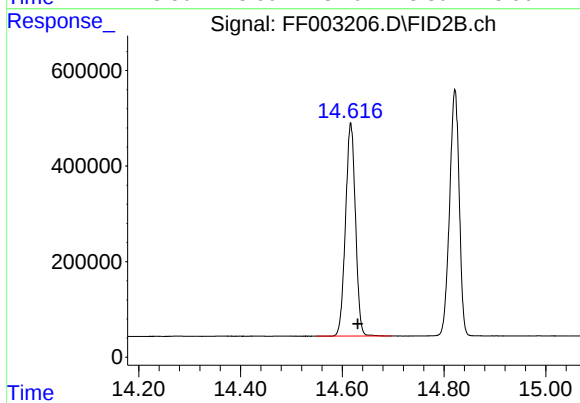

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.617 min
Delta R.T.: -0.014 min
Response: 6048213
Conc: 45.49 ug/ml

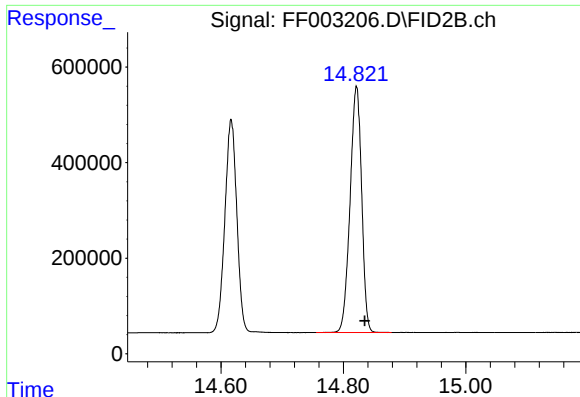

#10 N-TETRACOSANE


R.T.: 14.822 min
Delta R.T.: -0.013 min
Response: 6754845
Conc: 45.33 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

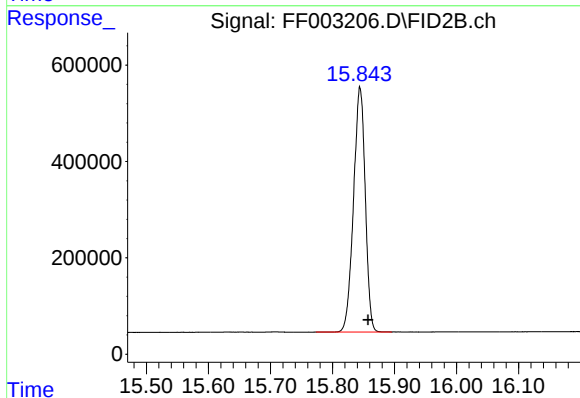

#11 N-HEXACOSANE

R.T.: 15.844 min
Delta R.T.: -0.013 min
Response: 6665099
Conc: 45.30 ug/ml

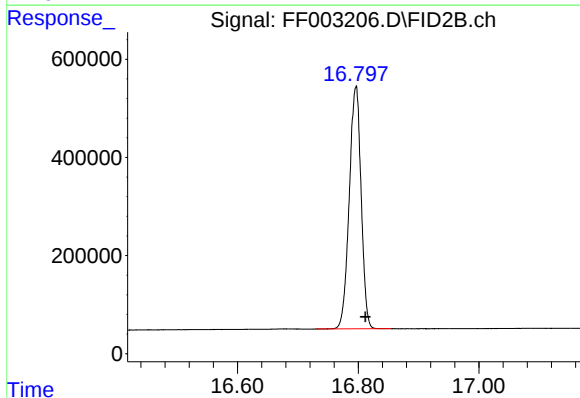

#12 N-OCTACOSANE

R.T.: 16.796 min
Delta R.T.: -0.016 min
Response: 6741926
Conc: 46.32 ug/ml