

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
 Data File : FF003213.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jan 2019 23:54
 Operator : AJ\SJ
 Sample : PB116288BS
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB116288BS

Integration File: autoint1.e
 Quant Time: Jan 11 01:11:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.612	2228469	16.762 ug/ml
Target Compounds			
2) N-DECANE	4.350	2918407	19.434 ug/ml
3) N-DODECANE	6.369	2946531	19.470 ug/ml
4) N-TETRADECANE	8.159	2886694	18.935 ug/ml
5) N-HEXADECANE	9.759	2827083	18.441 ug/ml
6) N-OCTADECANE	11.200	2768909	18.002 ug/ml
7) N-EICOSANE	12.511	2674825	17.566 ug/ml
8) N-DOCOSANE	13.710	2582518	17.130 ug/ml
10) N-TETRACOSANE	14.815	2514152	16.873 ug/ml
11) N-HEXACOSANE	15.839	2454248	16.681 ug/ml
12) N-OCTACOSANE	16.791	2461377	16.912 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
Data File : FF003213.D
Signal(s) : FID2B.ch
Acq On : 10 Jan 2019 23:54
Operator : AJ\SJ
Sample : PB116288BS
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB116288BS

Integration File: autoint1.e
Quant Time: Jan 11 01:11:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

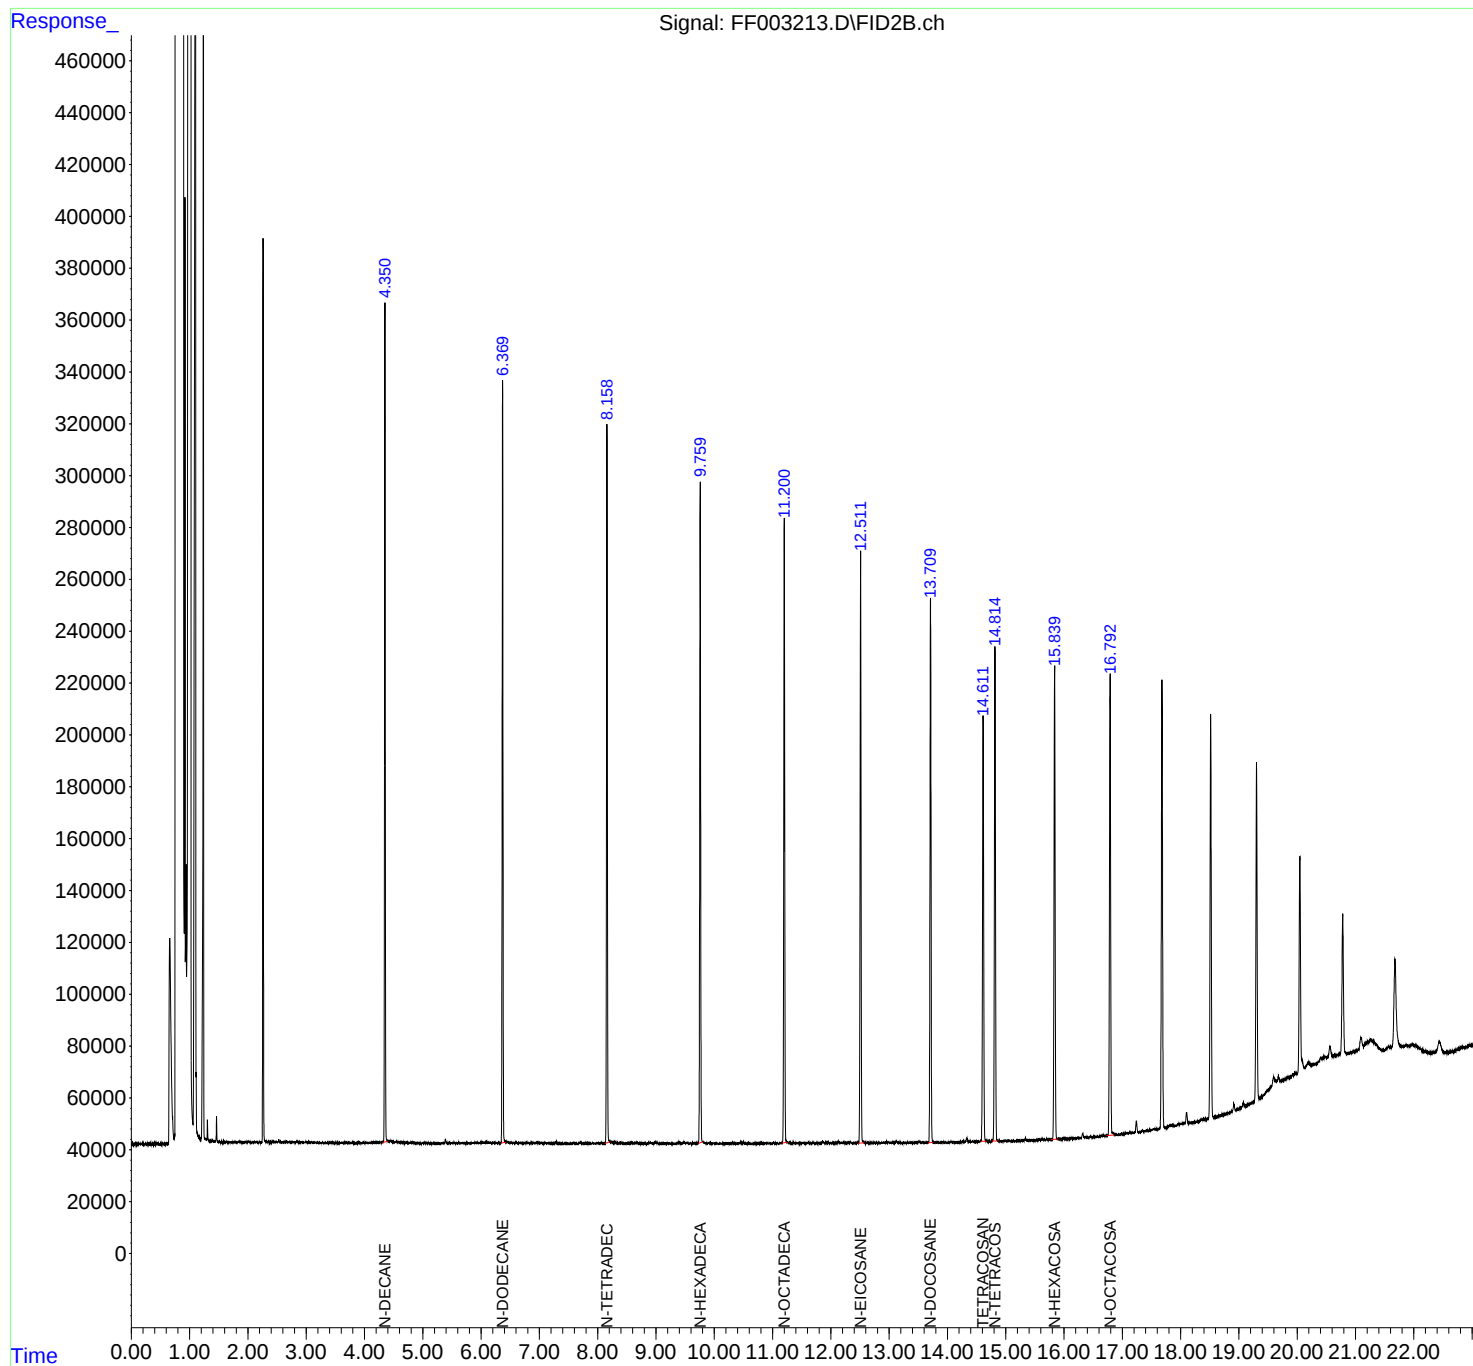


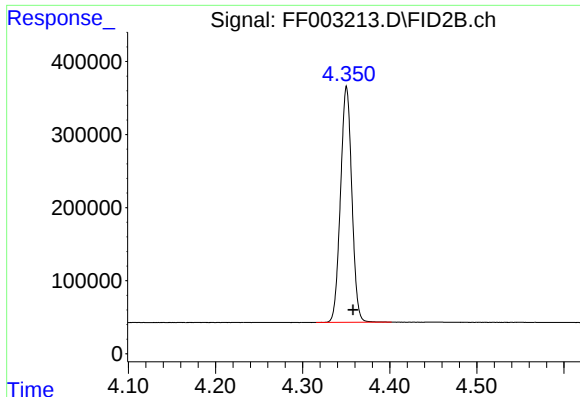

#2 N-DECANE


R.T.: 4.350 min
Delta R.T.: -0.007 min
Response: 2918407
Conc: 19.43 ug/ml

Instrument :
FID_F
ClientSampleId :
PB116288BS

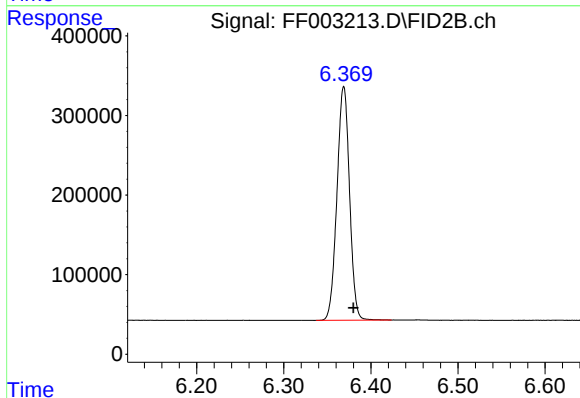


#3 N-DODECANE

R.T.: 6.369 min
Delta R.T.: -0.011 min
Response: 2946531
Conc: 19.47 ug/ml

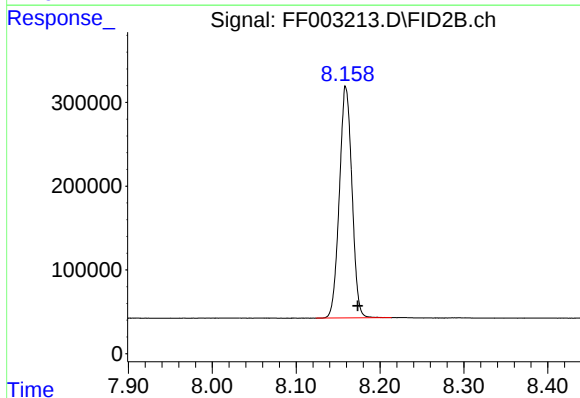


#4 N-TETRADECANE

R.T.: 8.159 min
Delta R.T.: -0.014 min
Response: 2886694
Conc: 18.94 ug/ml

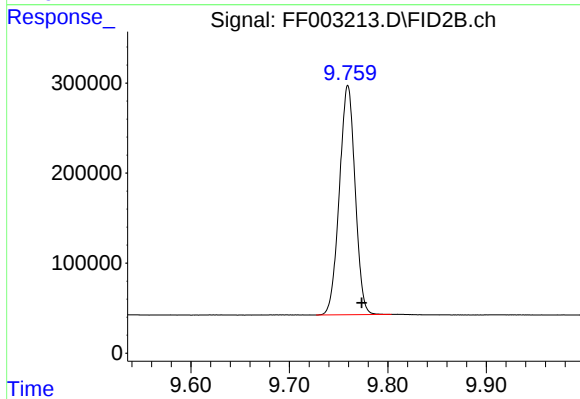

#5 N-HEXADECANE


R.T.: 9.759 min
Delta R.T.: -0.014 min
Response: 2827083
Conc: 18.44 ug/ml

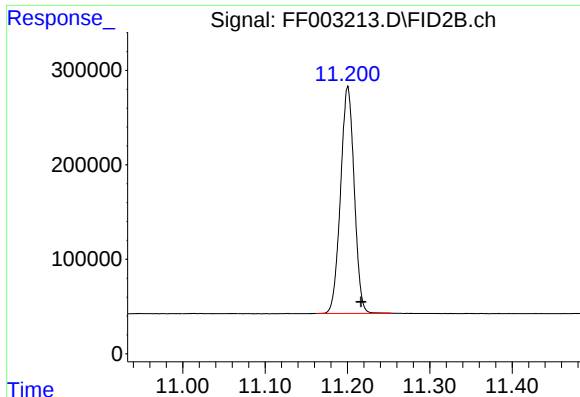

#6 N-OCTADECANE


R.T.: 11.200 min
Delta R.T.: -0.016 min
Response: 2768909
Conc: 18.00 ug/ml

Instrument :
FID_F
ClientSampleId :
PB116288BS

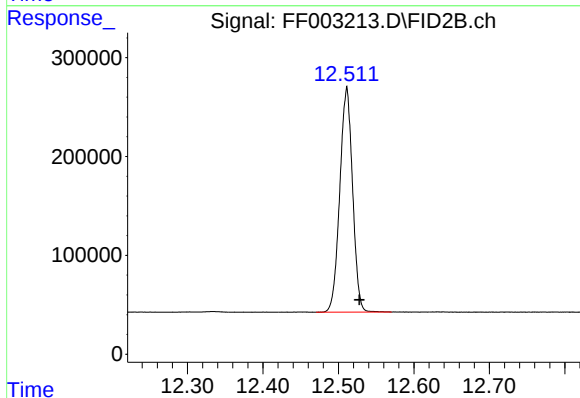


#7 N-EICOSANE

R.T.: 12.511 min
Delta R.T.: -0.017 min
Response: 2674825
Conc: 17.57 ug/ml

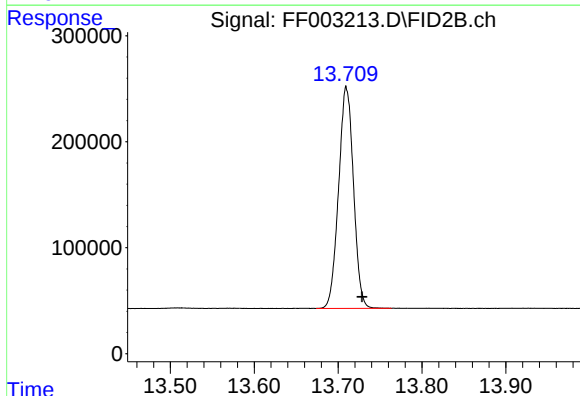


#8 N-DOCOSANE

R.T.: 13.710 min
Delta R.T.: -0.019 min
Response: 2582518
Conc: 17.13 ug/ml

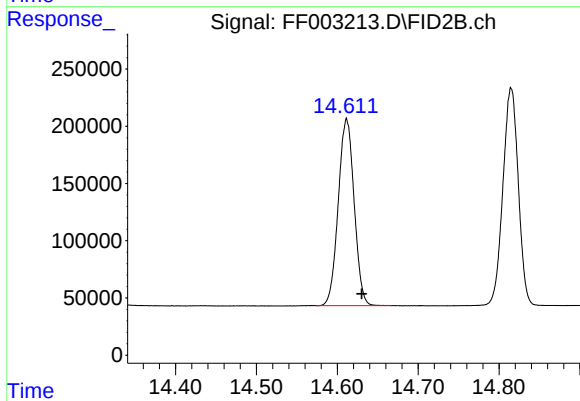

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.612 min
Delta R.T.: -0.019 min
Response: 2228469
Conc: 16.76 ug/ml

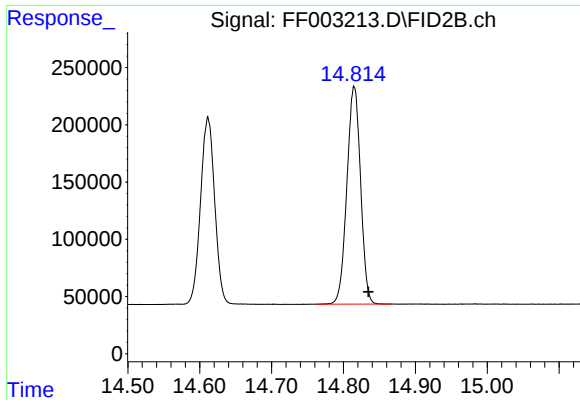

#10 N-TETRACOSANE


R.T.: 14.815 min
Delta R.T.: -0.020 min
Response: 2514152
Conc: 16.87 ug/ml

Instrument :
FID_F
ClientSampleId :
PB116288BS

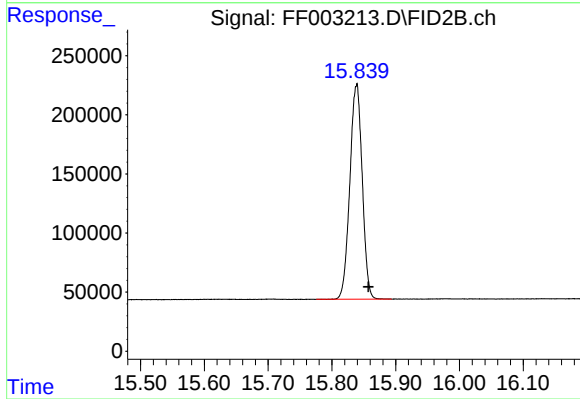

#11 N-HEXACOSANE

R.T.: 15.839 min
Delta R.T.: -0.019 min
Response: 2454248
Conc: 16.68 ug/ml

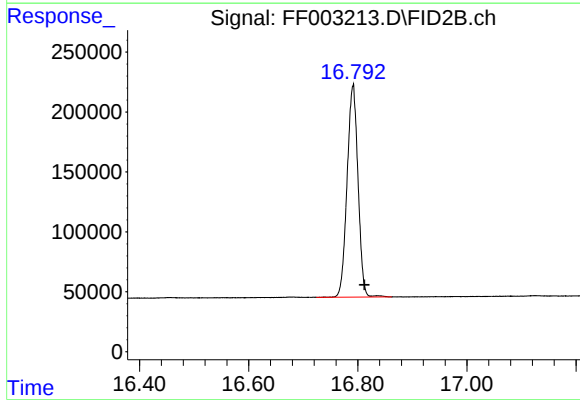

#12 N-OCTACOSANE

R.T.: 16.791 min
Delta R.T.: -0.021 min
Response: 2461377
Conc: 16.91 ug/ml