

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
 Data File : FF003214.D
 Signal(s) : FID2B.ch
 Acq On : 11 Jan 2019 00:24
 Operator : AJ\SJ
 Sample : PB116288BSD
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB116288BSD

Integration File: autoint1.e
 Quant Time: Jan 11 01:11:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.611	2070583	15.575 ug/ml
Target Compounds			
2) N-DECANE	4.351	2687175	17.895 ug/ml
3) N-DODECANE	6.369	2713694	17.931 ug/ml
4) N-TETRADECANE	8.160	2662662	17.466 ug/ml
5) N-HEXADECANE	9.758	2607896	17.011 ug/ml
6) N-OCTADECANE	11.200	2556140	16.619 ug/ml
7) N-EICOSANE	12.511	2465805	16.193 ug/ml
8) N-DOCOSANE	13.710	2390536	15.857 ug/ml
10) N-TETRACOSANE	14.815	2340759	15.709 ug/ml
11) N-HEXACOSANE	15.837	2295020	15.599 ug/ml
12) N-OCTACOSANE	16.791	2281172	15.674 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
Data File : FF003214.D
Signal(s) : FID2B.ch
Acq On : 11 Jan 2019 00:24
Operator : AJ\SJ
Sample : PB116288BSD
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB116288BSD

Integration File: autoint1.e
Quant Time: Jan 11 01:11:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

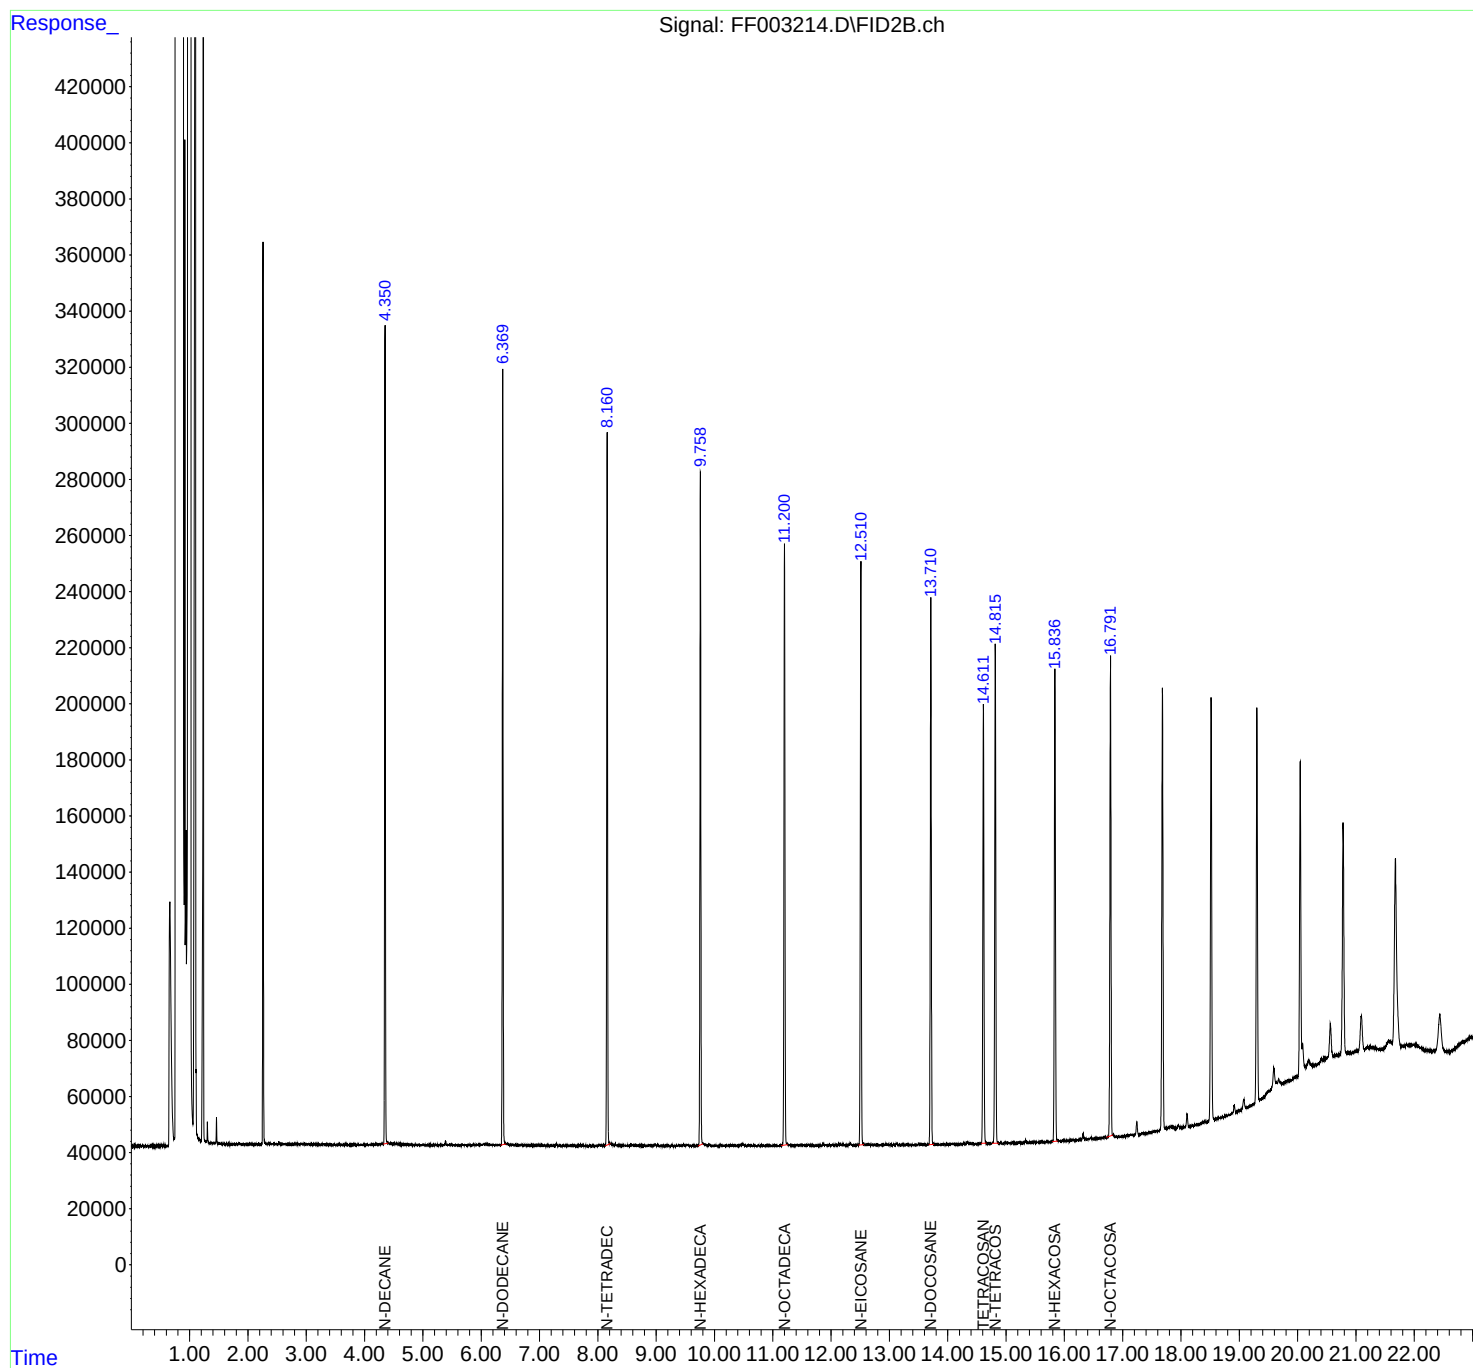


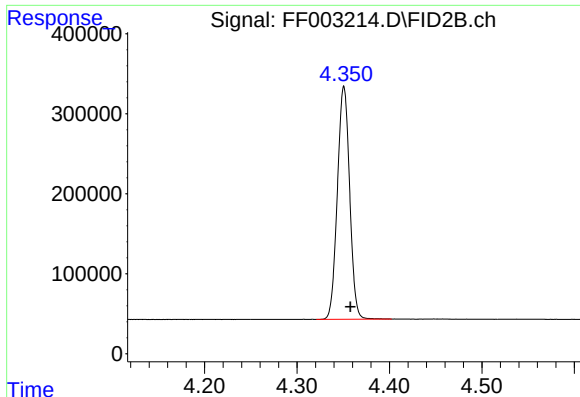

#2 N-DECANE


R.T.: 4.351 min
Delta R.T.: -0.007 min
Response: 2687175
Conc: 17.89 ug/ml

Instrument :
FID_F
ClientSampleId :
PB116288BSD

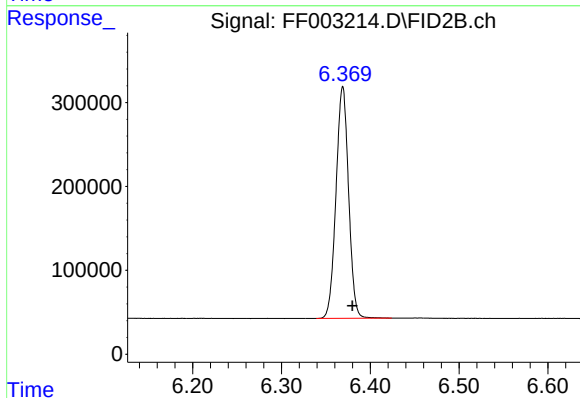


#3 N-DODECANE

R.T.: 6.369 min
Delta R.T.: -0.011 min
Response: 2713694
Conc: 17.93 ug/ml

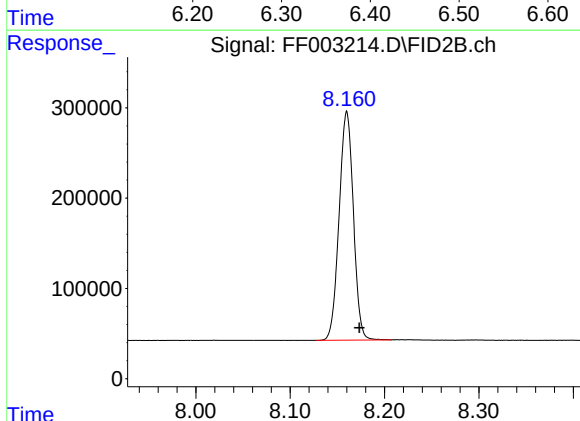


#4 N-TETRADECANE

R.T.: 8.160 min
Delta R.T.: -0.014 min
Response: 2662662
Conc: 17.47 ug/ml

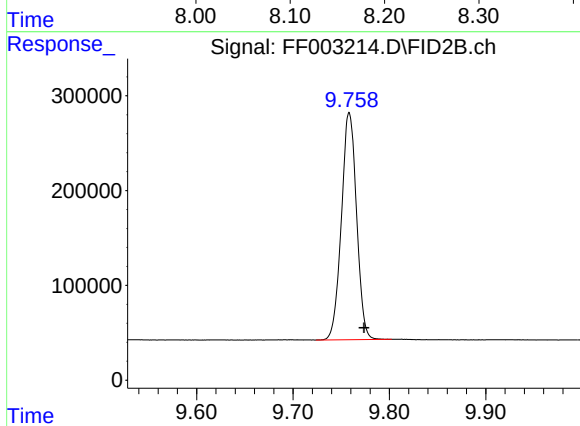

#5 N-HEXADECANE


R.T.: 9.758 min
Delta R.T.: -0.015 min
Response: 2607896
Conc: 17.01 ug/ml

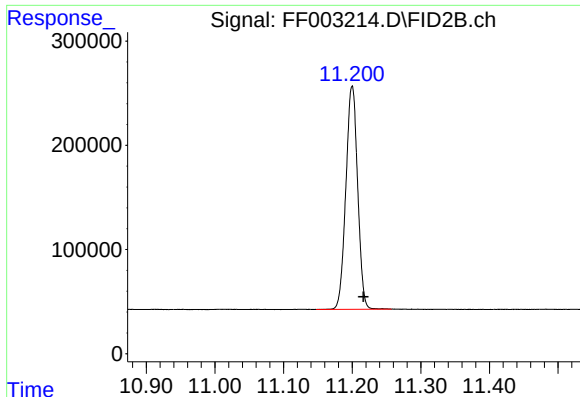

#6 N-OCTADECANE


R.T.: 11.200 min
Delta R.T.: -0.016 min
Response: 2556140
Conc: 16.62 ug/ml

Instrument :
FID_F
ClientSampleId :
PB116288BSD

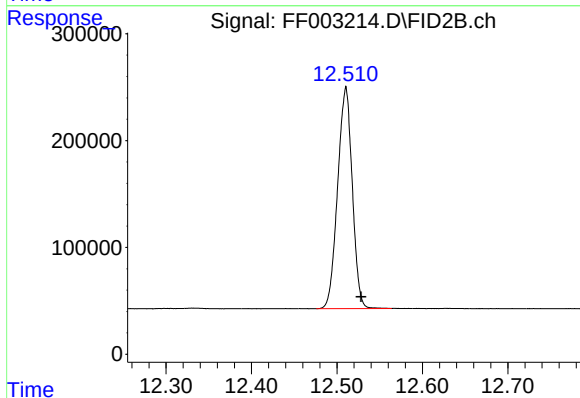


#7 N-EICOSANE

R.T.: 12.511 min
Delta R.T.: -0.017 min
Response: 2465805
Conc: 16.19 ug/ml

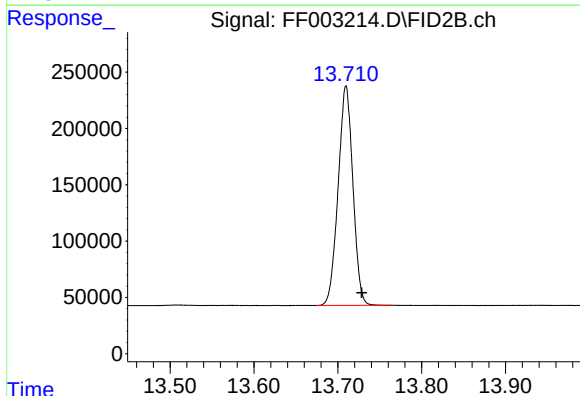


#8 N-DOCOSANE

R.T.: 13.710 min
Delta R.T.: -0.019 min
Response: 2390536
Conc: 15.86 ug/ml

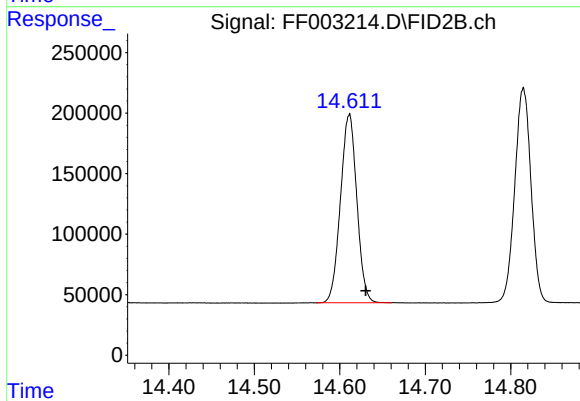

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.611 min
Delta R.T.: -0.019 min
Response: 2070583
Conc: 15.57 ug/ml

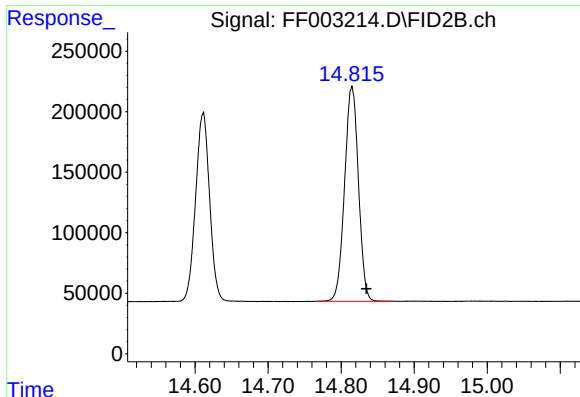

#10 N-TETRACOSANE


R.T.: 14.815 min
Delta R.T.: -0.020 min
Response: 2340759
Conc: 15.71 ug/ml

Instrument :
FID_F
ClientSampleId :
PB116288BSD

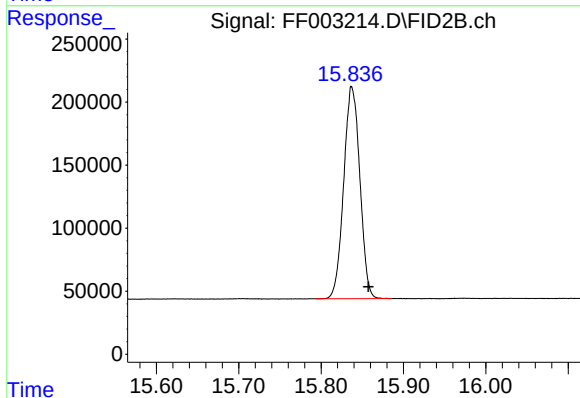

#11 N-HEXACOSANE

R.T.: 15.837 min
Delta R.T.: -0.020 min
Response: 2295020
Conc: 15.60 ug/ml

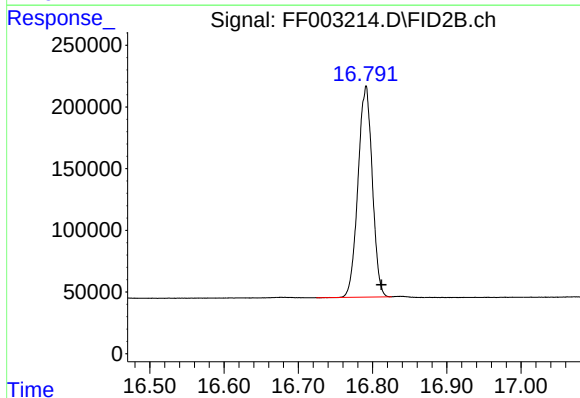

#12 N-OCTACOSANE

R.T.: 16.791 min
Delta R.T.: -0.021 min
Response: 2281172
Conc: 15.67 ug/ml