

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
 Data File : FF003215.D
 Signal(s) : FID2B.ch
 Acq On : 11 Jan 2019 00:54
 Operator : AJ\SJ
 Sample : IDOC-1 DRO-W-FE
 Misc : IDOC-1 DRO-W-FE
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 IDOC-1 DRO-W-FE

Integration File: autoint1.e
 Quant Time: Jan 11 06:12:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.612	1441454	10.842 ug/ml
Target Compounds			
2) N-DECANE	4.349	1699955	11.320 ug/ml
3) N-DODECANE	6.367	1749466	11.560 ug/ml
4) N-TETRADECANE	8.158	1735187	11.382 ug/ml
5) N-HEXADECANE	9.758	1727516	11.269 ug/ml
6) N-OCTADECANE	11.200	1693800	11.012 ug/ml
7) N-EICOSANE	12.510	1624423	10.668 ug/ml
8) N-DOCOSANE	13.710	1595888	10.586 ug/ml
10) N-TETRACOSANE	14.814	1954418	13.117 ug/ml
11) N-HEXACOSANE	15.838	1656663	11.260 ug/ml
12) N-OCTACOSANE	16.791	1808833	12.429 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
Data File : FF003215.D
Signal(s) : FID2B.ch
Acq On : 11 Jan 2019 00:54
Operator : AJ\SJ
Sample : IDOC-1 DRO-W-FE
Misc : IDOC-1 DRO-W-FE
ALS Vial : 73 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
IDOC-1 DRO-W-FE

Integration File: autoint1.e
Quant Time: Jan 11 06:12:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

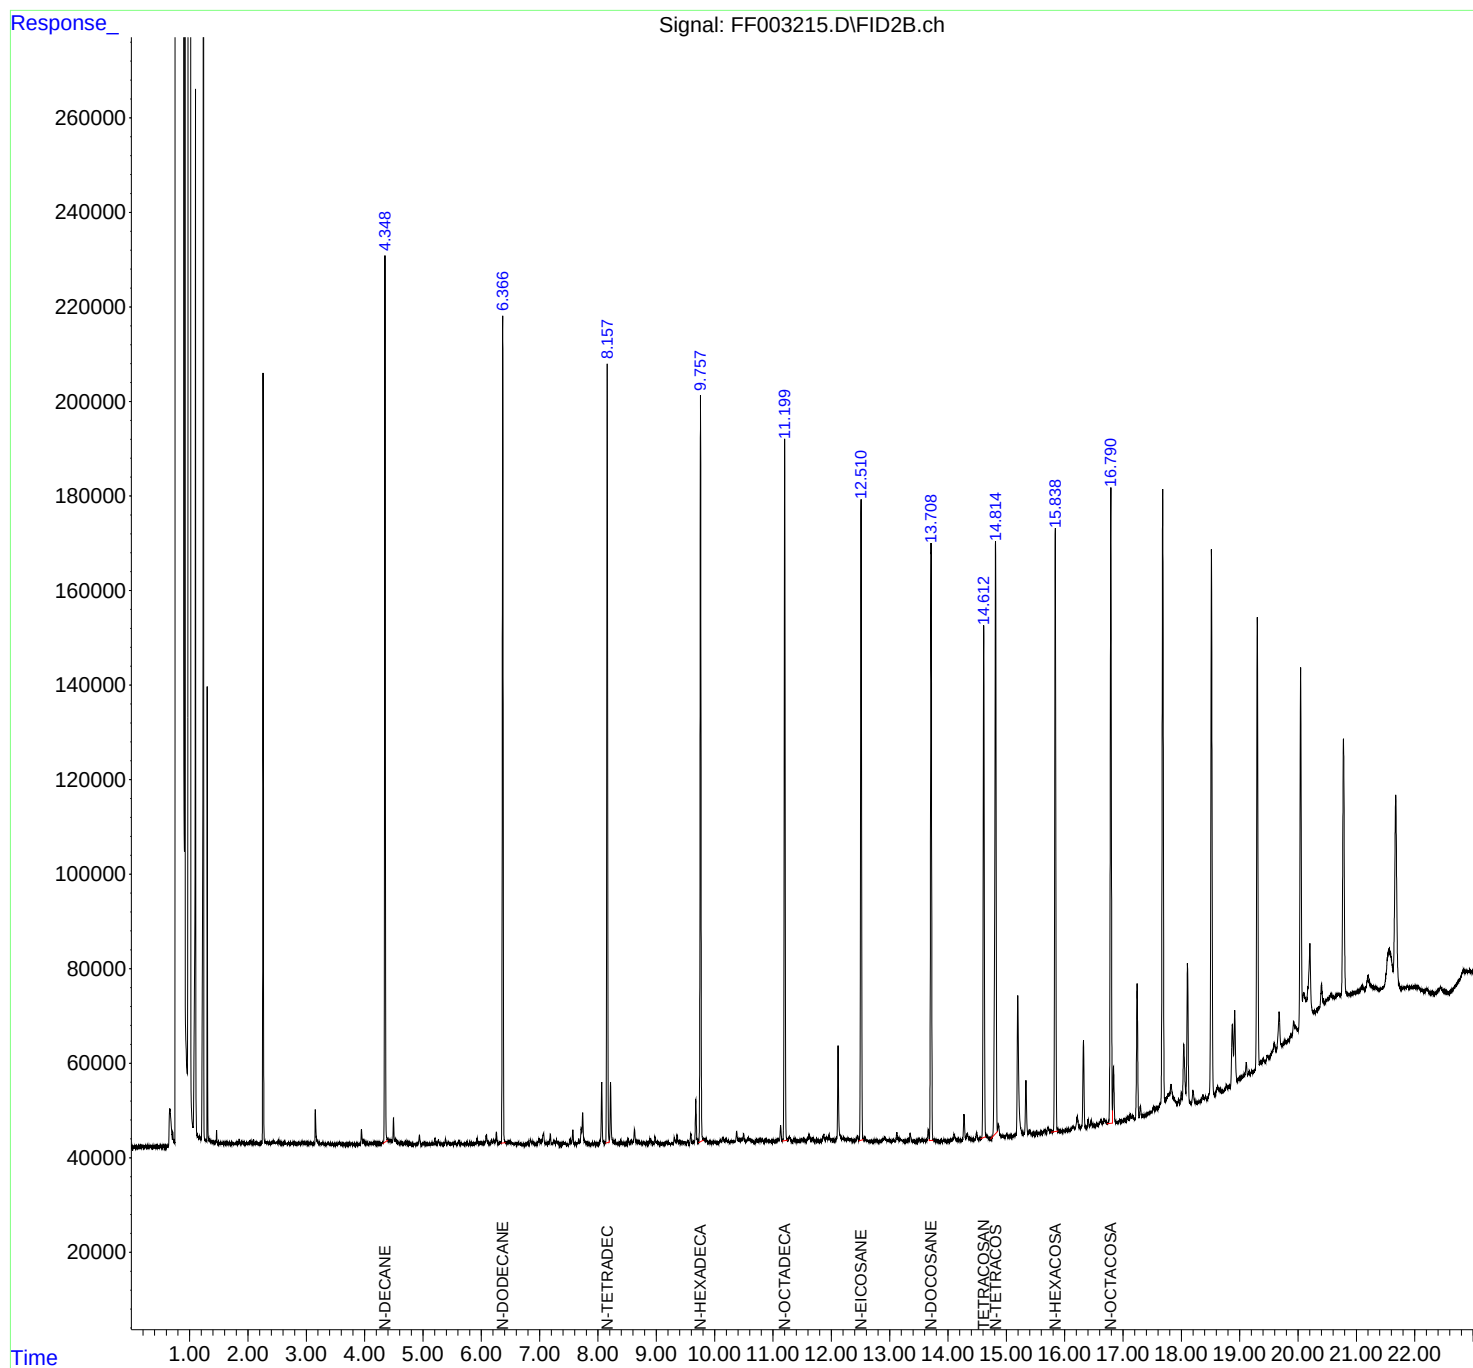


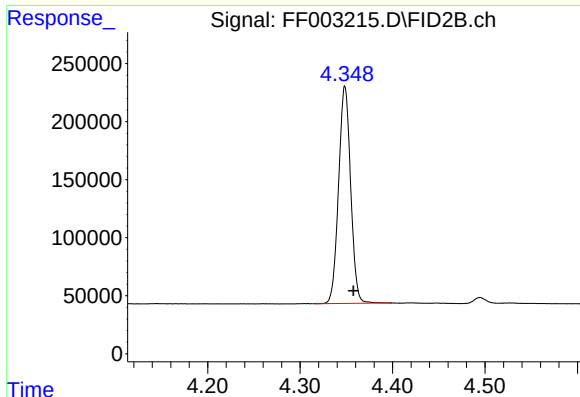

#2 N-DECANE


R.T.: 4.349 min
Delta R.T.: -0.009 min
Response: 1699955
Conc: 11.32 ug/ml

Instrument :
FID_F
ClientSampleId :
IDOC-1 DRO-W-FE

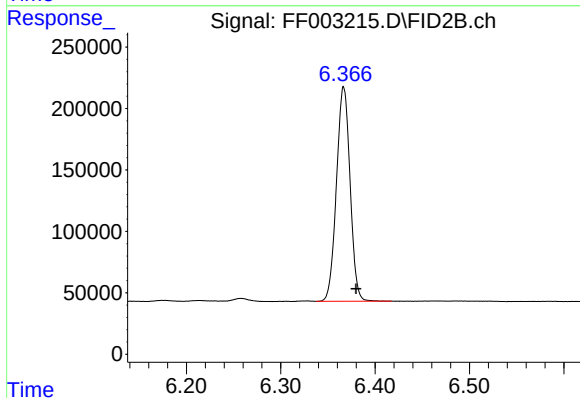


#3 N-DODECANE

R.T.: 6.367 min
Delta R.T.: -0.013 min
Response: 1749466
Conc: 11.56 ug/ml

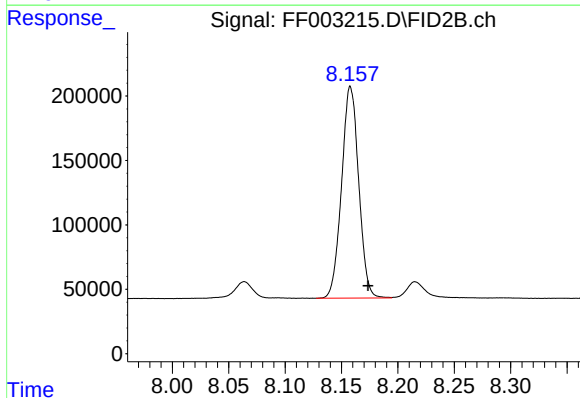


#4 N-TETRADECANE

R.T.: 8.158 min
Delta R.T.: -0.015 min
Response: 1735187
Conc: 11.38 ug/ml

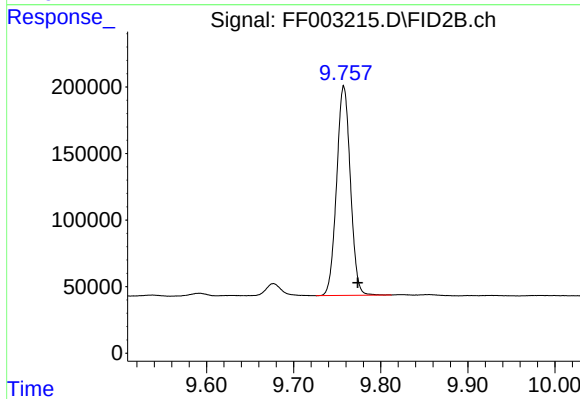

#5 N-HEXADECANE


R.T.: 9.758 min
Delta R.T.: -0.016 min
Response: 1727516
Conc: 11.27 ug/ml

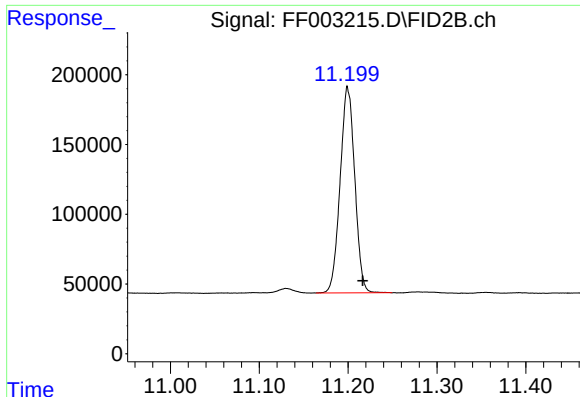

#6 N-OCTADECANE


R.T.: 11.200 min
Delta R.T.: -0.017 min
Response: 1693800
Conc: 11.01 ug/ml

Instrument :
FID_F
ClientSampleId :
IDOC-1 DRO-W-FE

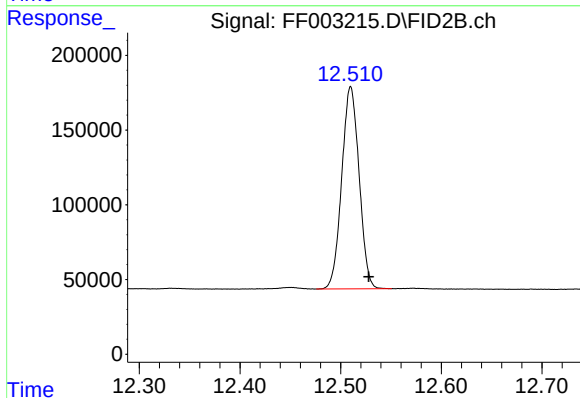


#7 N-EICOSANE

R.T.: 12.510 min
Delta R.T.: -0.018 min
Response: 1624423
Conc: 10.67 ug/ml

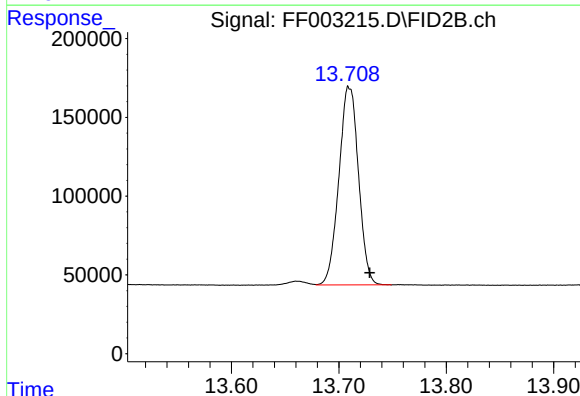


#8 N-DOCOSANE

R.T.: 13.710 min
Delta R.T.: -0.019 min
Response: 1595888
Conc: 10.59 ug/ml

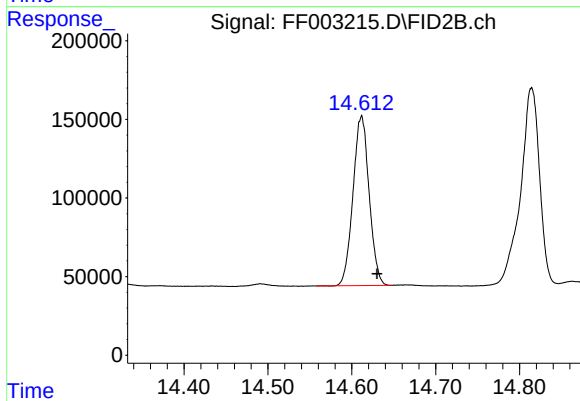

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.612 min
Delta R.T.: -0.019 min
Response: 1441454
Conc: 10.84 ug/ml

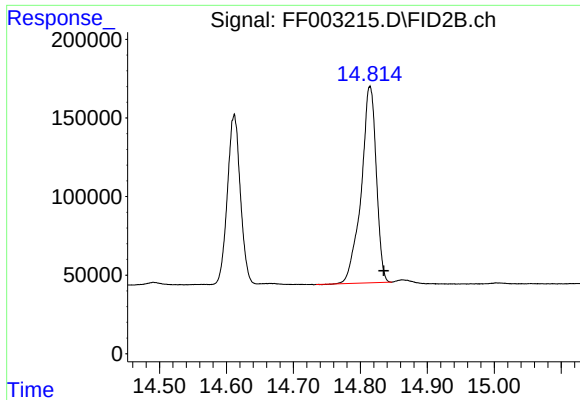

#10 N-TETRACOSANE


R.T.: 14.814 min
Delta R.T.: -0.021 min
Response: 1954418
Conc: 13.12 ug/ml

Instrument :
FID_F
ClientSampleId :
IDOC-1 DRO-W-FE

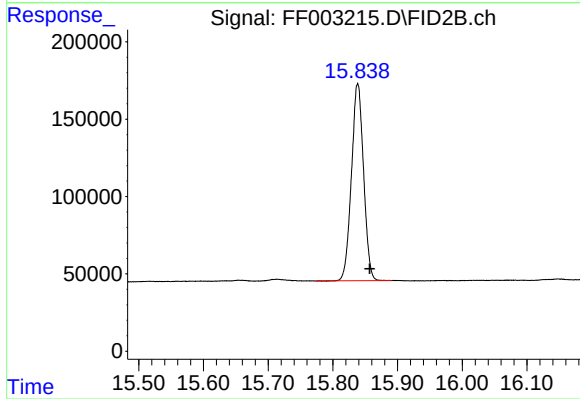

#11 N-HEXACOSANE

R.T.: 15.838 min
Delta R.T.: -0.019 min
Response: 1656663
Conc: 11.26 ug/ml

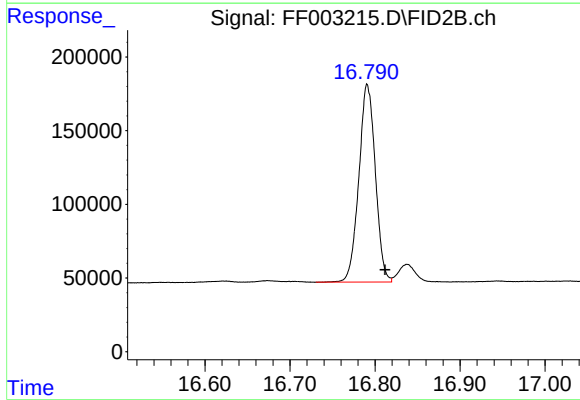

#12 N-OCTACOSANE

R.T.: 16.791 min
Delta R.T.: -0.021 min
Response: 1808833
Conc: 12.43 ug/ml