

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
 Data File : FF003217.D
 Signal(s) : FID2B.ch
 Acq On : 11 Jan 2019 01:54
 Operator : AJ\SJ
 Sample : IDOC-3 DRO-W-FE
 Misc : IDOC-3 DRO-W-FE
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 IDOC-3 DRO-W-FE

Integration File: autoint1.e
 Quant Time: Jan 11 06:13:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.611	1679797	12.635 ug/ml
Target Compounds			
2) N-DECANE	4.351	2104596	14.015 ug/ml
3) N-DODECANE	6.368	2159648	14.270 ug/ml
4) N-TETRADECANE	8.159	2132585	13.989 ug/ml
5) N-HEXADECANE	9.758	2144425	13.988 ug/ml
6) N-OCTADECANE	11.200	2047852	13.314 ug/ml
7) N-EICOSANE	12.510	1963044	12.892 ug/ml
8) N-DOCOSANE	13.709	1930650	12.806 ug/ml
10) N-TETRACOSANE	14.814	2400793	16.112 ug/ml
11) N-HEXACOSANE	15.838	1954372	13.283 ug/ml
12) N-OCTACOSANE	16.790	2054548	14.117 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
Data File : FF003217.D
Signal(s) : FID2B.ch
Acq On : 11 Jan 2019 01:54
Operator : AJ\SJ
Sample : IDOC-3 DRO-W-FE
Misc : IDOC-3 DRO-W-FE
ALS Vial : 75 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
IDOC-3 DRO-W-FE

Integration File: autoint1.e
Quant Time: Jan 11 06:13:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

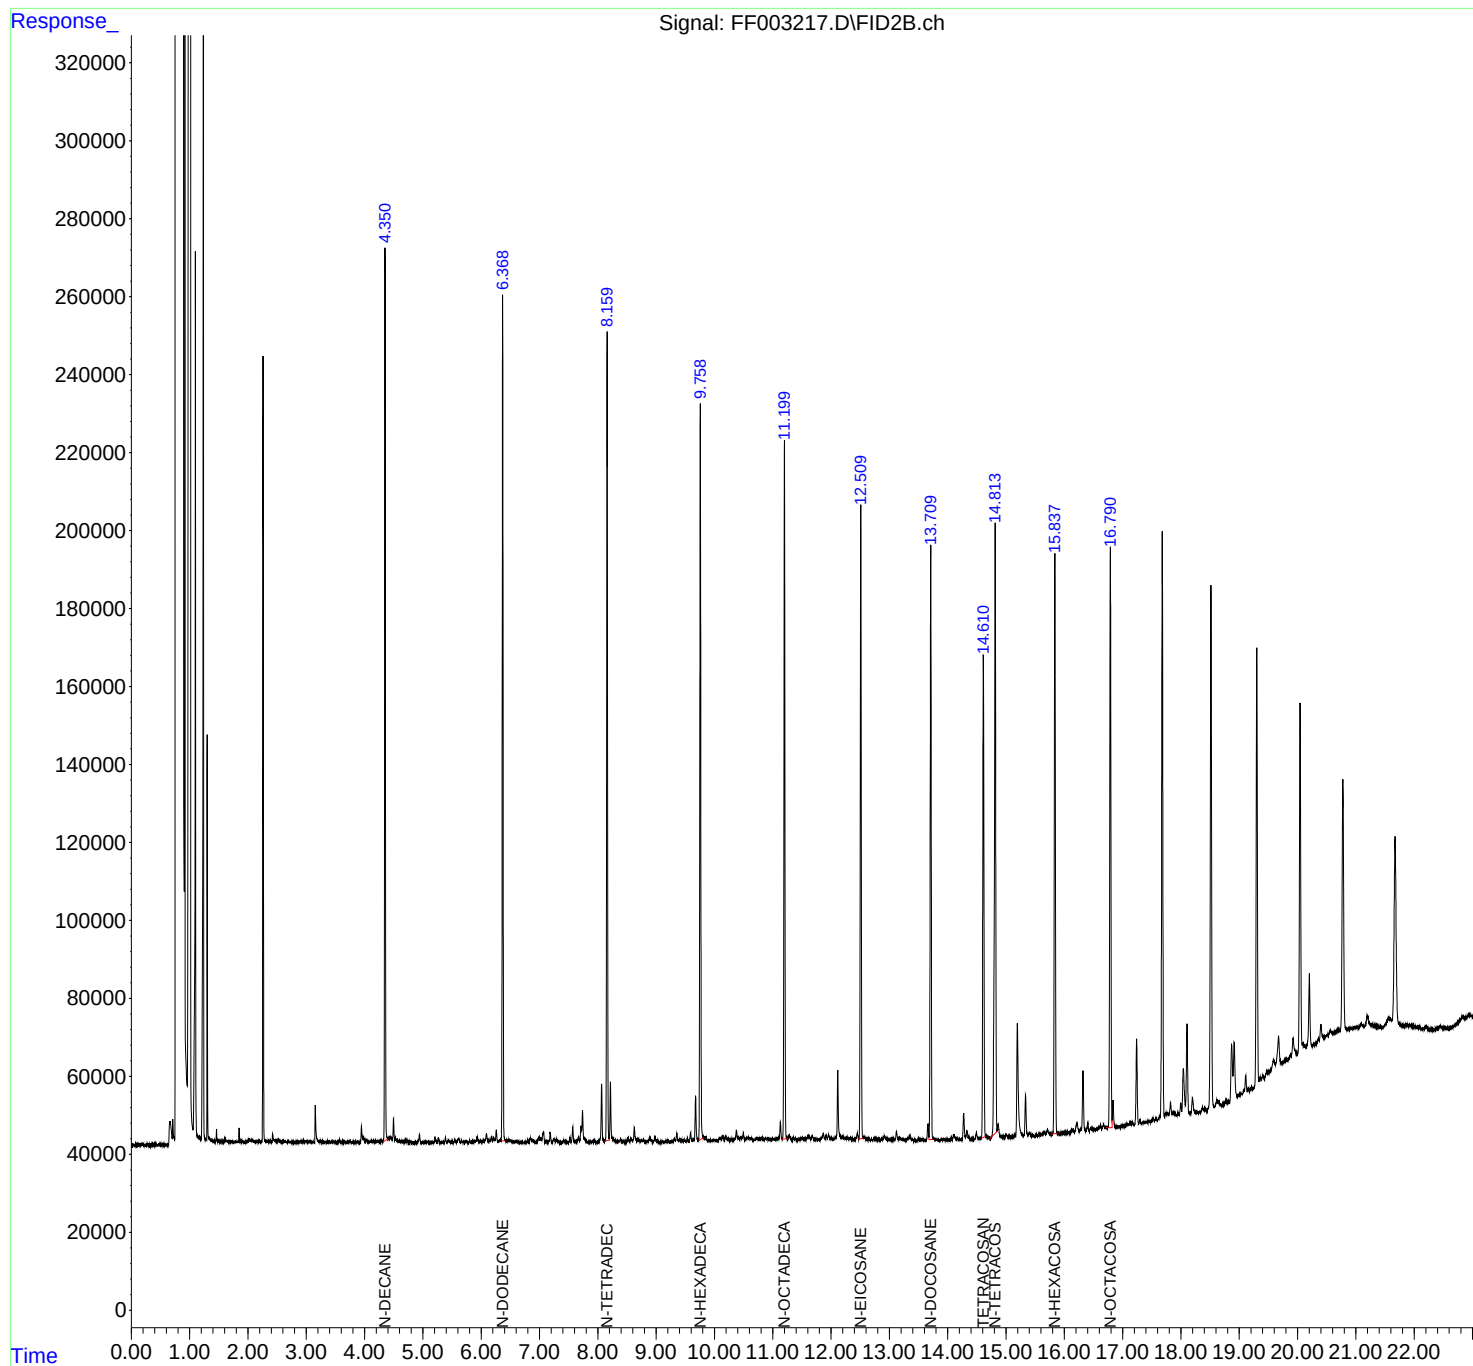


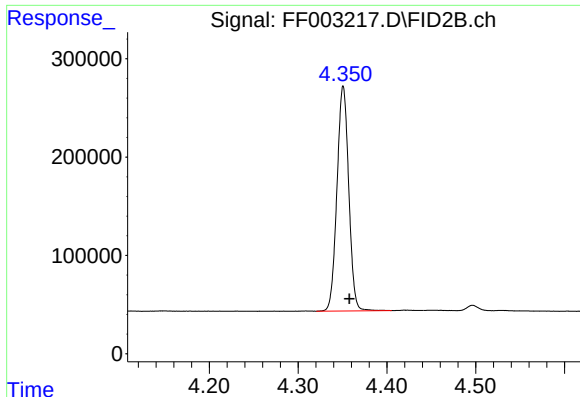

#2 N-DECANE


R.T.: 4.351 min
Delta R.T.: -0.007 min
Response: 2104596
Conc: 14.01 ug/ml

Instrument :
FID_F
ClientSampleId :
IDOC-3 DRO-W-FE

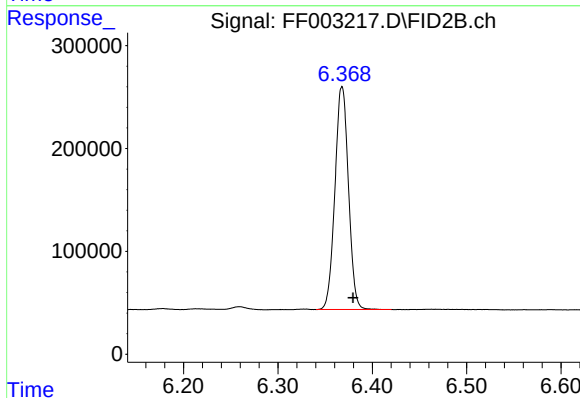


#3 N-DODECANE

R.T.: 6.368 min
Delta R.T.: -0.012 min
Response: 2159648
Conc: 14.27 ug/ml

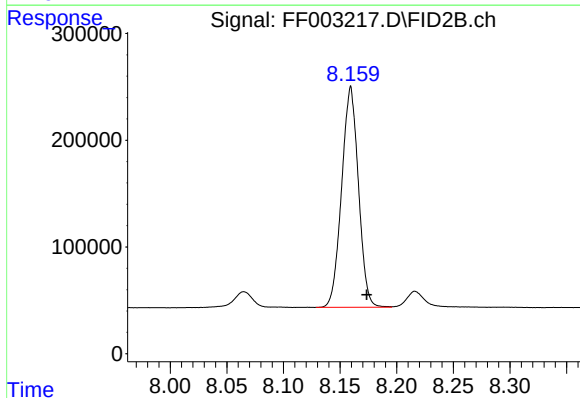


#4 N-TETRADECANE

R.T.: 8.159 min
Delta R.T.: -0.014 min
Response: 2132585
Conc: 13.99 ug/ml

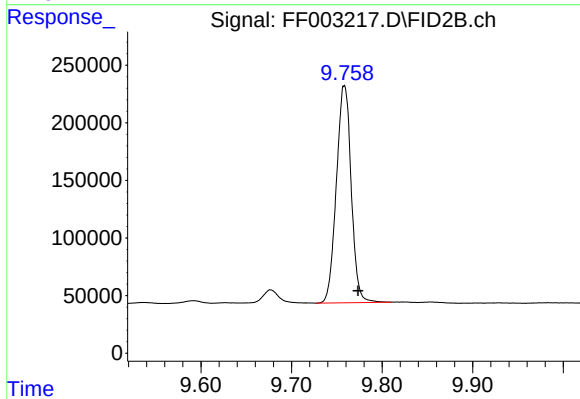

#5 N-HEXADECANE


R.T.: 9.758 min
Delta R.T.: -0.015 min
Response: 2144425
Conc: 13.99 ug/ml

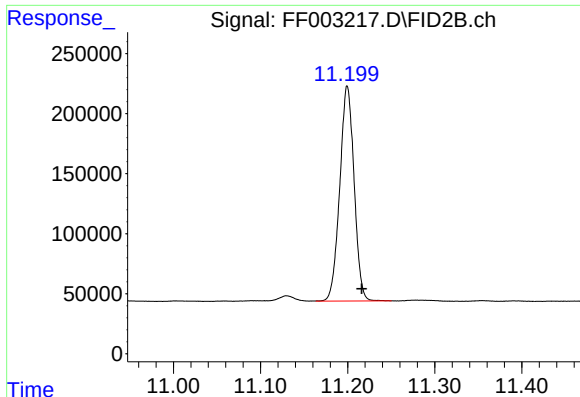

#6 N-OCTADECANE


R.T.: 11.200 min
Delta R.T.: -0.017 min
Response: 2047852
Conc: 13.31 ug/ml

Instrument :
FID_F
ClientSampleId :
IDOC-3 DRO-W-FE

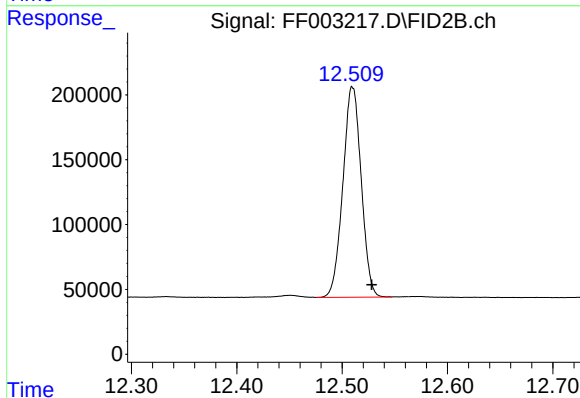


#7 N-EICOSANE

R.T.: 12.510 min
Delta R.T.: -0.018 min
Response: 1963044
Conc: 12.89 ug/ml

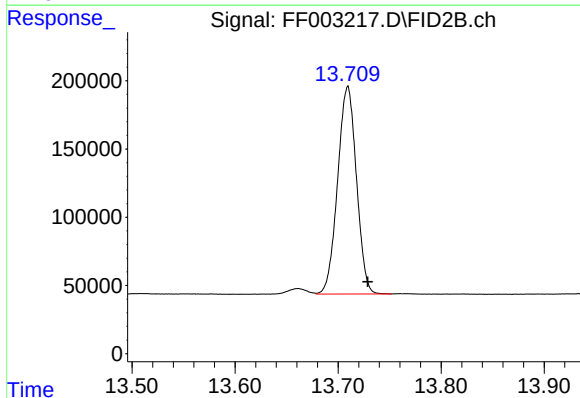


#8 N-DOCOSANE

R.T.: 13.709 min
Delta R.T.: -0.019 min
Response: 1930650
Conc: 12.81 ug/ml

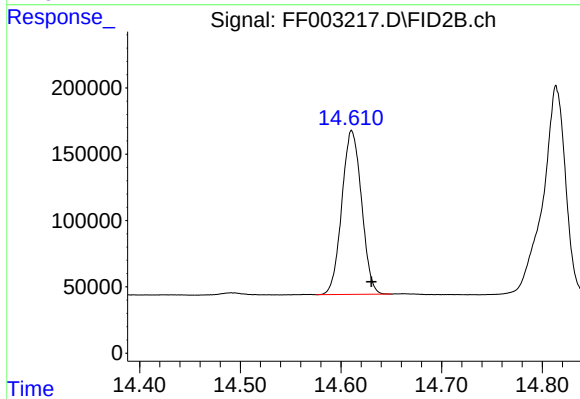

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.611 min
Delta R.T.: -0.020 min
Response: 1679797
Conc: 12.64 ug/ml

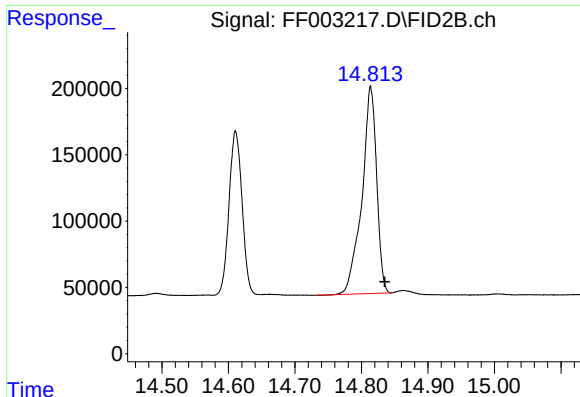

#10 N-TETRACOSANE


R.T.: 14.814 min
Delta R.T.: -0.021 min
Response: 2400793
Conc: 16.11 ug/ml

Instrument :
FID_F
ClientSampleId :
IDOC-3 DRO-W-FE

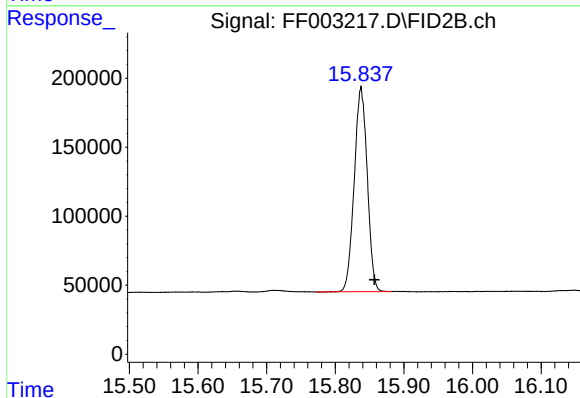

#11 N-HEXACOSANE

R.T.: 15.838 min
Delta R.T.: -0.020 min
Response: 1954372
Conc: 13.28 ug/ml

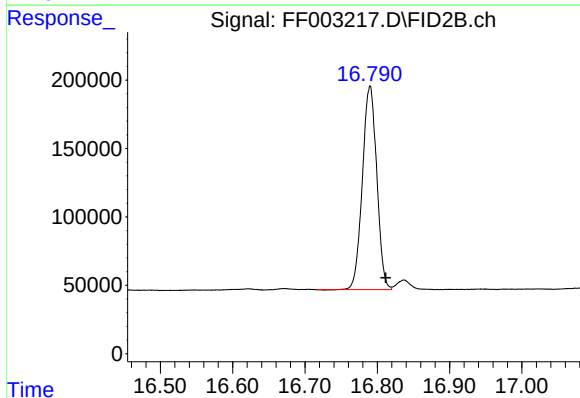

#12 N-OCTACOSANE

R.T.: 16.790 min
Delta R.T.: -0.022 min
Response: 2054548
Conc: 14.12 ug/ml