

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
 Data File : FF003218.D
 Signal(s) : FID2B.ch
 Acq On : 11 Jan 2019 02:24
 Operator : AJ\SJ
 Sample : IDOC-4 DRO-W-FE
 Misc : IDOC-4 DRO-W-FE
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 IDOC-4 DRO-W-FE

Integration File: autoint1.e
 Quant Time: Jan 11 06:14:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.612	1739240	13.082 ug/ml
Target Compounds			
2) N-DECANE	4.350	2167204	14.432 ug/ml
3) N-DODECANE	6.368	2243391	14.824 ug/ml
4) N-TETRADECANE	8.159	2206372	14.473 ug/ml
5) N-HEXADECANE	9.758	2162350	14.105 ug/ml
6) N-OCTADECANE	11.200	2108518	13.709 ug/ml
7) N-EICOSANE	12.510	2015541	13.236 ug/ml
8) N-DOCOSANE	13.709	1973818	13.093 ug/ml
10) N-TETRACOSANE	14.814	2408015	16.161 ug/ml
11) N-HEXACOSANE	15.838	1933156	13.139 ug/ml
12) N-OCTACOSANE	16.790	1948533	13.388 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011019\
Data File : FF003218.D
Signal(s) : FID2B.ch
Acq On : 11 Jan 2019 02:24
Operator : AJ\SJ
Sample : IDOC-4 DRO-W-FE
Misc : IDOC-4 DRO-W-FE
ALS Vial : 76 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
IDOC-4 DRO-W-FE

Integration File: autoint1.e
Quant Time: Jan 11 06:14:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

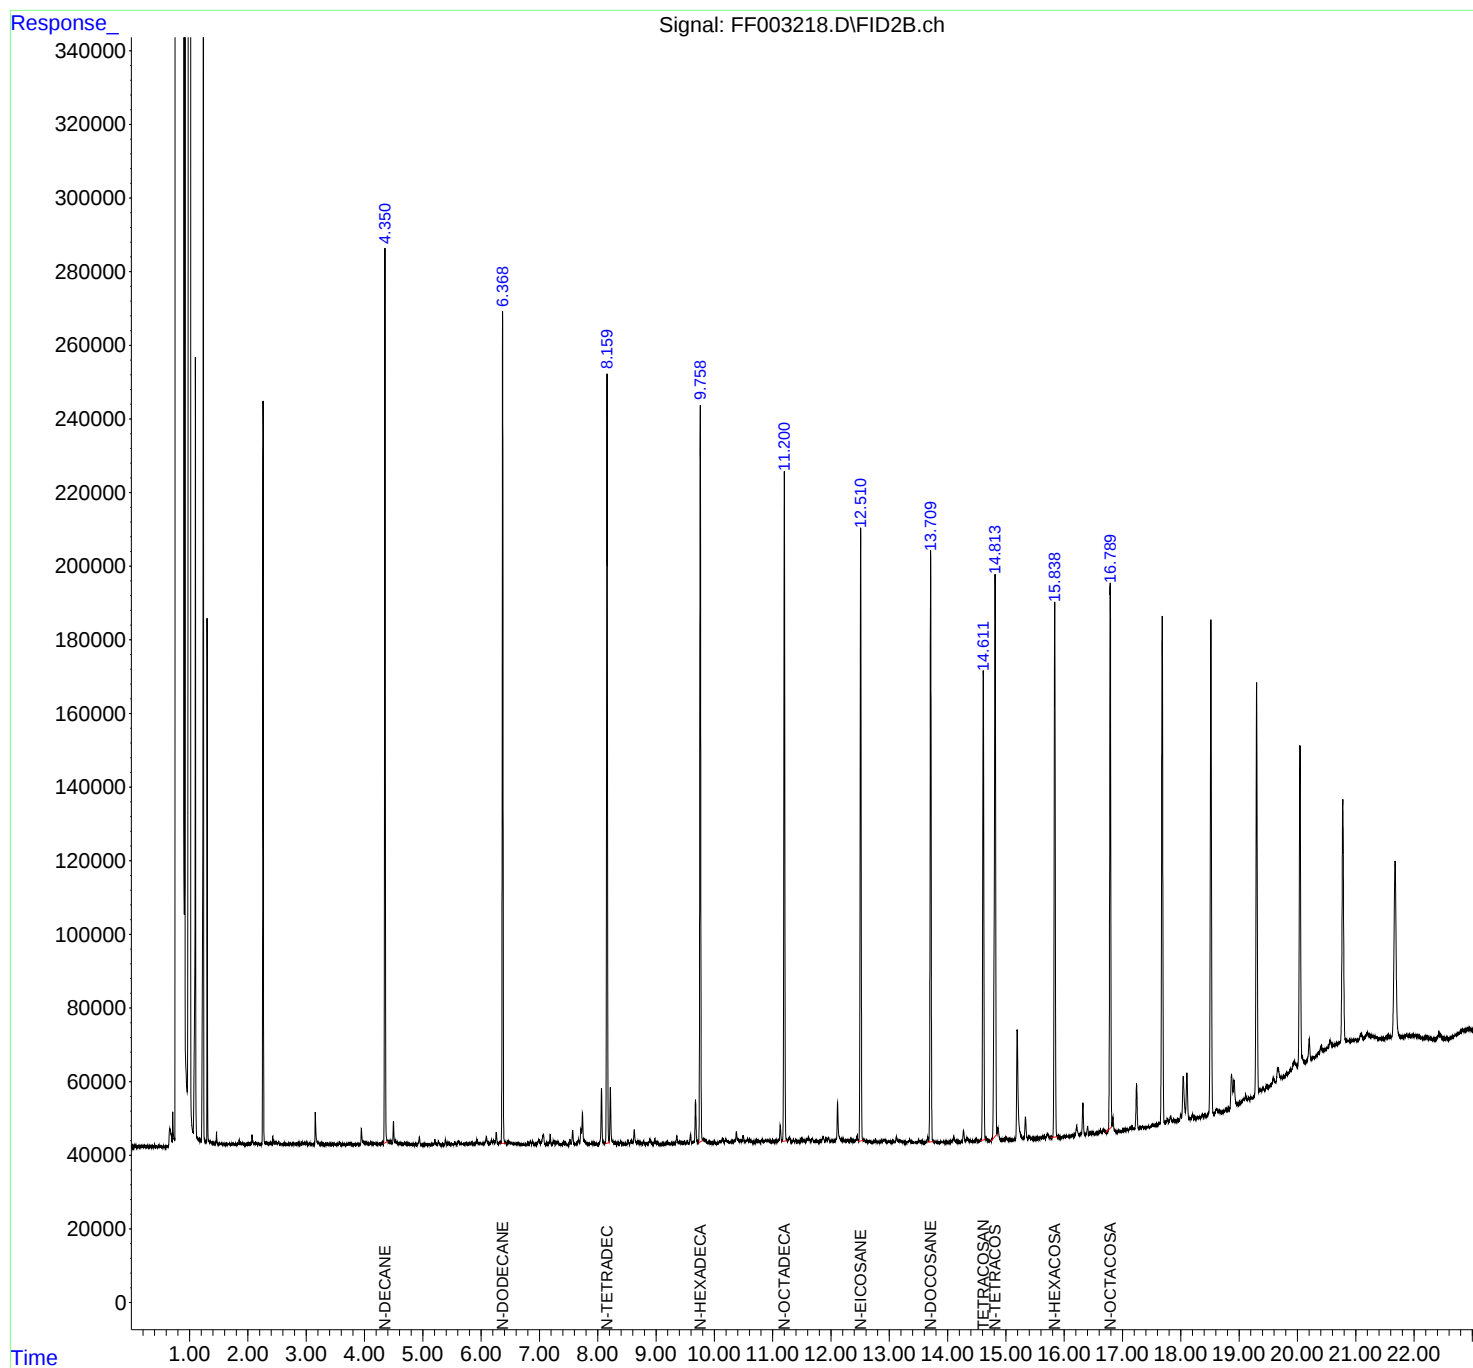


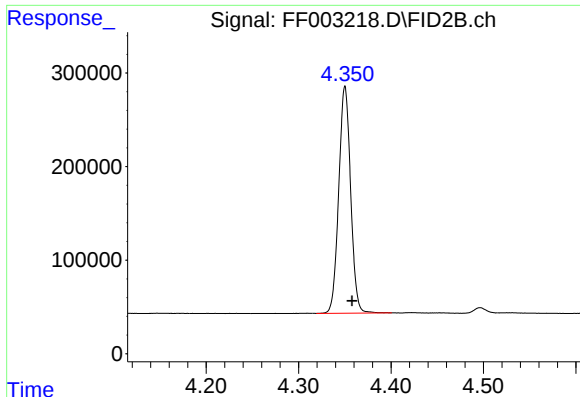

#2 N-DECANE


R.T.: 4.350 min
Delta R.T.: -0.008 min
Response: 2167204
Conc: 14.43 ug/ml

Instrument :
FID_F
ClientSampleId :
IDOC-4 DRO-W-FE

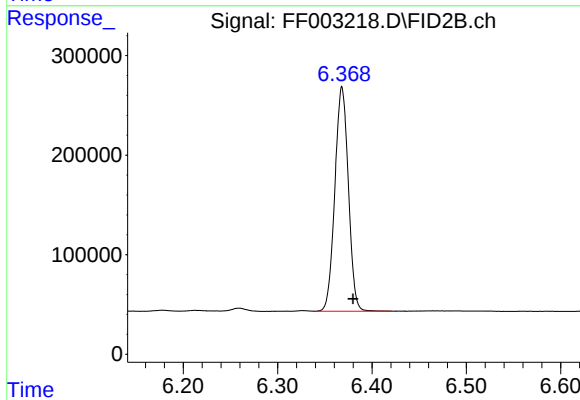


#3 N-DODECANE

R.T.: 6.368 min
Delta R.T.: -0.011 min
Response: 2243391
Conc: 14.82 ug/ml

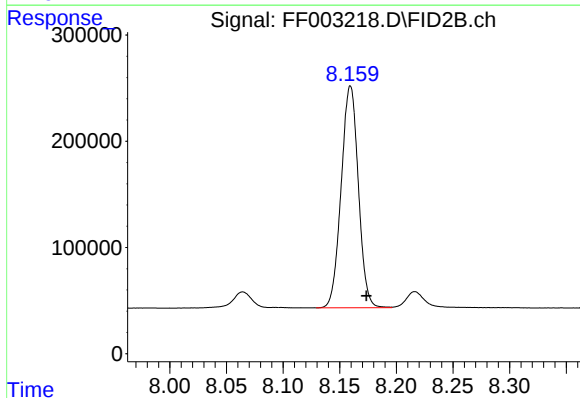


#4 N-TETRADECANE

R.T.: 8.159 min
Delta R.T.: -0.014 min
Response: 2206372
Conc: 14.47 ug/ml

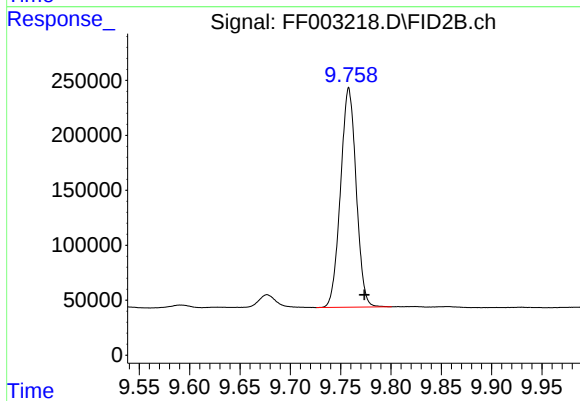

#5 N-HEXADECANE


R.T.: 9.758 min
Delta R.T.: -0.015 min
Response: 2162350
Conc: 14.11 ug/ml

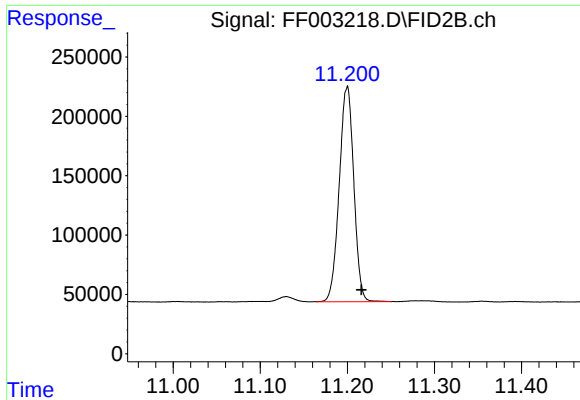

#6 N-OCTADECANE


R.T.: 11.200 min
Delta R.T.: -0.016 min
Response: 2108518
Conc: 13.71 ug/ml

Instrument :
FID_F
ClientSampleId :
IDOC-4 DRO-W-FE

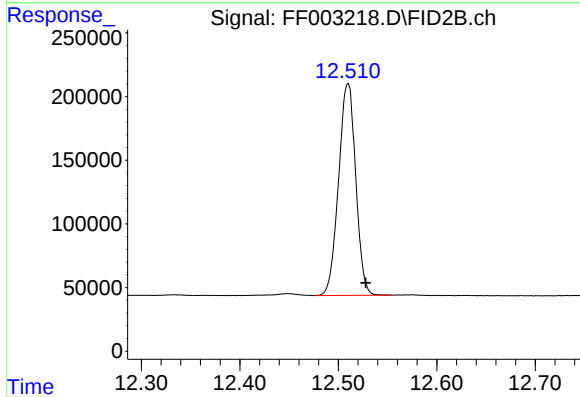


#7 N-EICOSANE

R.T.: 12.510 min
Delta R.T.: -0.018 min
Response: 2015541
Conc: 13.24 ug/ml

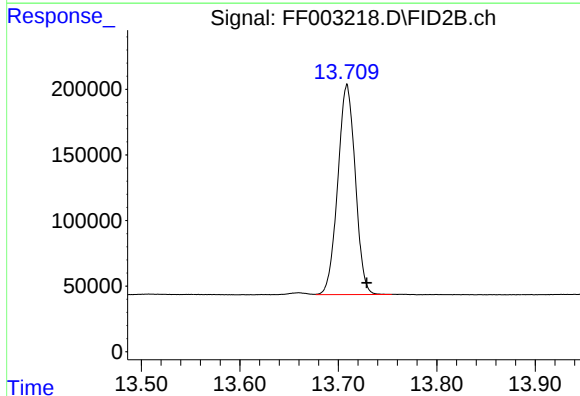


#8 N-DOCOSANE

R.T.: 13.709 min
Delta R.T.: -0.020 min
Response: 1973818
Conc: 13.09 ug/ml

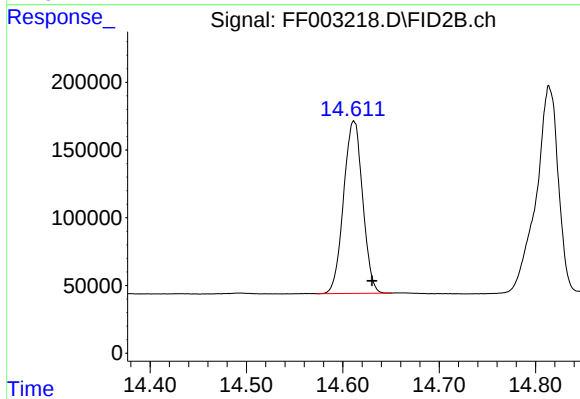

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.612 min
Delta R.T.: -0.019 min
Response: 1739240
Conc: 13.08 ug/ml

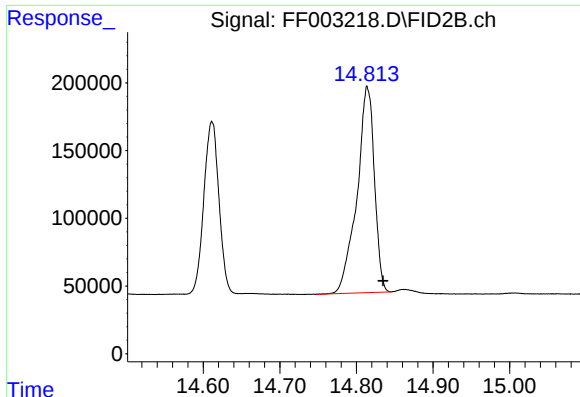

#10 N-TETRACOSANE


R.T.: 14.814 min
Delta R.T.: -0.021 min
Response: 2408015
Conc: 16.16 ug/ml

Instrument :
FID_F
ClientSampleId :
IDOC-4 DRO-W-FE

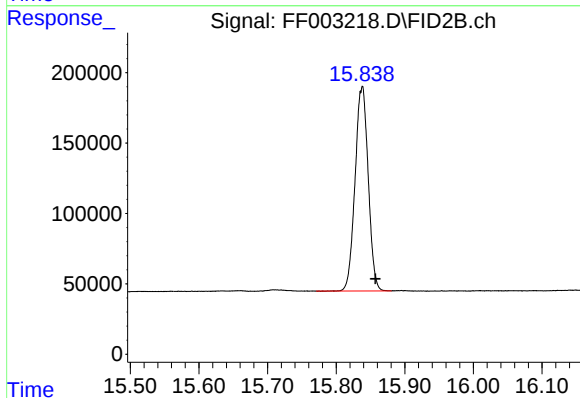

#11 N-HEXACOSANE

R.T.: 15.838 min
Delta R.T.: -0.019 min
Response: 1933156
Conc: 13.14 ug/ml

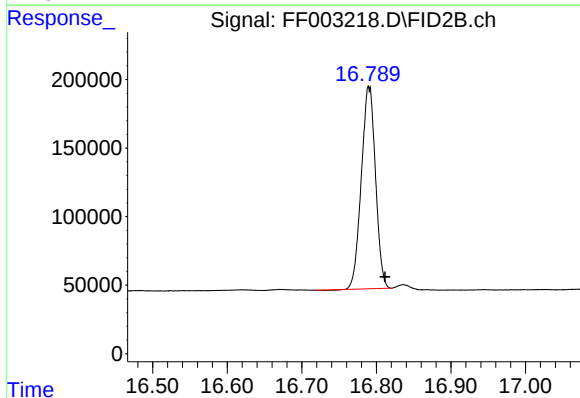

#12 N-OCTACOSANE

R.T.: 16.790 min
Delta R.T.: -0.022 min
Response: 1948533
Conc: 13.39 ug/ml