

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011022\
 Data File : FF009662.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jan 2022 16:16
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 10 17:29:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.457	2095911	18.093 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.623	81019	0.680 ug/ml
13) N-TRIACONTANE	17.507	213490	1.864 ug/ml
14) N-DOTRIACONTANE	18.336	298563	2.732 ug/ml
15) N-TETRATRIACONTANE	19.117	461543	4.357 ug/ml
16) N-HEXATRIACONTANE	19.855	189218	1.889 ug/ml
17) N-OCTATRIACONTANE	20.559	63634	0.648 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011022\
Data File : FF009662.D
Signal(s) : FID2B.ch
Acq On : 10 Jan 2022 16:16
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 10 17:29:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

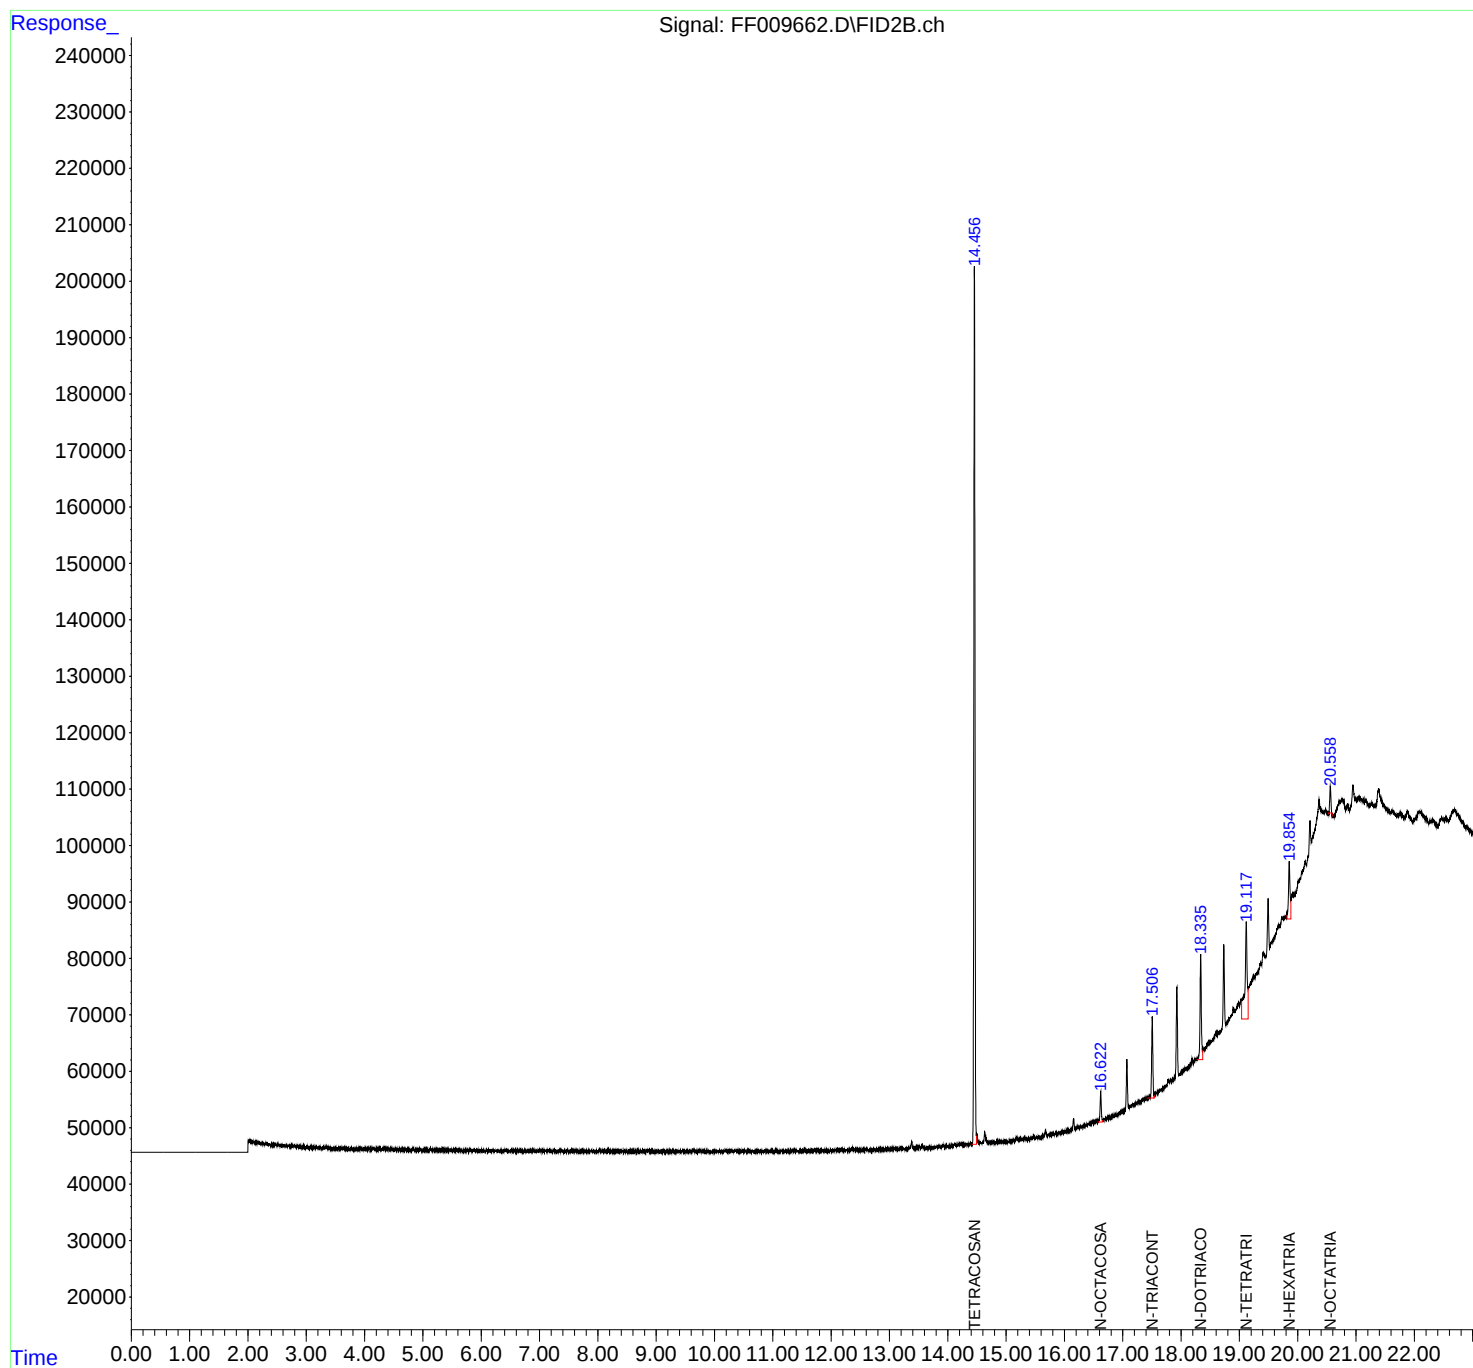


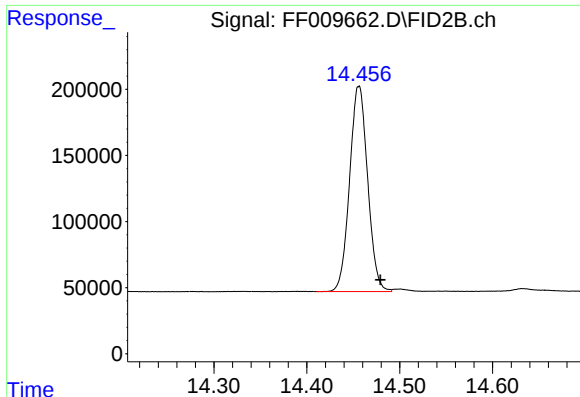

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.457 min
Delta R.T.: -0.023 min
Response: 2095911
Conc: 18.09 ug/ml

Instrument :
FID_F
ClientSampleId :

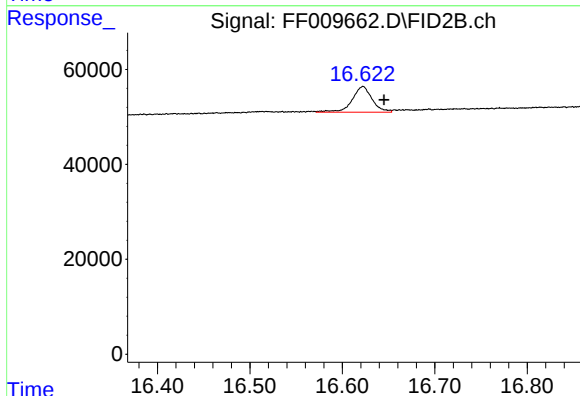


#12 N-OCTACOSANE

R.T.: 16.623 min
Delta R.T.: -0.023 min
Response: 81019
Conc: 0.68 ug/ml

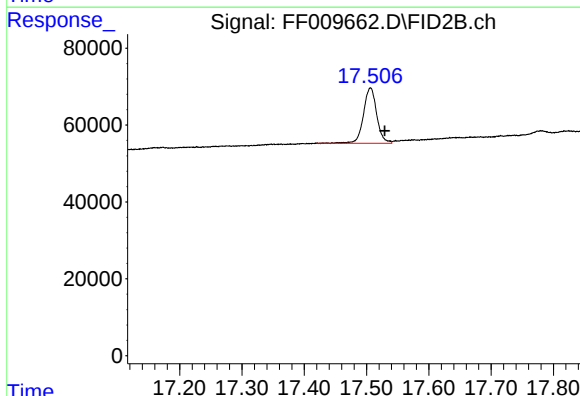


#13 N-TRIACONTANE

R.T.: 17.507 min
Delta R.T.: -0.023 min
Response: 213490
Conc: 1.86 ug/ml

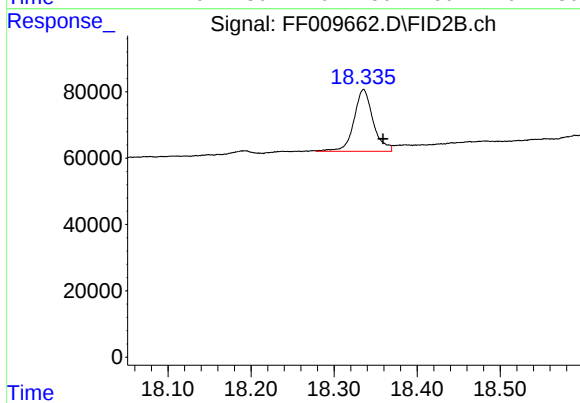

#14 N-DOTRIACONTANE


R.T.: 18.336 min
Delta R.T.: -0.023 min
Response: 298563
Conc: 2.73 ug/ml

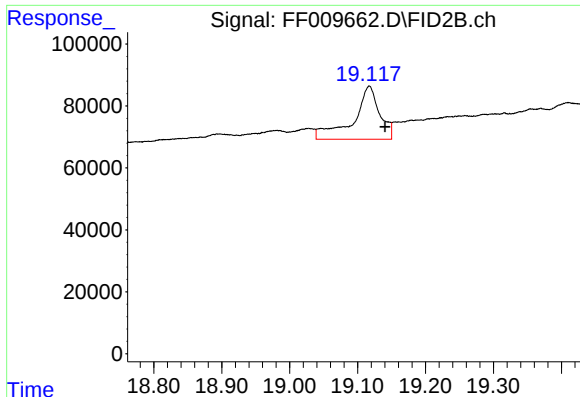

#15 N-TETRATRIACONTANE


R.T.: 19.117 min
Delta R.T.: -0.023 min
Response: 461543
Conc: 4.36 ug/ml

Instrument :
FID_F
ClientSampleId :

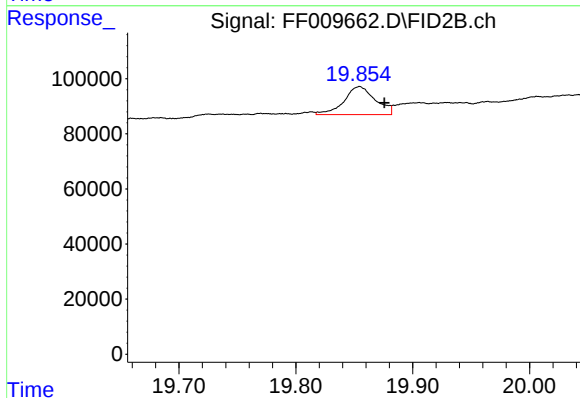

#16 N-HEXATRIACONTANE

R.T.: 19.855 min
Delta R.T.: -0.021 min
Response: 189218
Conc: 1.89 ug/ml

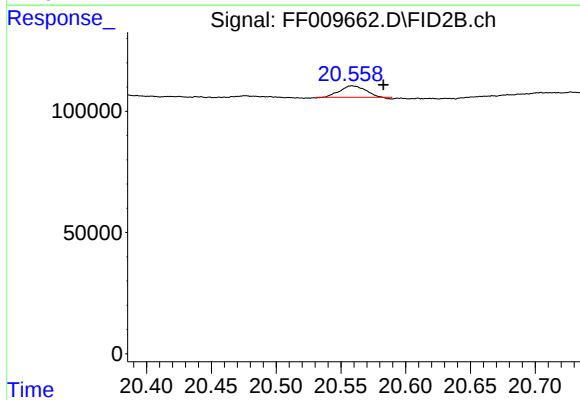

#17 N-OCTATRIACONTANE

R.T.: 20.559 min
Delta R.T.: -0.024 min
Response: 63634
Conc: 0.65 ug/ml