

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011022\
 Data File : FF009671.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jan 2022 21:37
 Operator : AJ\MA
 Sample : N1051-06MSD
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB-6-(4.5-5)MSD

Integration File: Sample.e
 Quant Time: Jan 11 06:42:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.453	1707082	14.737 ug/ml
Target Compounds			
2) N-DECANE	4.242	2752606	19.306 ug/ml
3) N-DODECANE	6.248	2769750	19.153 ug/ml
4) N-TETRADECANE	8.033	2788338	19.178 ug/ml
5) N-HEXADECANE	9.625	2460497	17.132 ug/ml
6) N-OCTADECANE	11.060	2593011	17.966 ug/ml
7) N-EICOSANE	12.364	2474882	17.463 ug/ml
8) N-DOCOSANE	13.558	2383353	17.491 ug/ml
10) N-TETRACOSANE	14.657	2363827	17.953 ug/ml
11) N-HEXACOSANE	15.674	2252253	18.021 ug/ml
12) N-OCTACOSANE	16.621	2299818	19.314 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011022\
Data File : FF009671.D
Signal(s) : FID2B.ch
Acq On : 10 Jan 2022 21:37
Operator : AJ\MA
Sample : N1051-06MSD
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-6-(4.5-5)MSD

Integration File: Sample.e
Quant Time: Jan 11 06:42:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

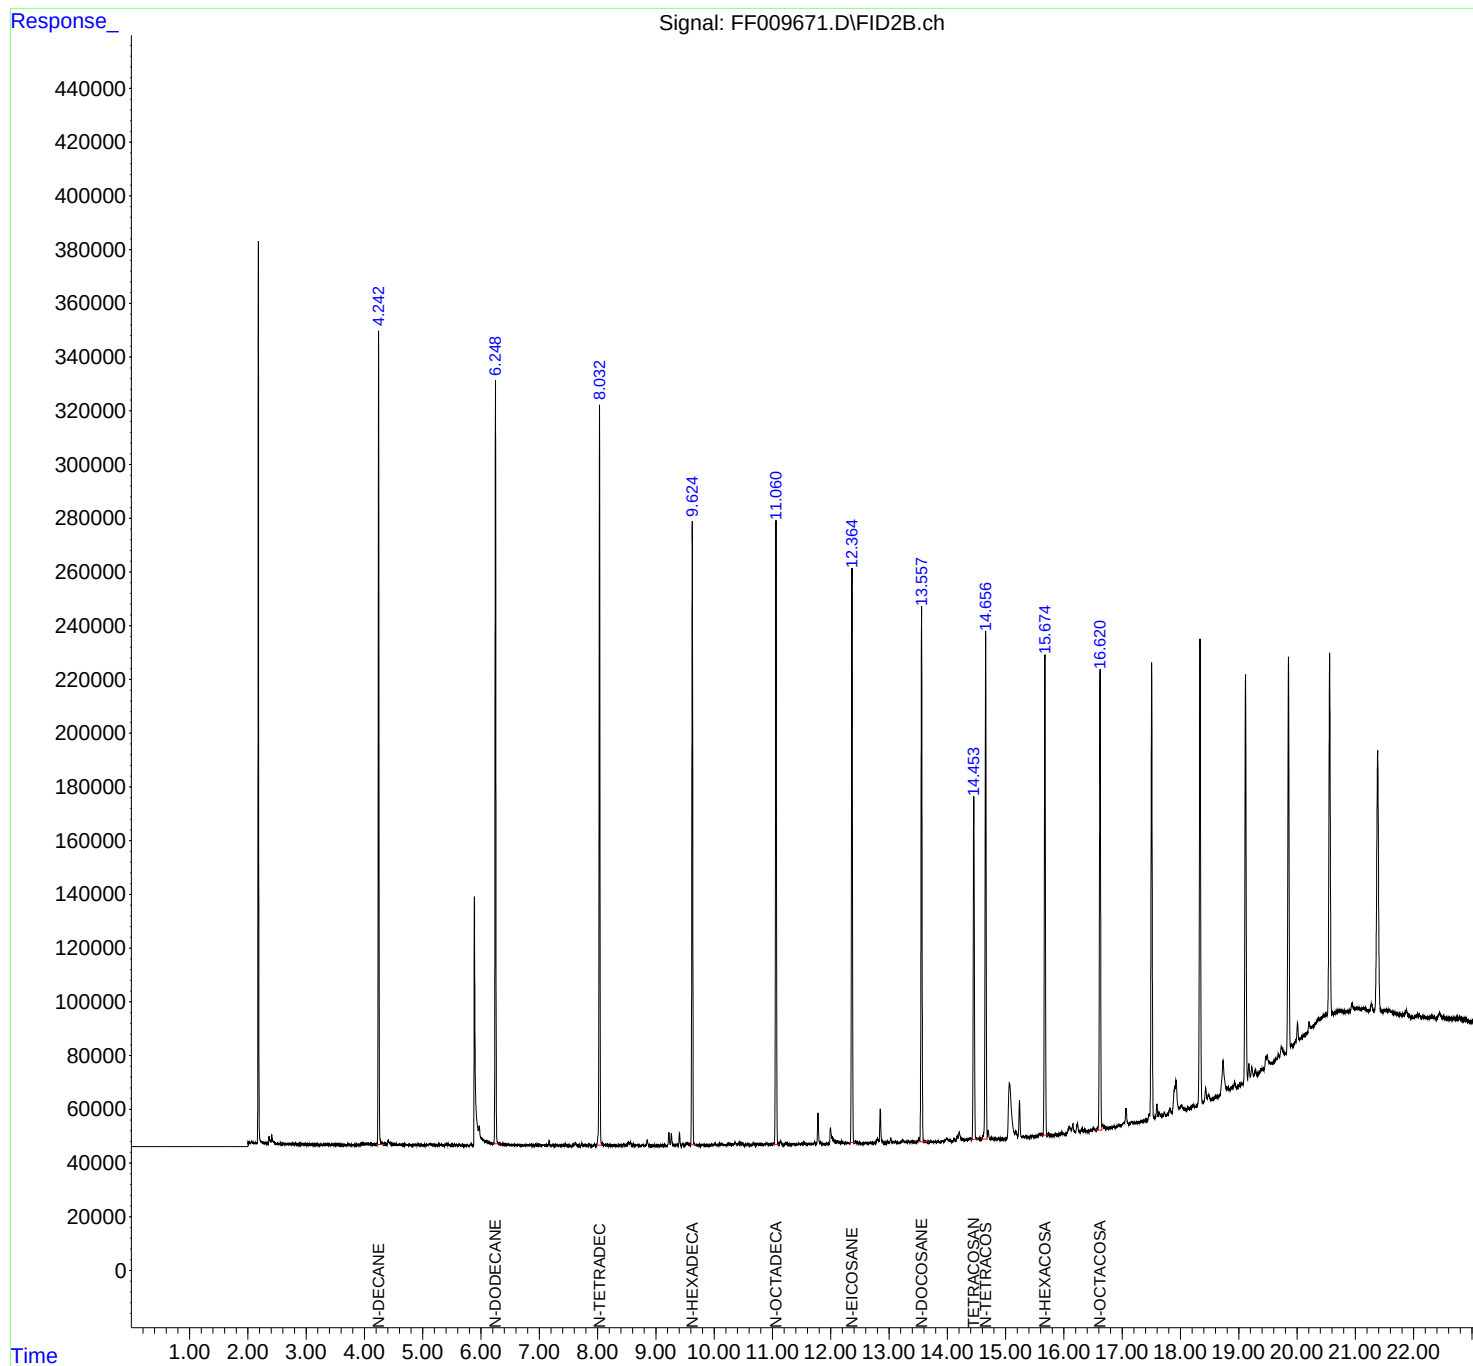


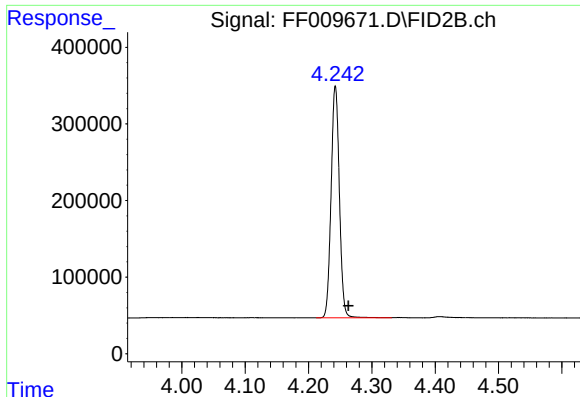

#2 N-DECANE


R.T.: 4.242 min
Delta R.T.: -0.021 min
Response: 2752606
Conc: 19.31 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-6-(4.5-5)MSD

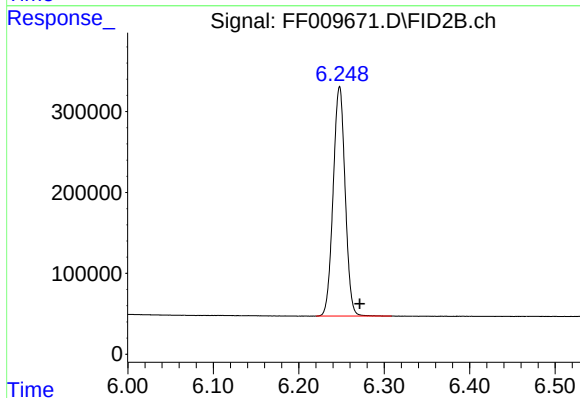


#3 N-DODECANE

R.T.: 6.248 min
Delta R.T.: -0.023 min
Response: 2769750
Conc: 19.15 ug/ml

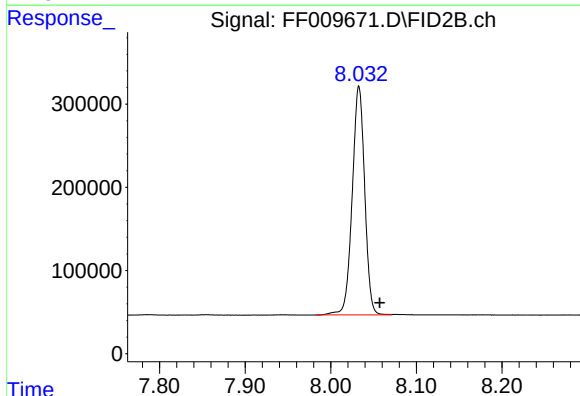


#4 N-TETRADECANE

R.T.: 8.033 min
Delta R.T.: -0.024 min
Response: 2788338
Conc: 19.18 ug/ml

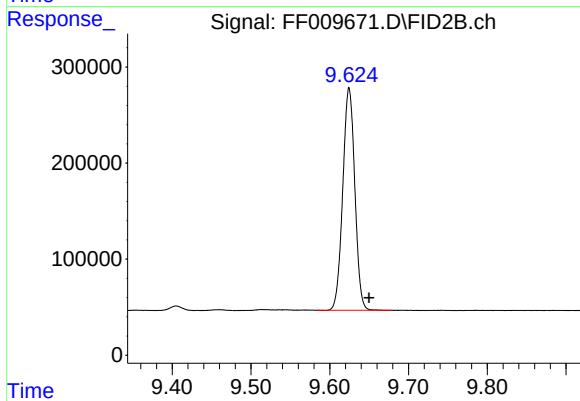

#5 N-HEXADECANE


R.T.: 9.625 min
Delta R.T.: -0.025 min
Response: 2460497
Conc: 17.13 ug/ml

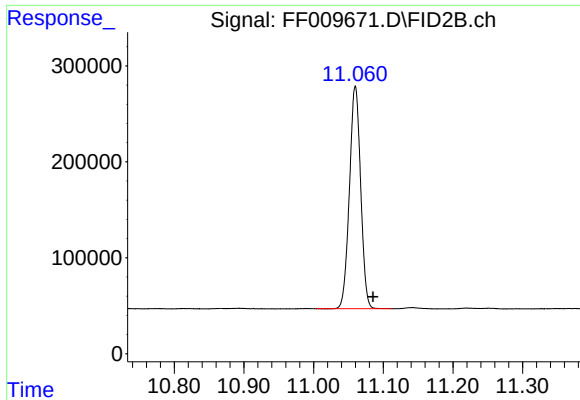

#6 N-OCTADECANE


R.T.: 11.060 min
Delta R.T.: -0.025 min
Response: 2593011
Conc: 17.97 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-6-(4.5-5)MSD

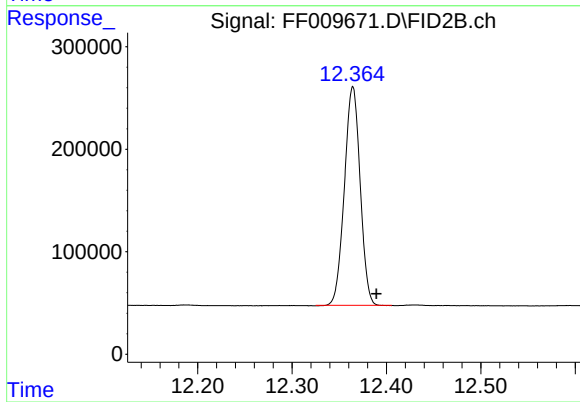


#7 N-EICOSANE

R.T.: 12.364 min
Delta R.T.: -0.025 min
Response: 2474882
Conc: 17.46 ug/ml

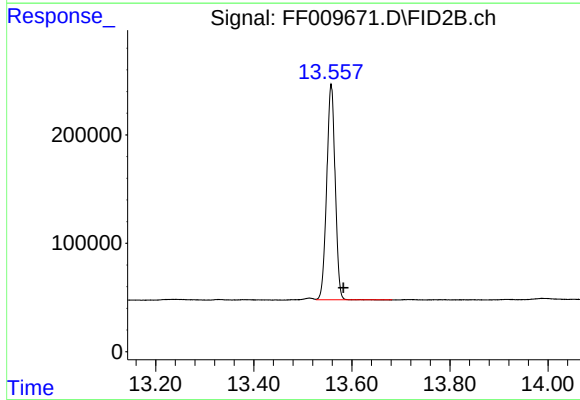


#8 N-DOCOSANE

R.T.: 13.558 min
Delta R.T.: -0.025 min
Response: 2383353
Conc: 17.49 ug/ml

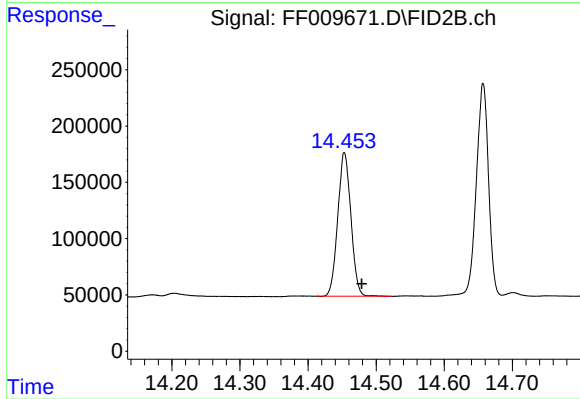

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.453 min
Delta R.T.: -0.026 min
Response: 1707082
Conc: 14.74 ug/ml

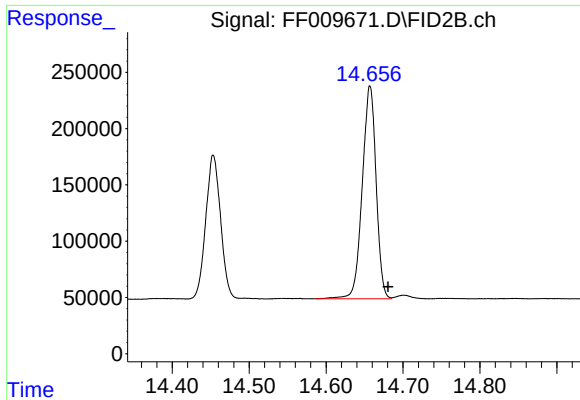

#10 N-TETRACOSANE


R.T.: 14.657 min
Delta R.T.: -0.024 min
Response: 2363827
Conc: 17.95 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-6-(4.5-5)MSD

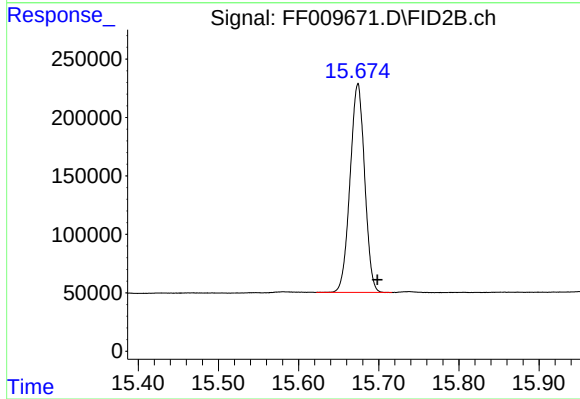

#11 N-HEXACOSANE

R.T.: 15.674 min
Delta R.T.: -0.024 min
Response: 2252253
Conc: 18.02 ug/ml

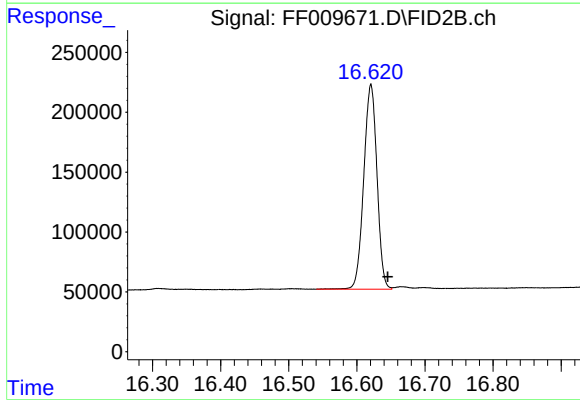

#12 N-OCTACOSANE

R.T.: 16.621 min
Delta R.T.: -0.024 min
Response: 2299818
Conc: 19.31 ug/ml