

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011023\
 Data File : FF011849.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jan 2023 14:01
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 11 04:52:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
 Quant Title :
 QLast Update : Mon Jan 02 03:26:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.765	3239145	20.123 ug/ml
12) N-OCTACOSANE	17.218	3509985	20.291 ug/ml
13) N-TRIACONTANE	18.104	142236	0.850 ug/ml
14) N-DOTRIACONTANE	18.936	183600	1.134 ug/ml
15) N-TETRATRIACONTANE	19.718	133014	0.892 ug/ml
16) N-HEXATRIACONTANE	20.457	78063	0.582 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011023\
 Data File : FF011849.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jan 2023 14:01
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 11 04:52:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
 Quant Title :
 QLast Update : Mon Jan 02 03:26:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

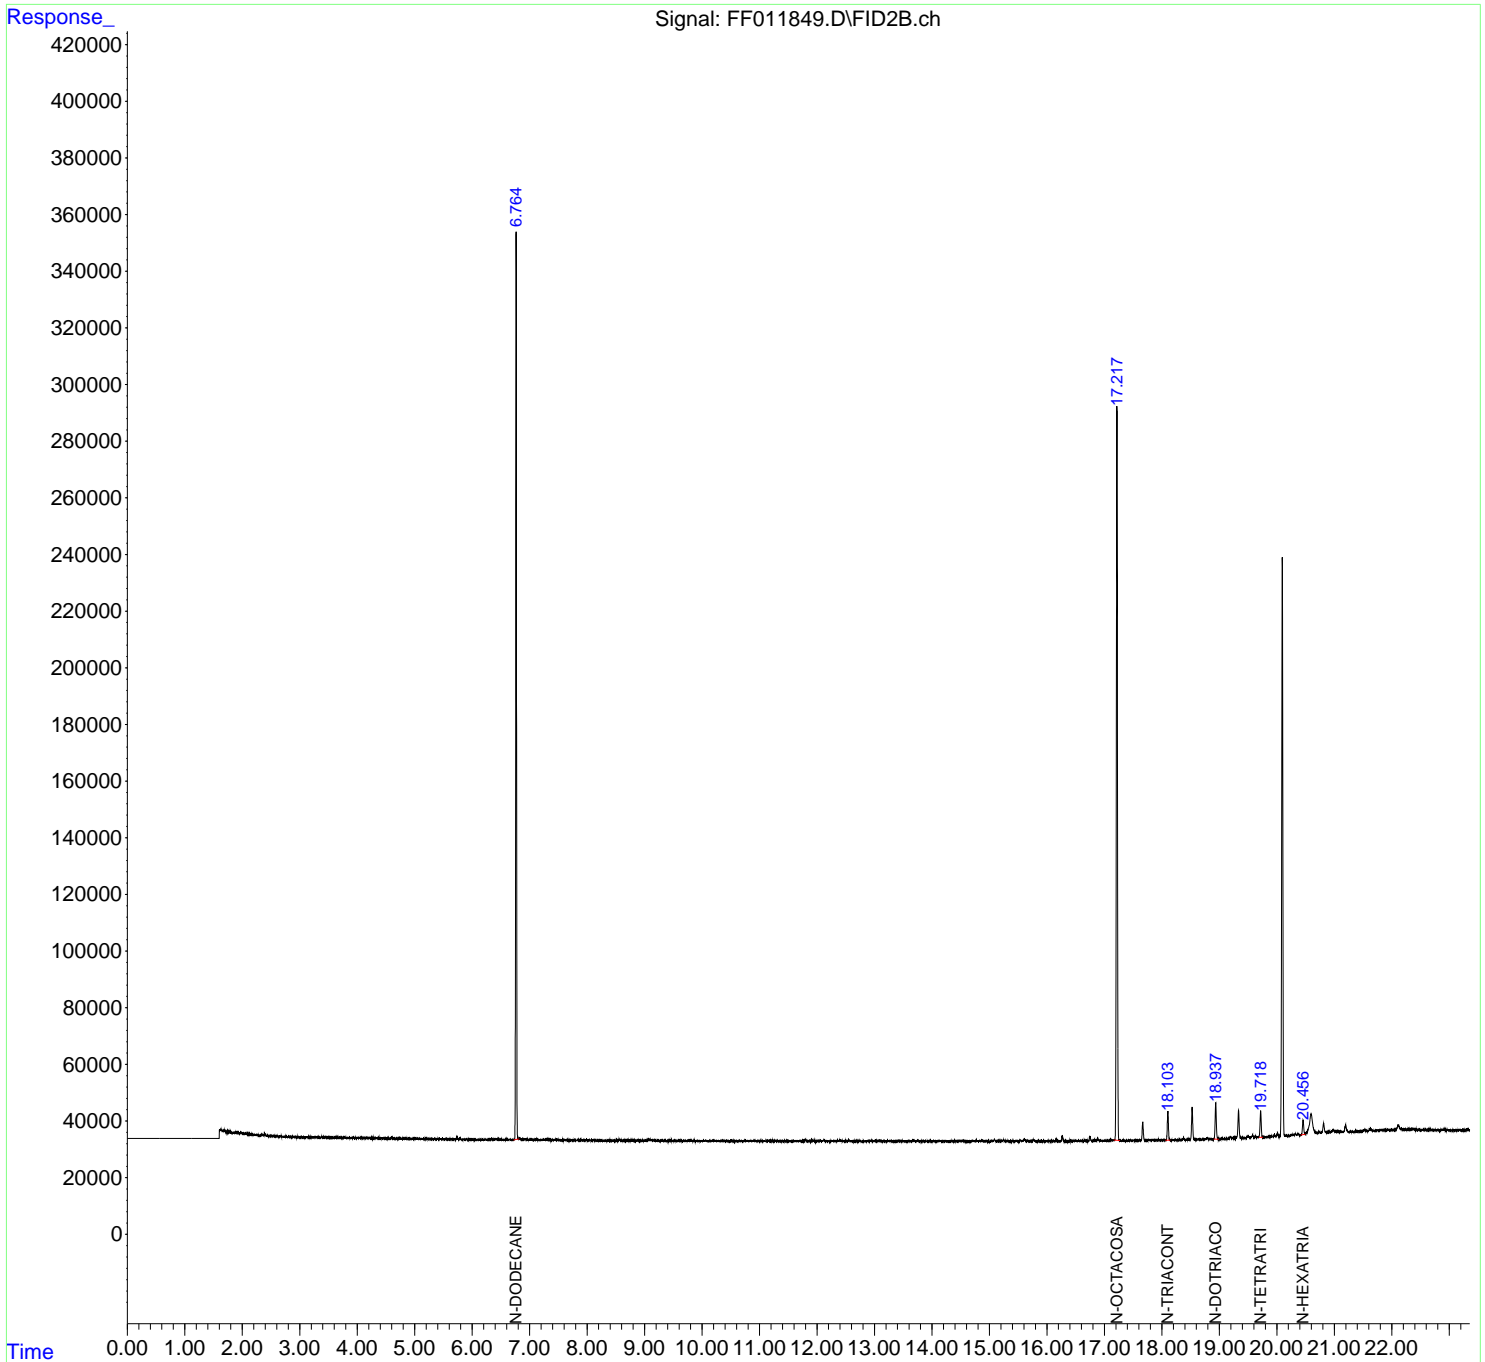


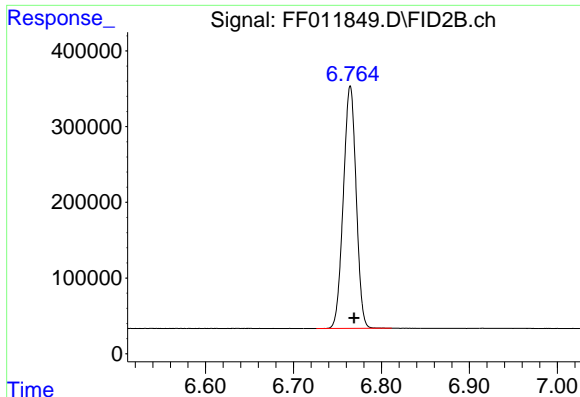

#3 N-DODECANE


R.T.: 6.765 min
 Delta R.T.: -0.004 min
 Response: 3239145
 Conc: 20.12 ug/ml

Instrument :
 FID_F
 ClientSampleId :

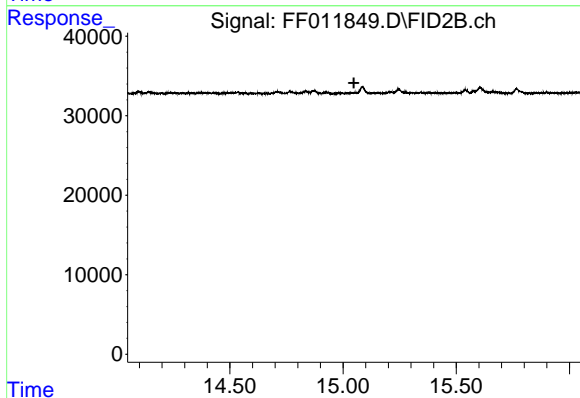


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
 Exp R.T. : 15.048 min
 Response: 0
 Conc: N.D.

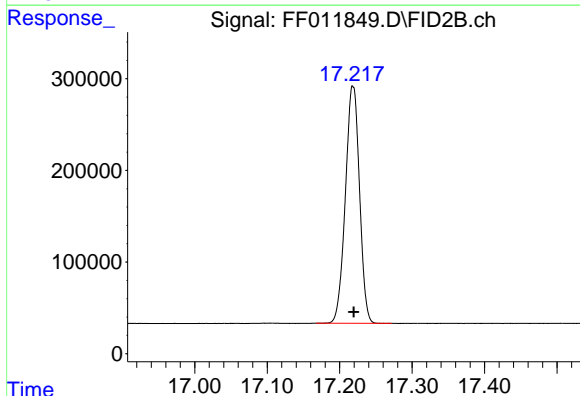


#12 N-OCTACOSANE

R.T.: 17.218 min
 Delta R.T.: -0.001 min
 Response: 3509985
 Conc: 20.29 ug/ml

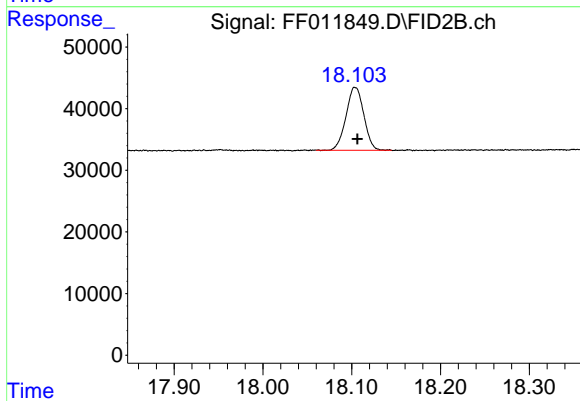

#13 N-TRIACONTANE


R.T.: 18.104 min
 Delta R.T.: -0.003 min
 Response: 142236
 Conc: 0.85 ug/ml

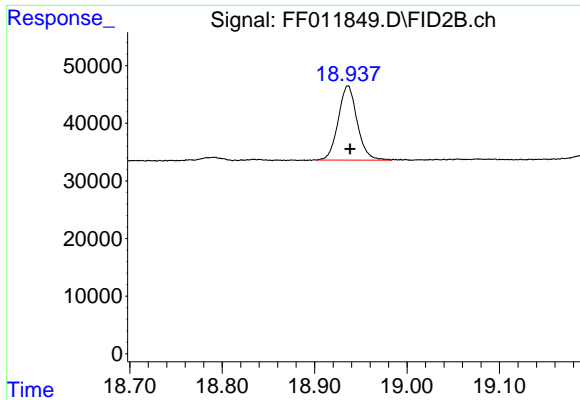

#14 N-DOTRIACONTANE


R.T.: 18.936 min
 Delta R.T.: -0.002 min
 Response: 183600
 Conc: 1.13 ug/ml

Instrument :
 FID_F
 ClientSampleId :

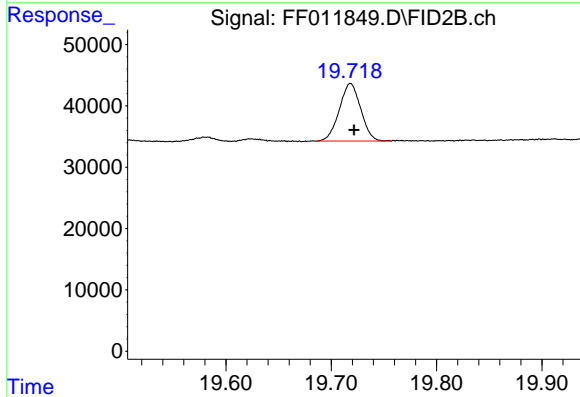

#15 N-TETRATRIACONTANE

R.T.: 19.718 min
 Delta R.T.: -0.004 min
 Response: 133014
 Conc: 0.89 ug/ml

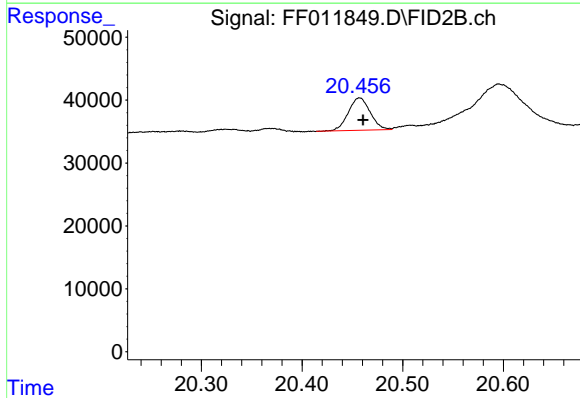

#16 N-HEXATRIACONTANE

R.T.: 20.457 min
 Delta R.T.: -0.003 min
 Response: 78063
 Conc: 0.58 ug/ml