

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011023\
 Data File : FF011852.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jan 2023 15:32
 Operator : YP\AJ
 Sample : 01080-02
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 11 04:52:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
 Quant Title :
 QLast Update : Mon Jan 02 03:26:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.044	1626745	10.292 ug/ml
Target Compounds			
3) N-DODECANE	6.785	121633	0.756 ug/ml
4) N-TETRADECANE	8.588	222022	1.350 ug/ml
6) N-OCTADECANE	11.653	66458	0.376 ug/ml
10) N-TETRACOSANE	15.247	51043	0.283 ug/ml
11) N-HEXACOSANE	16.267	51141	0.287 ug/ml
12) N-OCTACOSANE	17.217	55755	0.322 ug/ml
13) N-TRIACONTANE	18.102	65950	0.394 ug/ml
14) N-DOTRIACONTANE	18.930	76445	0.472 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011023\
Data File : FF011852.D
Signal(s) : FID2B.ch
Acq On : 10 Jan 2023 15:32
Operator : YP\AJ
Sample : 01080-02
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 11 04:52:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

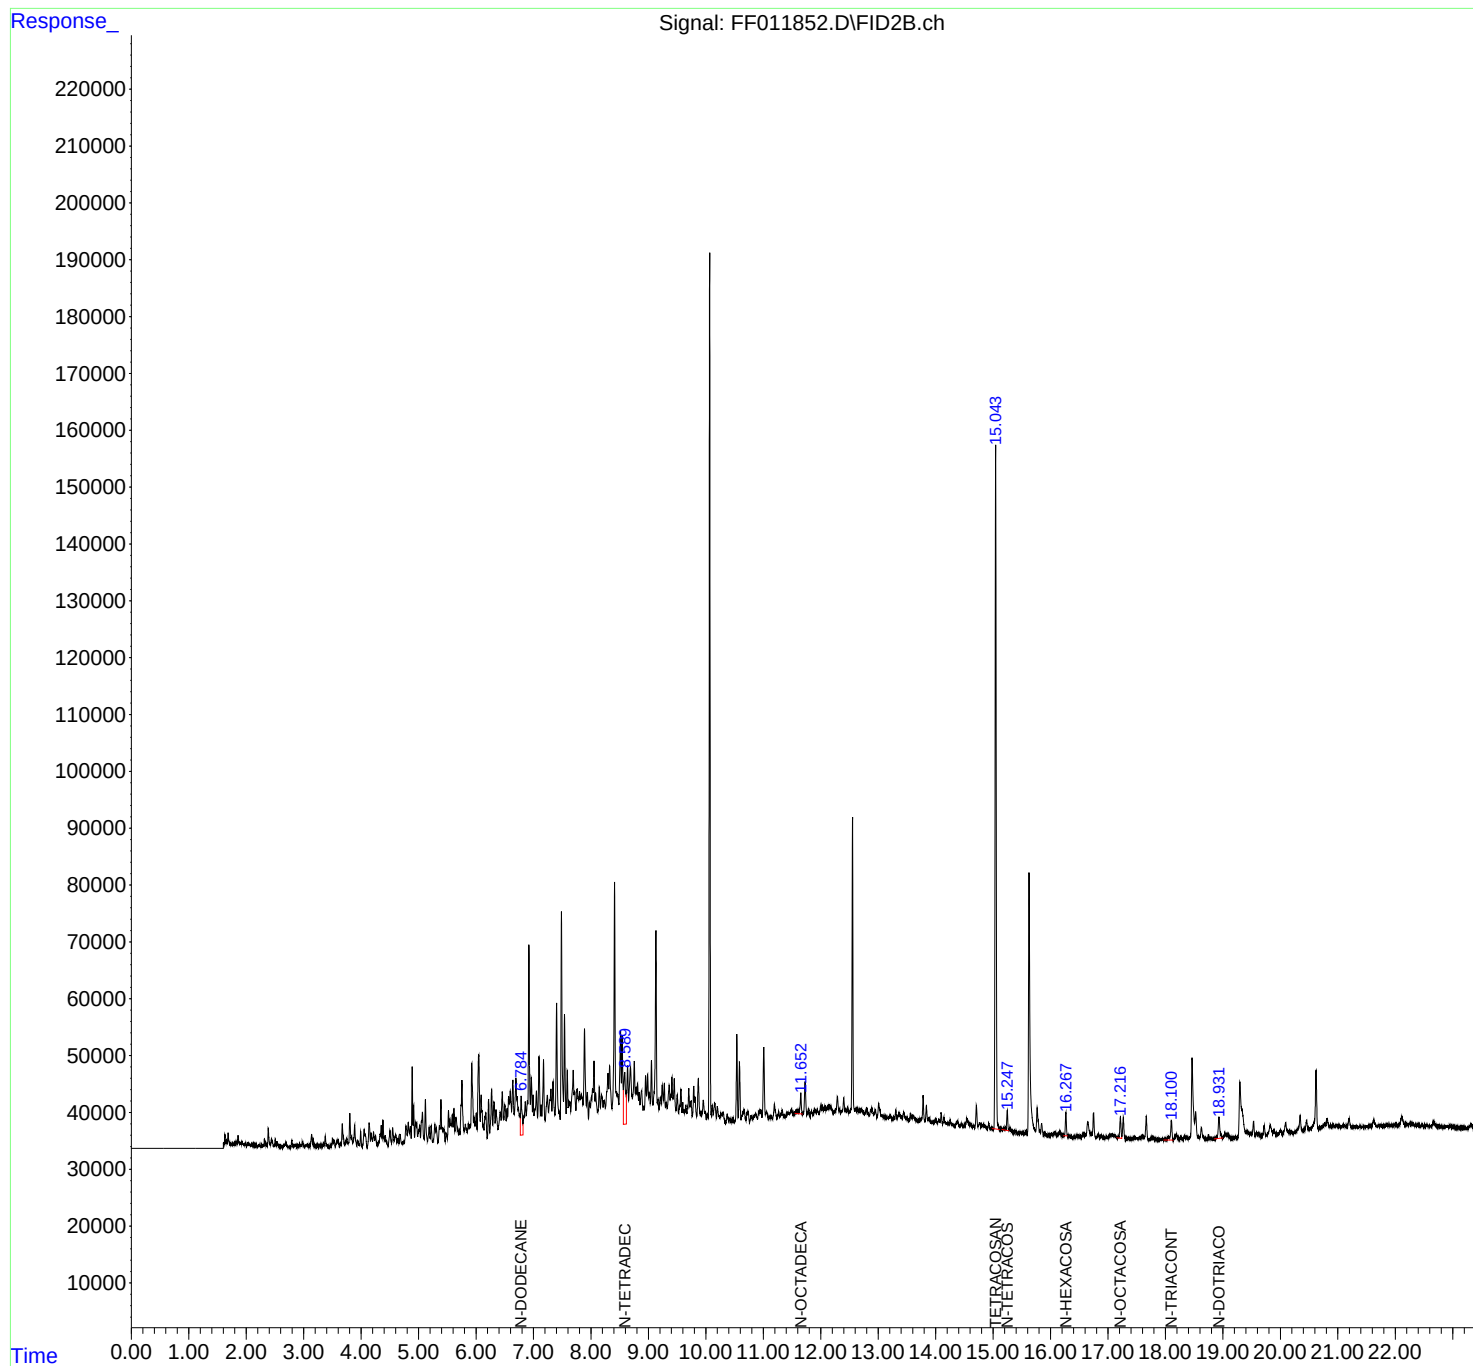


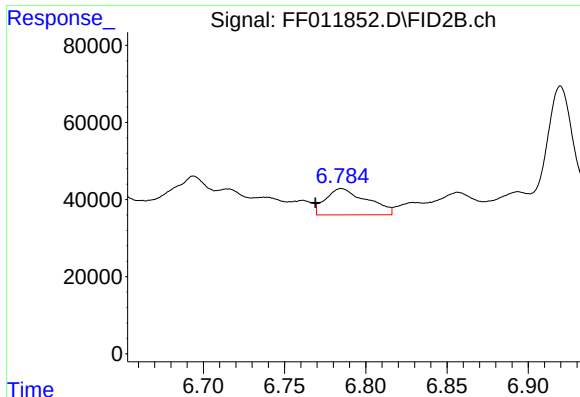

#3 N-DODECANE


R.T.: 6.785 min
Delta R.T.: 0.016 min
Response: 121633
Conc: 0.76 ug/ml

Instrument :
FID_F
ClientSampleId :

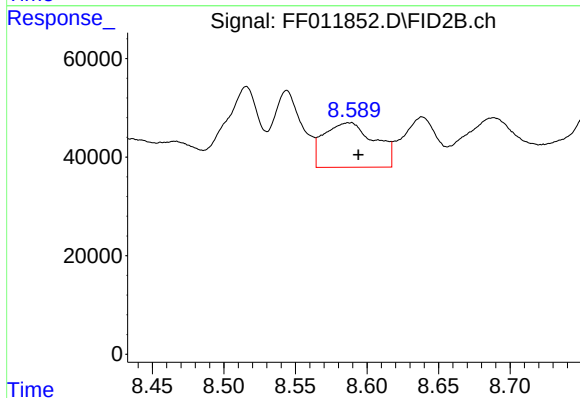


#4 N-TETRADECANE

R.T.: 8.588 min
Delta R.T.: -0.006 min
Response: 222022
Conc: 1.35 ug/ml

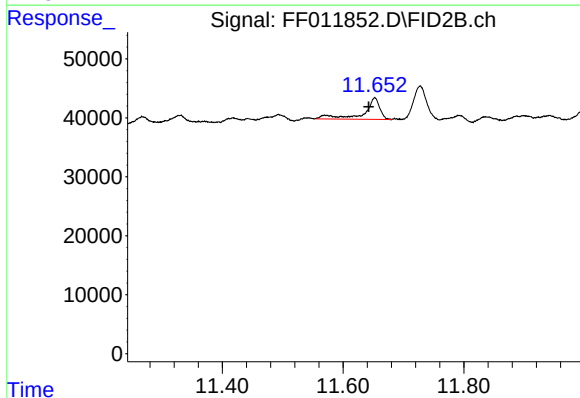


#6 N-OCTADECANE

R.T.: 11.653 min
Delta R.T.: 0.010 min
Response: 66458
Conc: 0.38 ug/ml

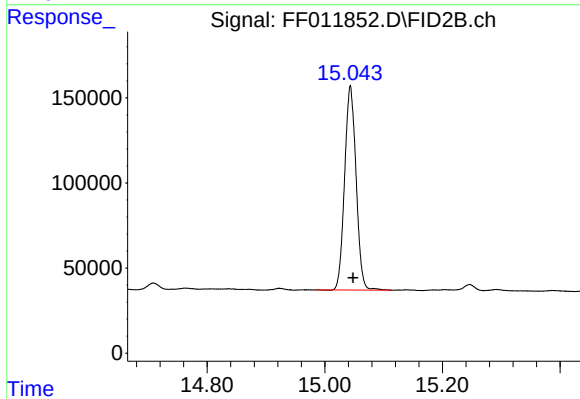

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.044 min
Delta R.T.: -0.004 min
Response: 1626745
Conc: 10.29 ug/ml

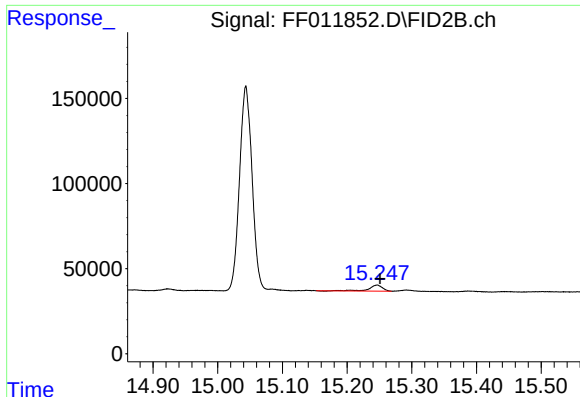

#10 N-TETRACOSANE


R.T.: 15.247 min
Delta R.T.: -0.004 min
Response: 51043
Conc: 0.28 ug/ml

Instrument :
FID_F
ClientSampleId :

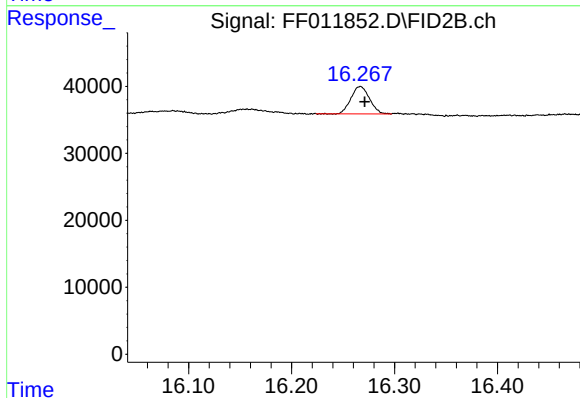


#11 N-HEXACOSANE

R.T.: 16.267 min
Delta R.T.: -0.004 min
Response: 51141
Conc: 0.29 ug/ml

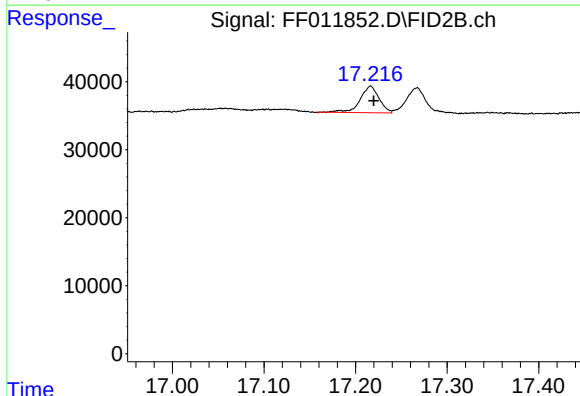


#12 N-OCTACOSANE

R.T.: 17.217 min
Delta R.T.: -0.003 min
Response: 55755
Conc: 0.32 ug/ml

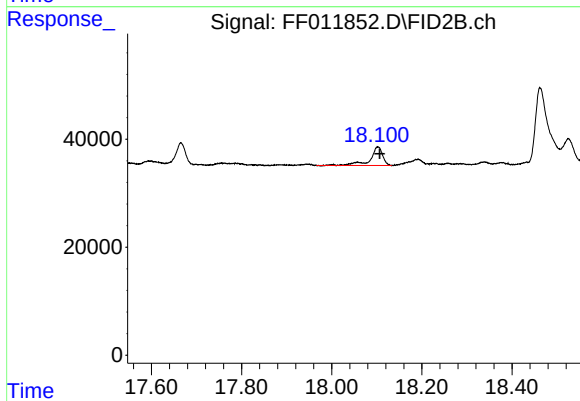

#13 N-TRIACONTANE

R.T.: 18.102 min
Delta R.T.: -0.004 min
Response: 65950
Conc: 0.39 ug/ml

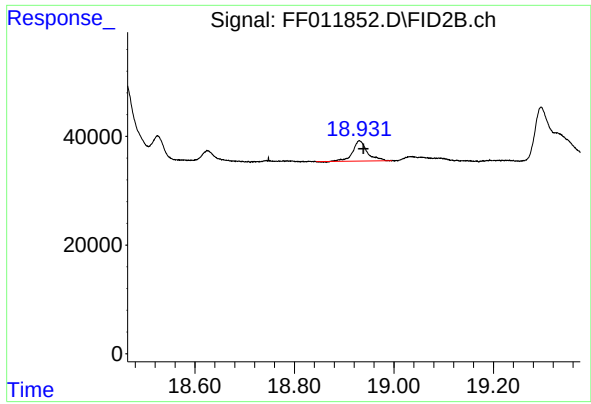

#14 N-DOTRIACONTANE

R.T.: 18.930 min
Delta R.T.: -0.008 min
Response: 76445
Conc: 0.47 ug/ml

Instrument :

FID_F

ClientSampleId :