

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011023\
 Data File : FF011855.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jan 2023 17:00
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 11 04:52:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
 Quant Title :
 QLast Update : Mon Jan 02 03:26:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.044	2546356	16.111 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.103	61465	0.367 ug/ml
14) N-DOTRIACONTANE	18.935	84783	0.524 ug/ml
15) N-TETRATRIACONTANE	19.717	52658	0.353 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011023\
Data File : FF011855.D
Signal(s) : FID2B.ch
Acq On : 10 Jan 2023 17:00
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 11 04:52:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

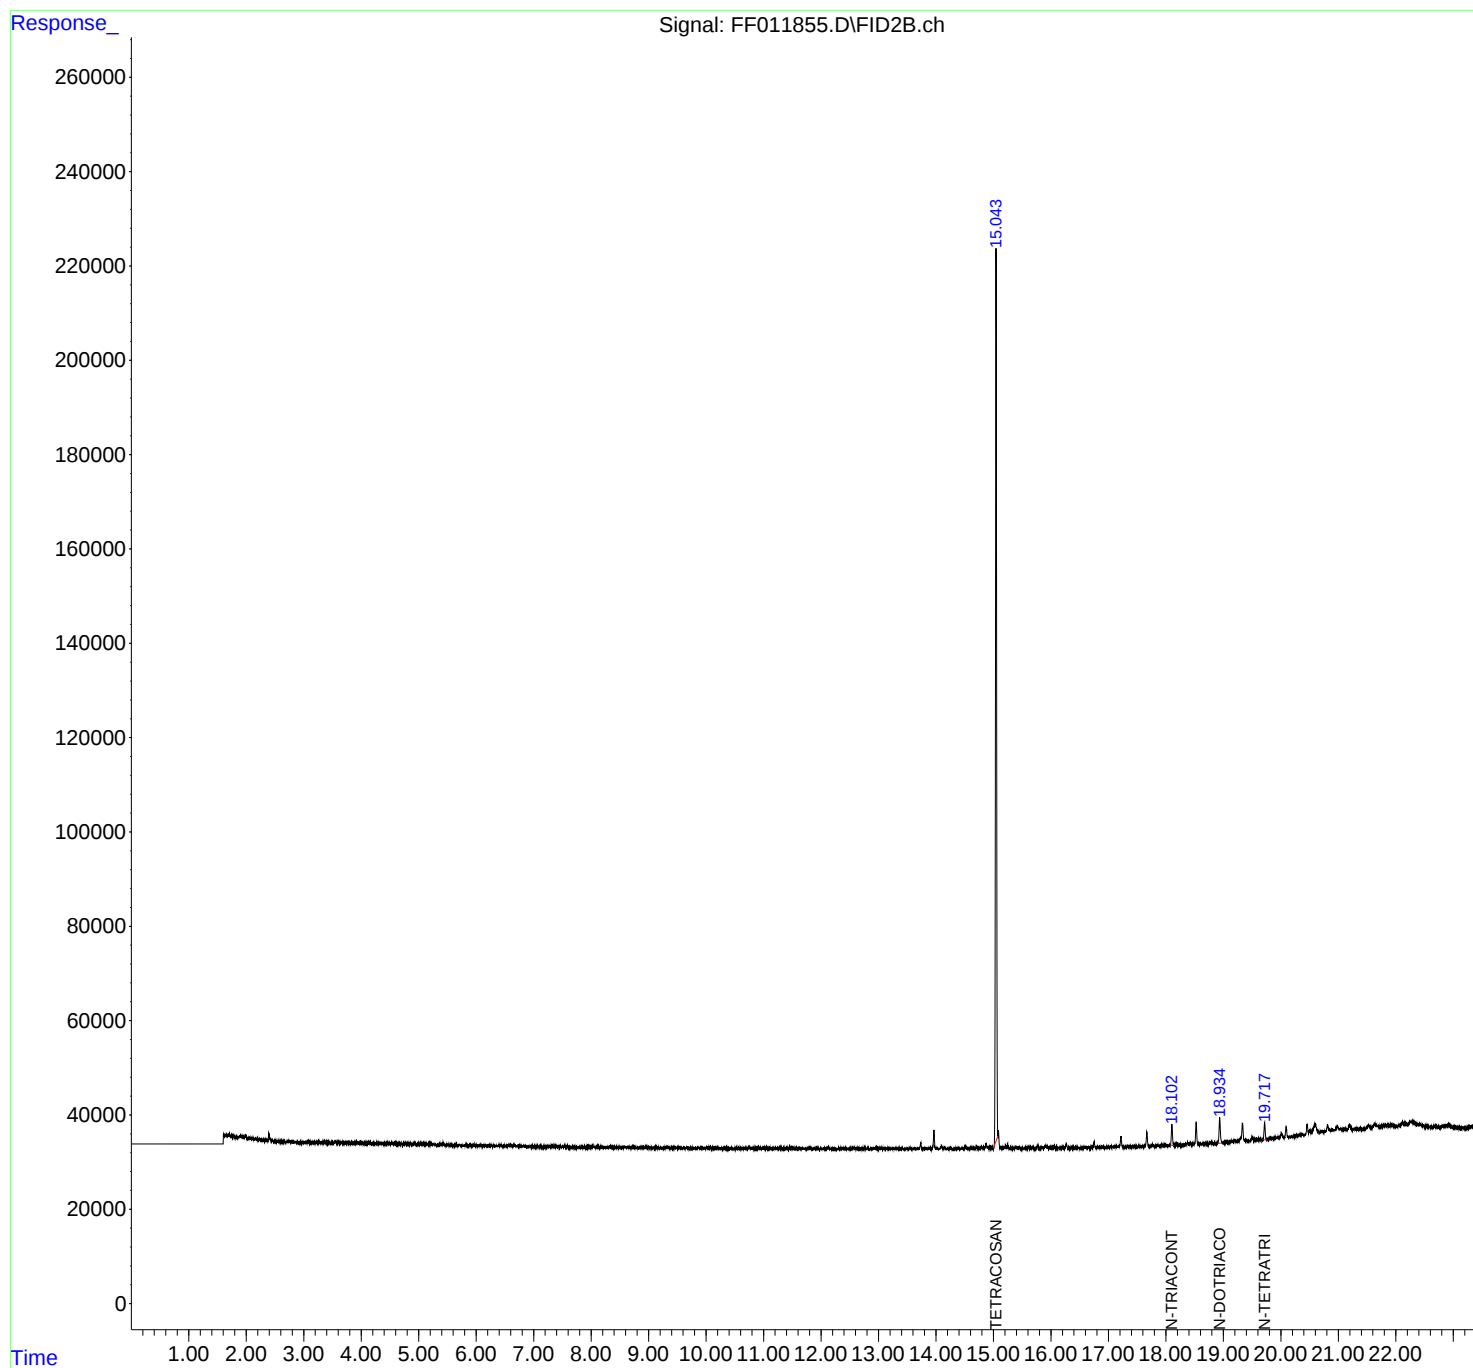


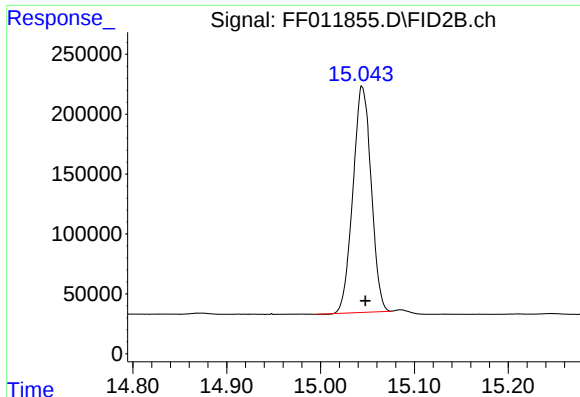

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.044 min
Delta R.T.: -0.004 min
Response: 2546356
Conc: 16.11 ug/ml

Instrument :
FID_F
ClientSampleId :

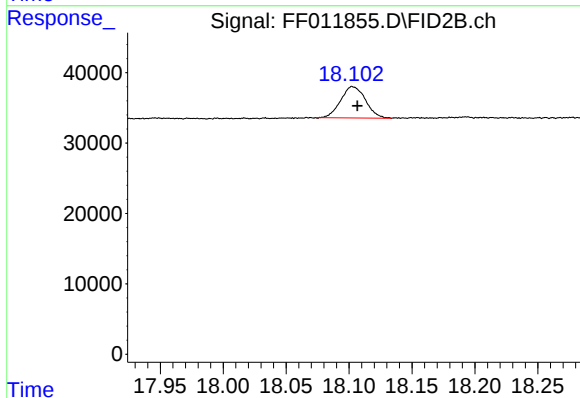


#13 N-TRIACONTANE

R.T.: 18.103 min
Delta R.T.: -0.004 min
Response: 61465
Conc: 0.37 ug/ml

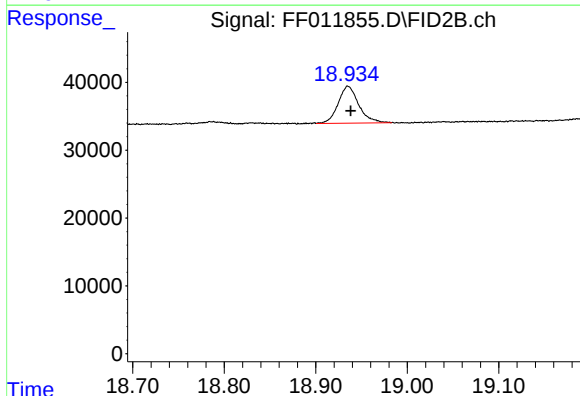

#14 N-DOTRIACONTANE

R.T.: 18.935 min
Delta R.T.: -0.003 min
Response: 84783
Conc: 0.52 ug/ml

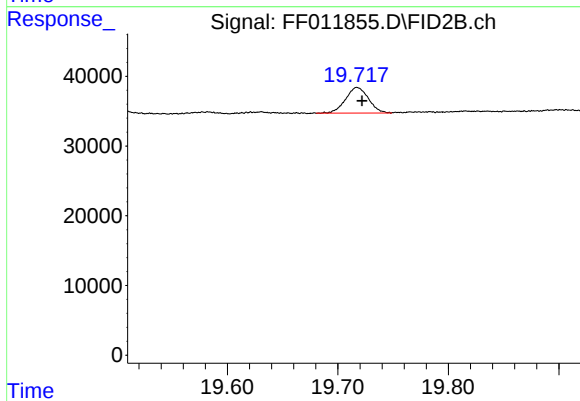

#15 N-TETRATRIACONTANE

R.T.: 19.717 min
Delta R.T.: -0.004 min
Response: 52658
Conc: 0.35 ug/ml