

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF011023\  
 Data File : FF011864.D  
 Signal(s) : FID2B.ch  
 Acq On : 10 Jan 2023 22:24  
 Operator : YP\AJ  
 Sample : 01076-01 10X  
 Misc :  
 ALS Vial : 73 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jan 11 04:55:03 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF123022.M  
 Quant Title :  
 QLast Update : Mon Jan 02 03:26:15 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.    | Response | Conc Units  |
|-------------------------------|---------|----------|-------------|
| -----                         |         |          |             |
| System Monitoring Compounds   |         |          |             |
| 9) S TETRACOSANE-d50 (SURR... | 15.047  | 163099   | 1.032 ug/ml |
| Target Compounds              |         |          |             |
| 7) N-EICOSANE                 | 13.013f | 66317    | 0.373 ug/ml |
| 14) N-DOTRIACONTANE           | 18.940  | 41984    | 0.259 ug/ml |
| 15) N-TETRATRIACONTANE        | 19.726  | 10973    | 0.074 ug/ml |
| 17) N-OCTATRIACONTANE         | 21.149f | 713467   | 5.504 ug/ml |
| -----                         |         |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF011023\  
Data File : FF011864.D  
Signal(s) : FID2B.ch  
Acq On : 10 Jan 2023 22:24  
Operator : YP\AJ  
Sample : 01076-01 10X  
Misc :  
ALS Vial : 73 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jan 11 04:55:03 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF123022.M  
Quant Title :  
QLast Update : Mon Jan 02 03:26:15 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

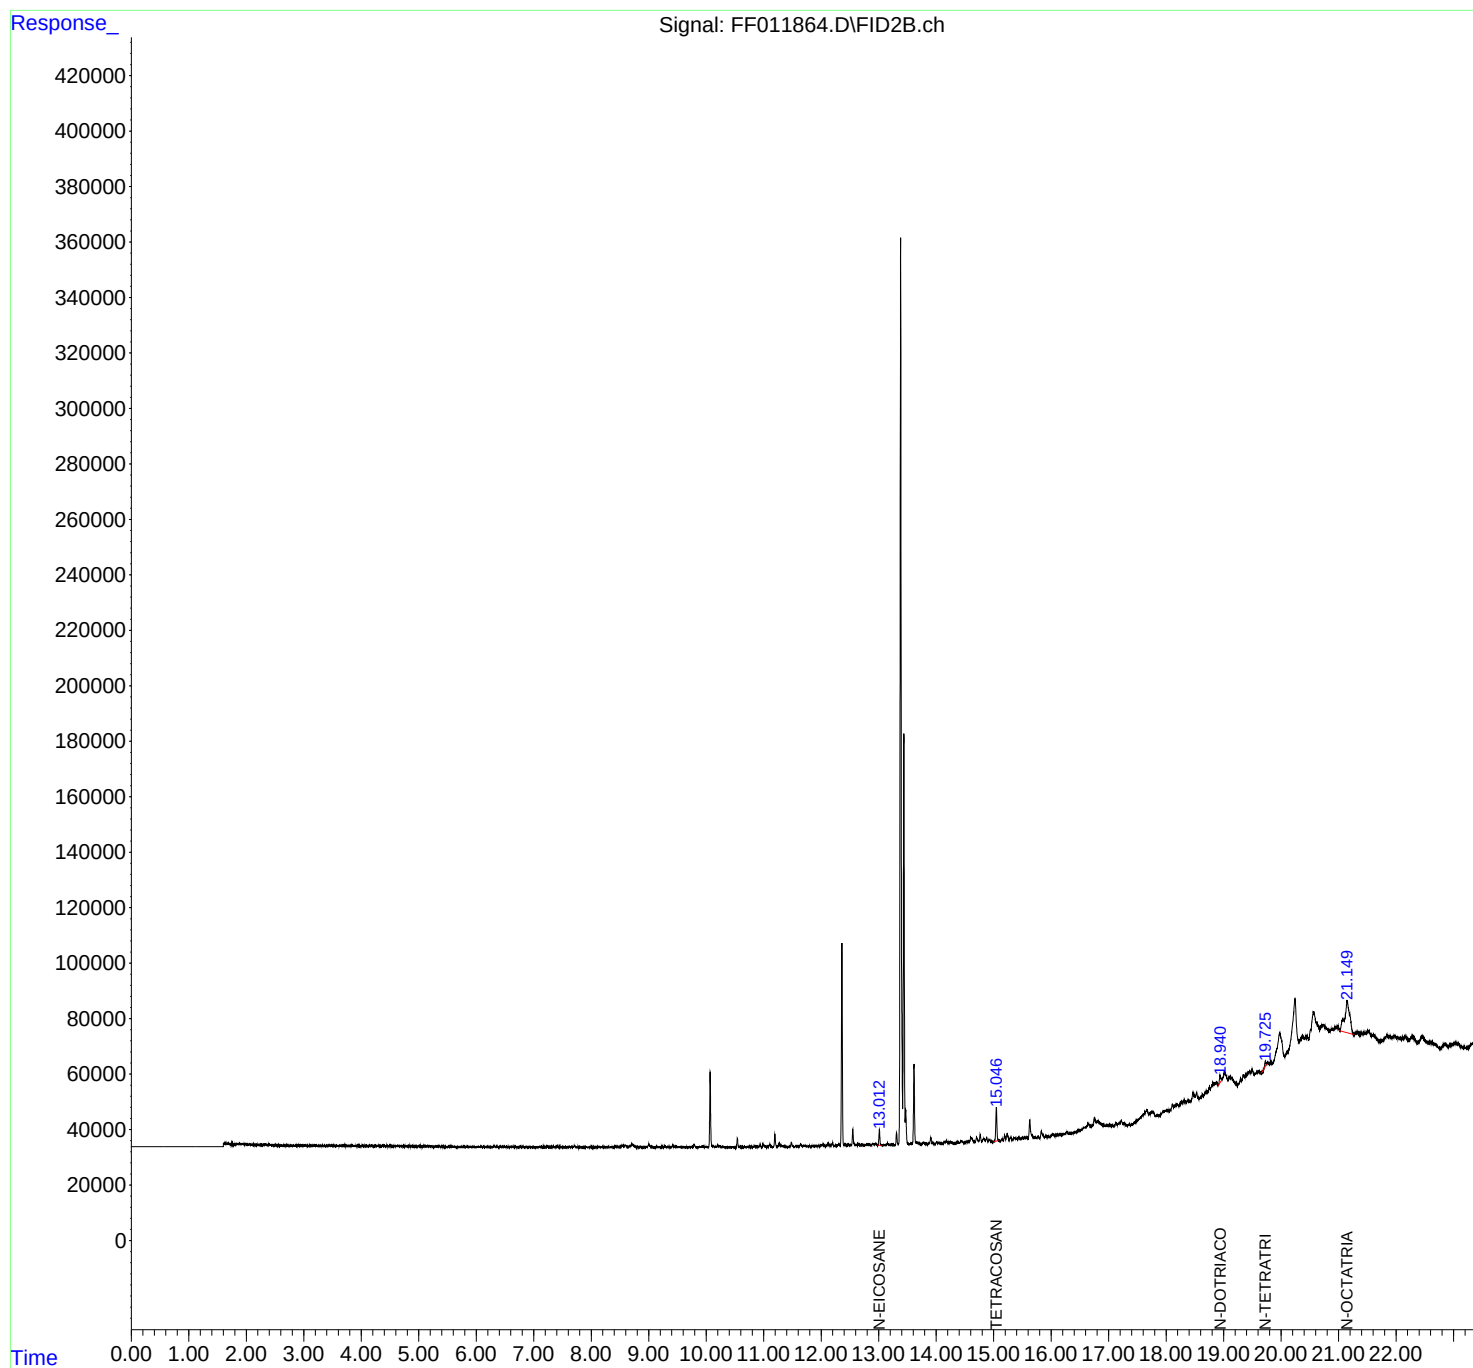


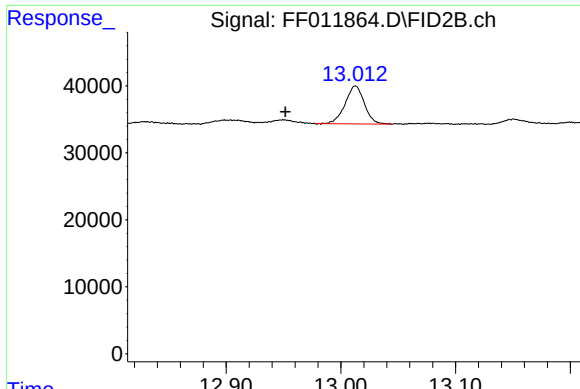

#7 N-EICOSANE


R.T.: 13.013 min  
Delta R.T.: 0.061 min  
Response: 66317  
Conc: 0.37 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

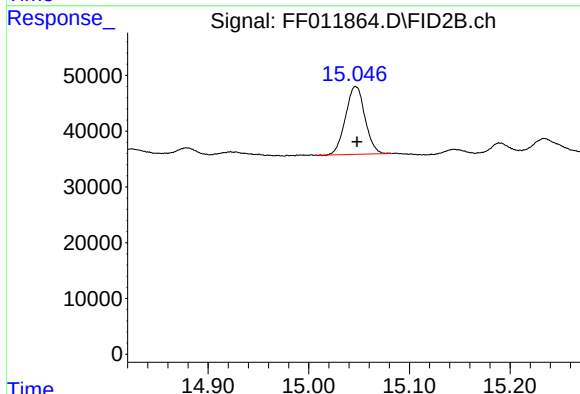


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.047 min  
Delta R.T.: -0.001 min  
Response: 163099  
Conc: 1.03 ug/ml

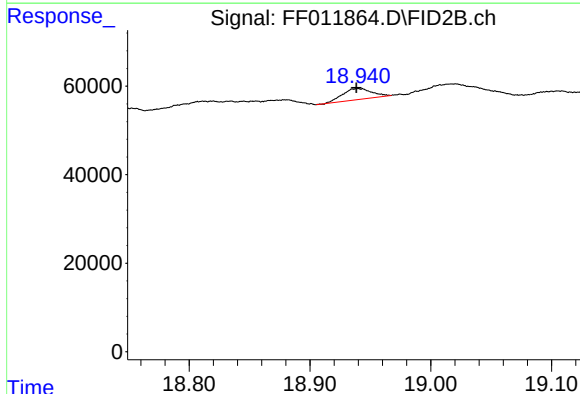


#14 N-DOTRIACONTANE

R.T.: 18.940 min  
Delta R.T.: 0.002 min  
Response: 41984  
Conc: 0.26 ug/ml

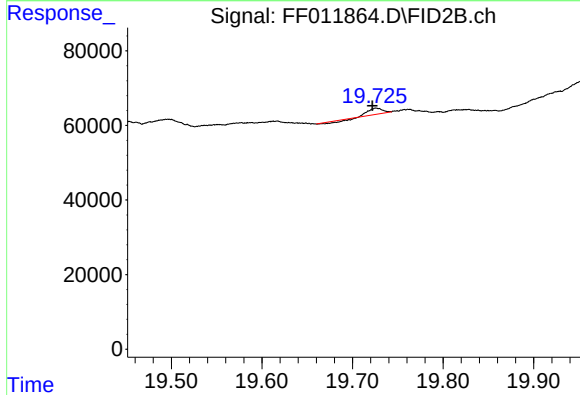

#15 N-TETRATRIACONTANE

R.T.: 19.726 min  
Delta R.T.: 0.004 min  
Response: 10973  
Conc: 0.07 ug/ml

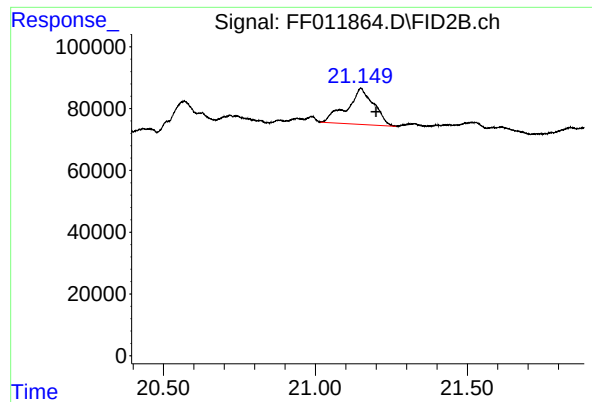

#17 N-OCTATRIACONTANE

R.T.: 21.149 min  
Delta R.T.: -0.051 min  
Response: 713467  
Conc: 5.50 ug/ml

Instrument :

FID\_F

ClientSampleId :