

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011023\
Data File : FF011863.D
Signal(s) : FID2B.ch
Acq On : 10 Jan 2023 21:55
Operator : YP\AJ
Sample : 01080-05 10X
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
B-3-(15-17)

Integration File: autoint1.e
Quant Time: Jan 11 04:54:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.065	986885	6.244 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011023\
Data File : FF011863.D
Signal(s) : FID2B.ch
Acq On : 10 Jan 2023 21:55
Operator : YP\AJ
Sample : 01080-05 10X
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
B-3-(15-17)

Integration File: autoint1.e
Quant Time: Jan 11 04:54:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

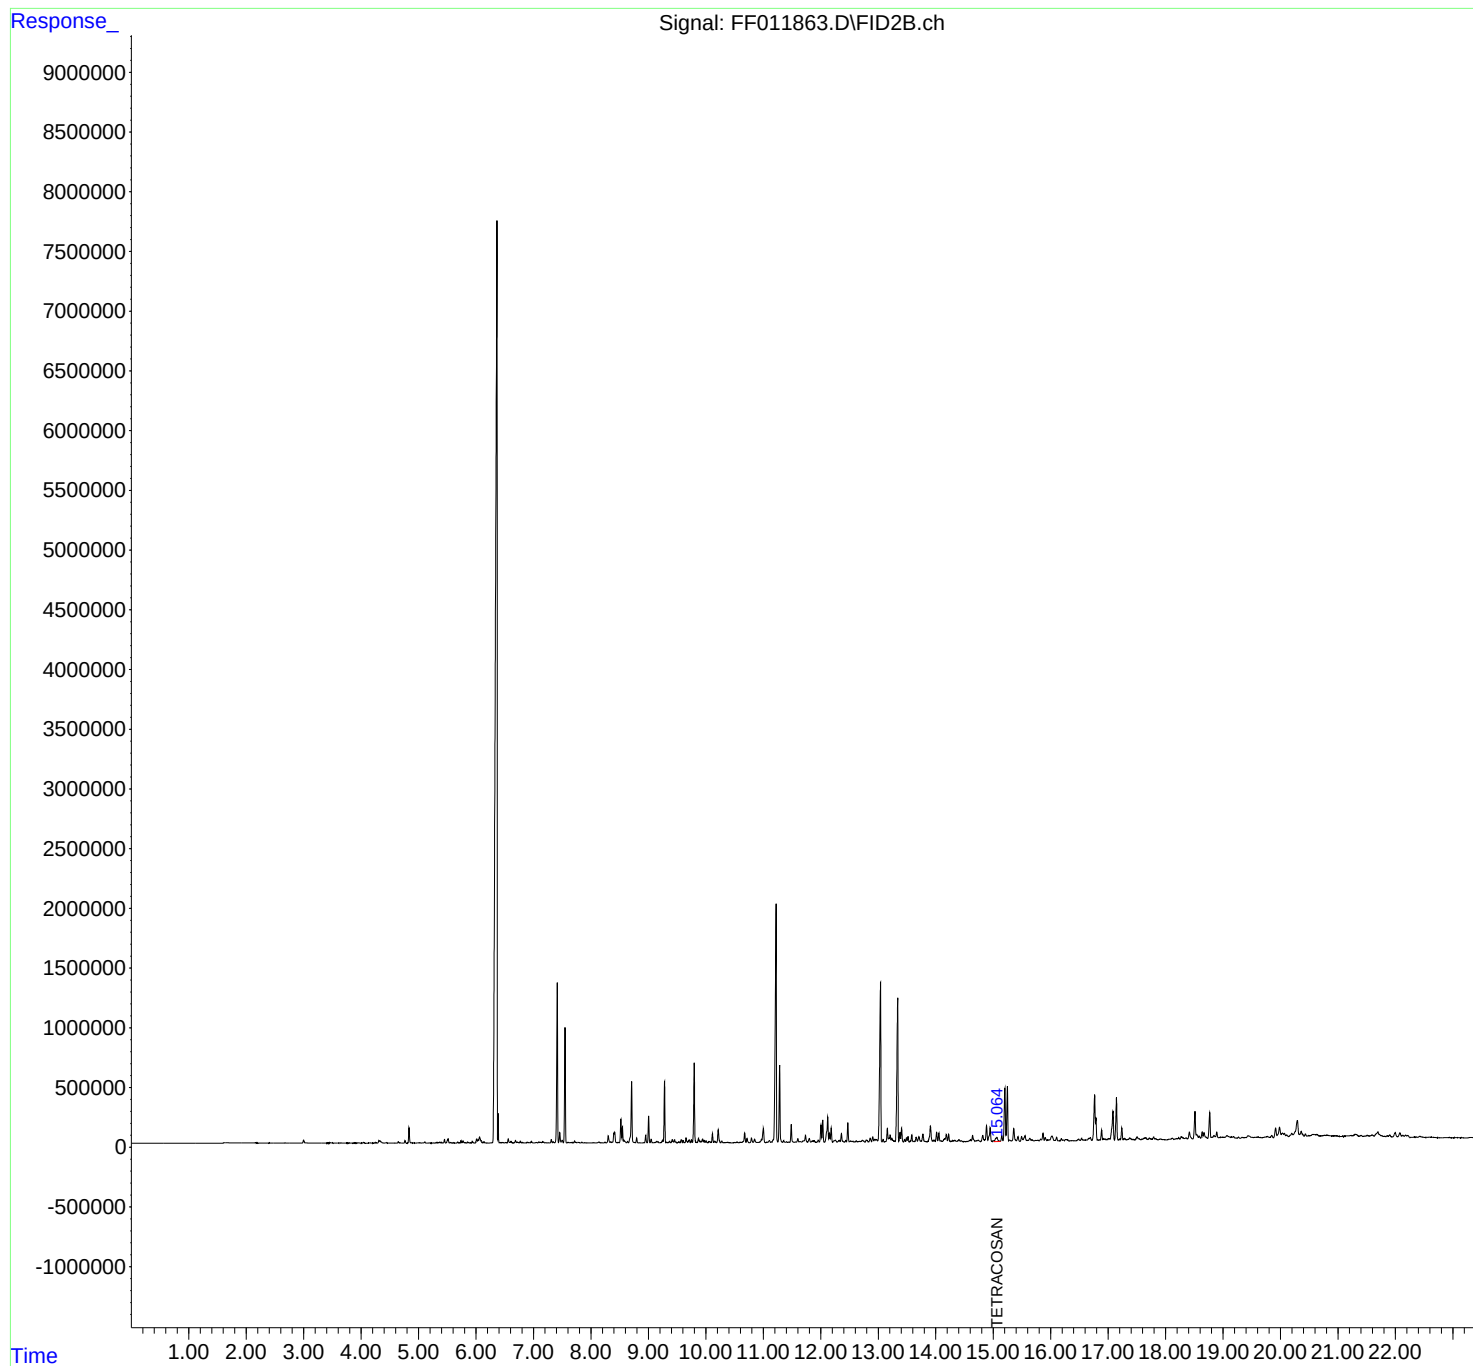

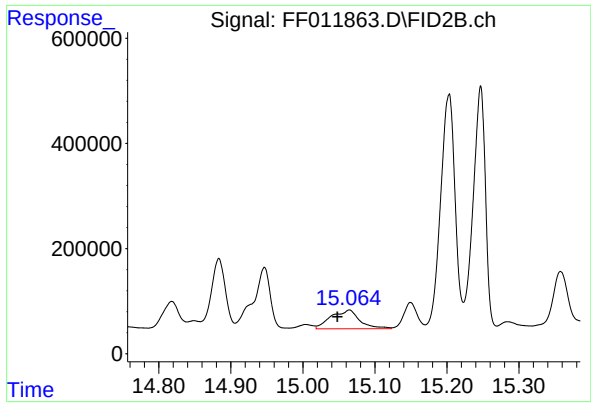

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.065 min
Delta R.T.: 0.017 min
Response: 986885
Conc: 6.24 ug/ml

Instrument :
FID_F
ClientSampleId :
B-3-(15-17)