

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011119\
 Data File : FF003223.D
 Signal(s) : FID2B.ch
 Acq On : 11 Jan 2019 10:04
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 11 22:16:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.612	6212589	46.730 ug/ml
Target Compounds			
2) N-DECANE	4.352	8514034	56.697 ug/ml
3) N-DODECANE	6.371	8371612	55.318 ug/ml
4) N-TETRADECANE	8.162	8157613	53.509 ug/ml
5) N-HEXADECANE	9.761	7955797	51.896 ug/ml
6) N-OCTADECANE	11.202	7708155	50.115 ug/ml
7) N-EICOSANE	12.513	7388517	48.522 ug/ml
8) N-DOCOSANE	13.712	7121199	47.236 ug/ml
10) N-TETRACOSANE	14.817	6919705	46.440 ug/ml
11) N-HEXACOSANE	15.840	6834957	46.455 ug/ml
12) N-OCTACOSANE	16.792	6915987	47.520 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011119\
Data File : FF003223.D
Signal(s) : FID2B.ch
Acq On : 11 Jan 2019 10:04
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 11 22:16:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

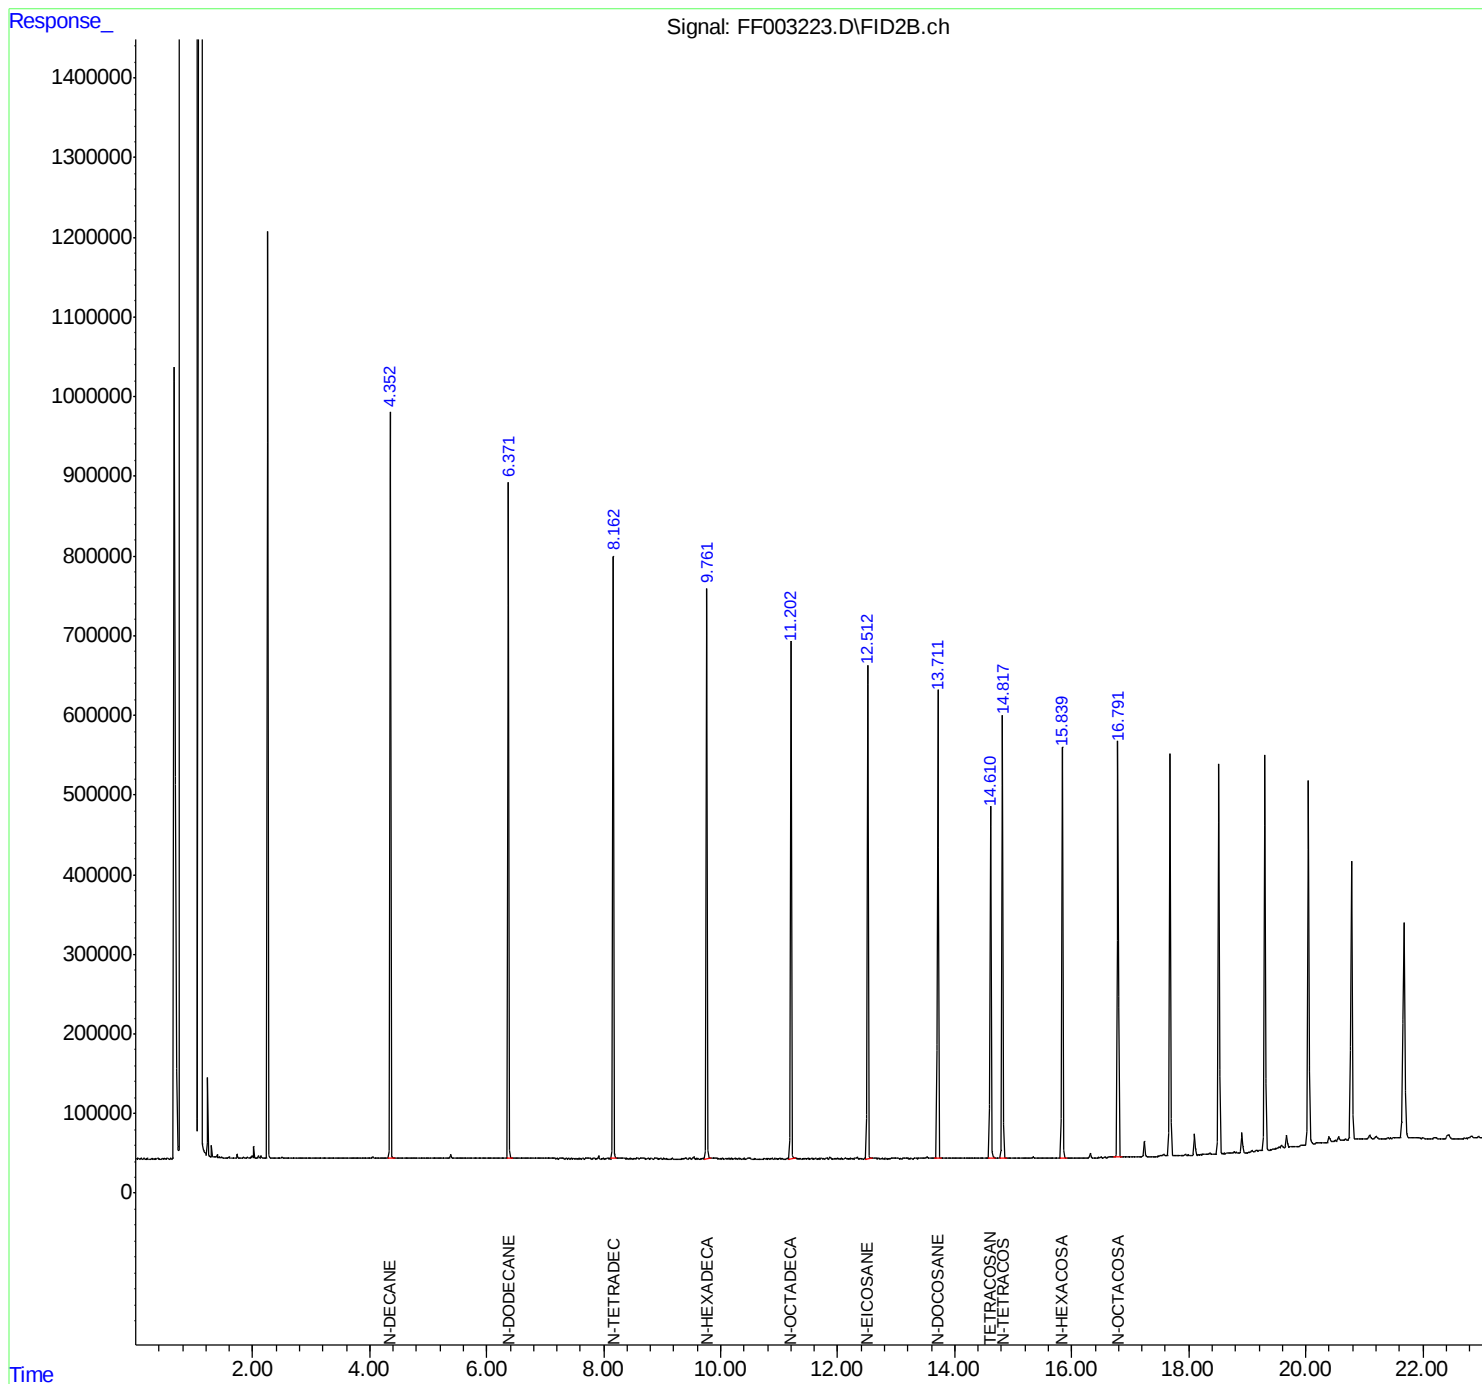

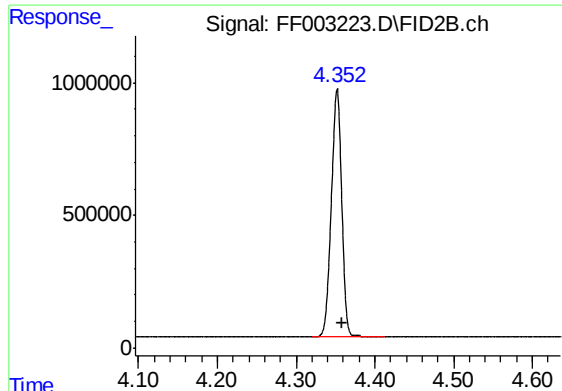


#2 N-DECANE

R.T.: 4.352 min
Delta R.T.: -0.006 min
Response: 8514034
Conc: 56.70 ug/ml

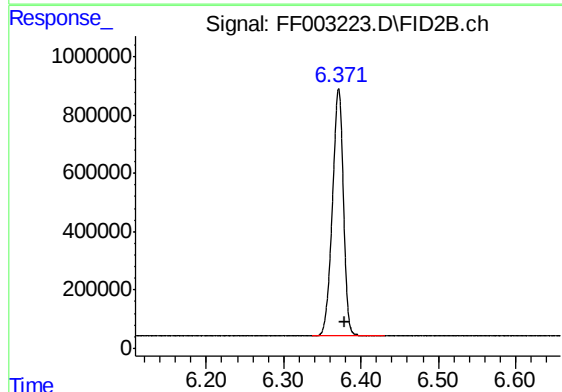


#3 N-DODECANE

R.T.: 6.371 min
Delta R.T.: -0.009 min
Response: 8371612
Conc: 55.32 ug/ml

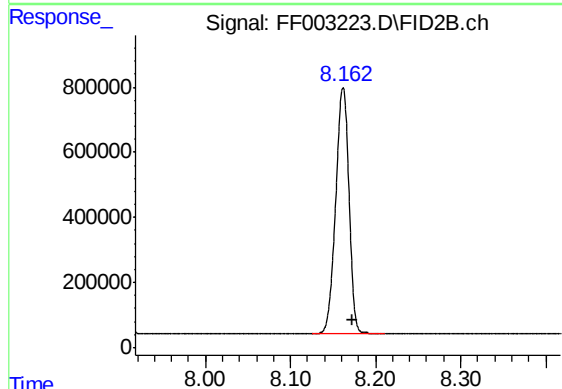


#4 N-TETRADECANE

R.T.: 8.162 min
Delta R.T.: -0.012 min
Response: 8157613
Conc: 53.51 ug/ml

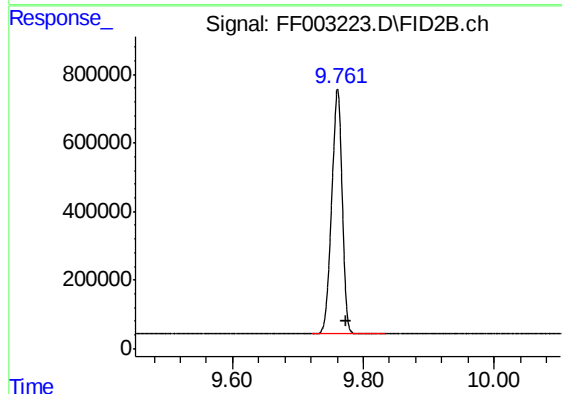


#5 N-HEXADECANE

R.T.: 9.761 min
Delta R.T.: -0.013 min
Response: 7955797
Conc: 51.90 ug/ml

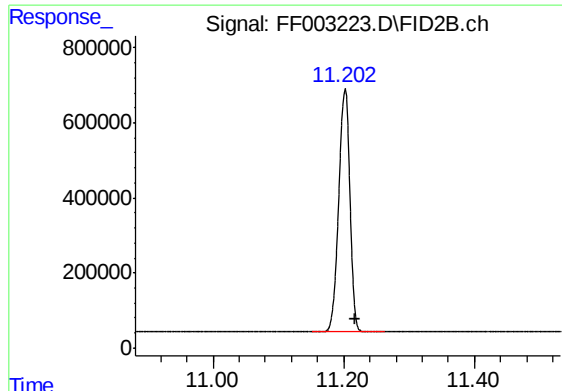


#6 N-OCTADECANE

R.T.: 11.202 min
Delta R.T.: -0.014 min
Response: 7708155
Conc: 50.12 ug/ml

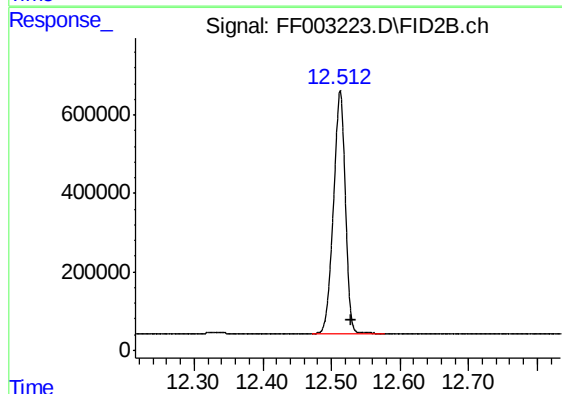


#7 N-EICOSANE

R.T.: 12.513 min
Delta R.T.: -0.015 min
Response: 7388517
Conc: 48.52 ug/ml

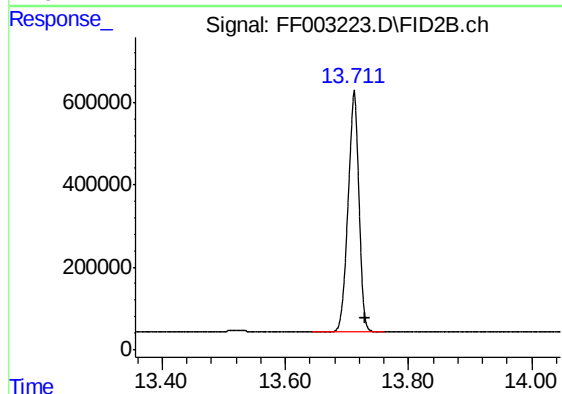


#8 N-DOCOSANE

R.T.: 13.712 min
Delta R.T.: -0.017 min
Response: 7121199
Conc: 47.24 ug/ml

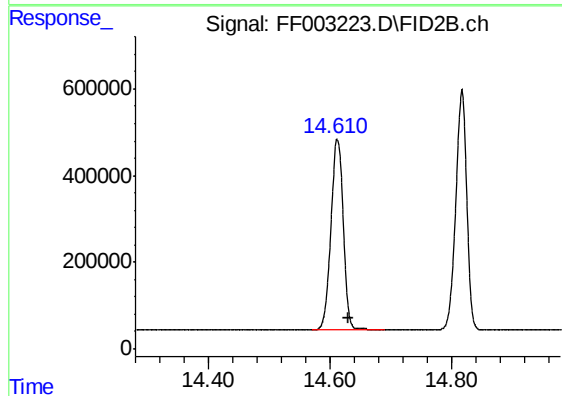


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.612 min
Delta R.T.: -0.019 min
Response: 6212589
Conc: 46.73 ug/ml

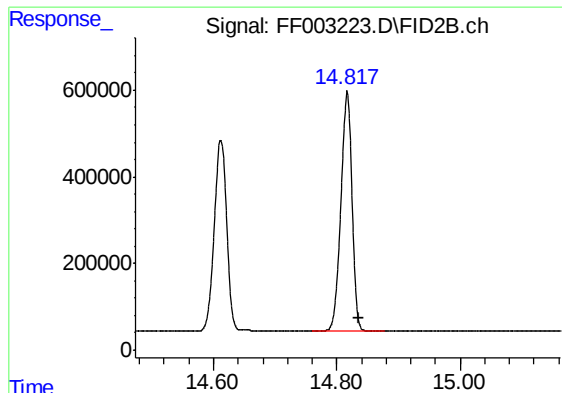


#10 N-TETRACOSANE

R.T.: 14.817 min
Delta R.T.: -0.018 min
Response: 6919705
Conc: 46.44 ug/ml

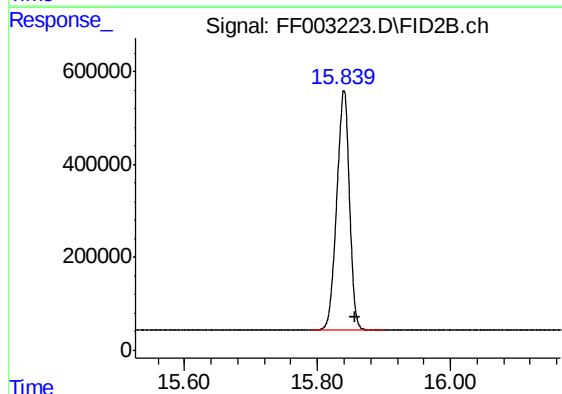

#11 N-HEXACOSANE

R.T.: 15.840 min
Delta R.T.: -0.017 min
Response: 6834957
Conc: 46.46 ug/ml

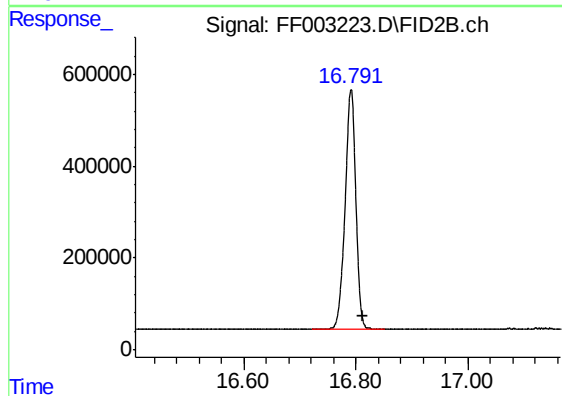

#12 N-OCTACOSANE

R.T.: 16.792 min
Delta R.T.: -0.020 min
Response: 6915987
Conc: 47.52 ug/ml