

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011123\
Data File : FF011867.D
Signal(s) : FID2B.ch
Acq On : 11 Jan 2023 08:36
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 12 02:46:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	15.226	83229	0.461 ug/ml
14)	N-DOTRIACONTANE	18.945	92088	0.569 ug/ml
16)	N-HEXATRIACONTANE	20.501	71821	0.536 ug/ml
18)	N-TETRACONTANE	22.115	84034	0.648 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011123\
Data File : FF011867.D
Signal(s) : FID2B.ch
Acq On : 11 Jan 2023 08:36
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 12 02:46:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

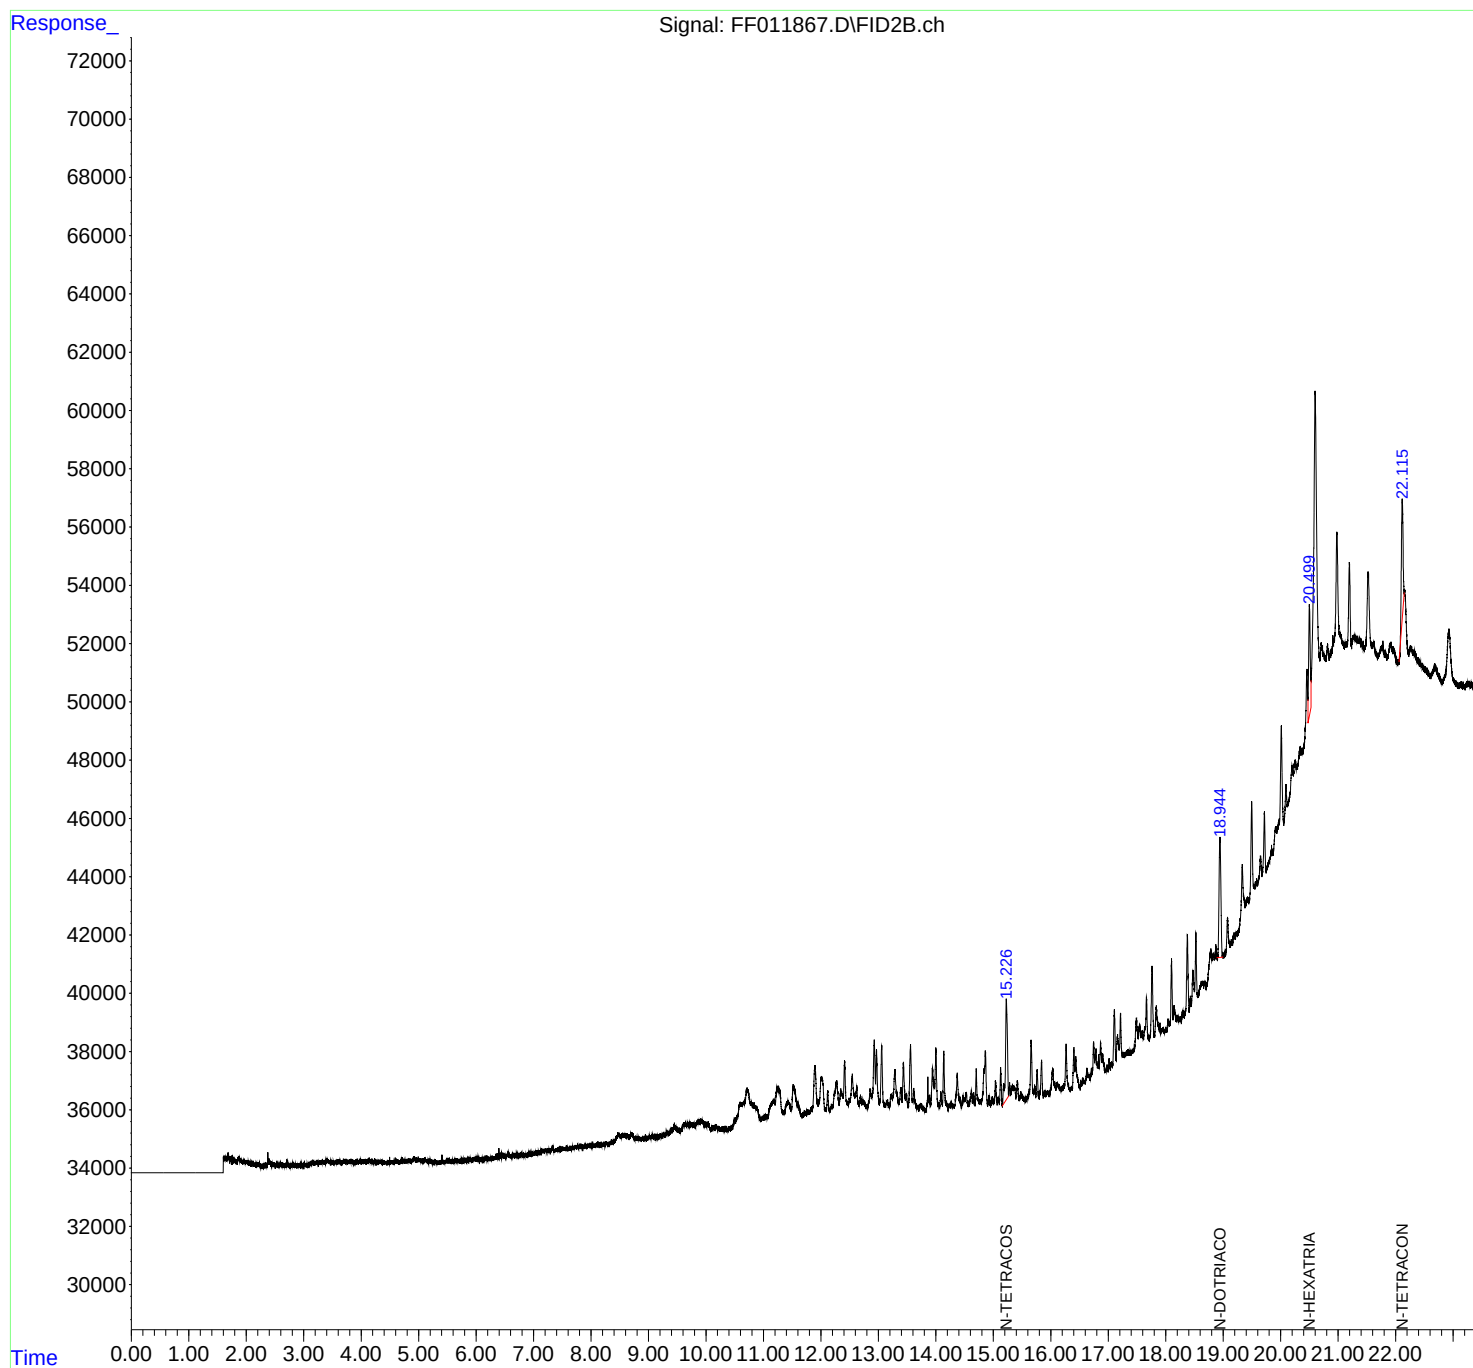


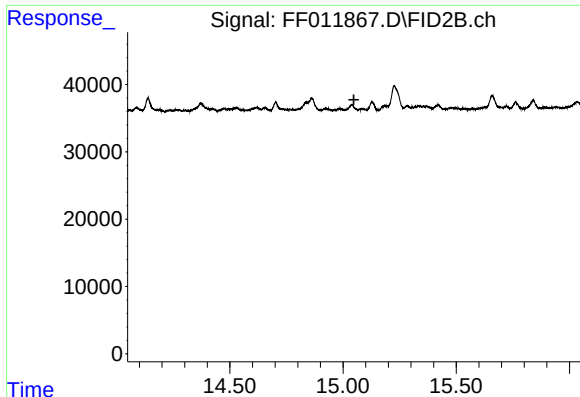

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.048 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

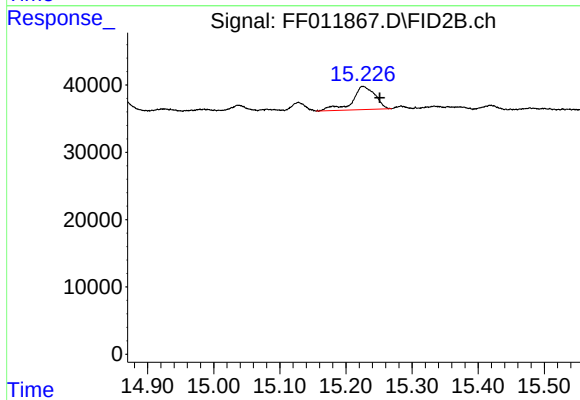


#10 N-TETRACOSANE

R.T.: 15.226 min
Delta R.T.: -0.025 min
Response: 83229
Conc: 0.46 ug/ml

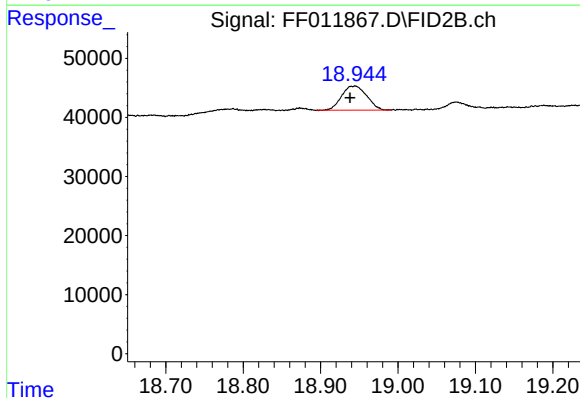


#14 N-DOTRIACONTANE

R.T.: 18.945 min
Delta R.T.: 0.006 min
Response: 92088
Conc: 0.57 ug/ml

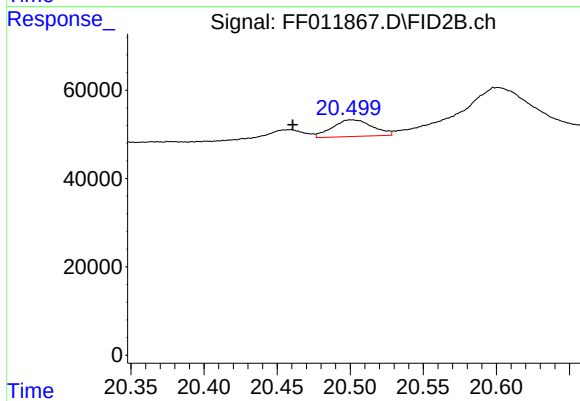

#16 N-HEXATRIACONTANE

R.T.: 20.501 min
Delta R.T.: 0.040 min
Response: 71821
Conc: 0.54 ug/ml

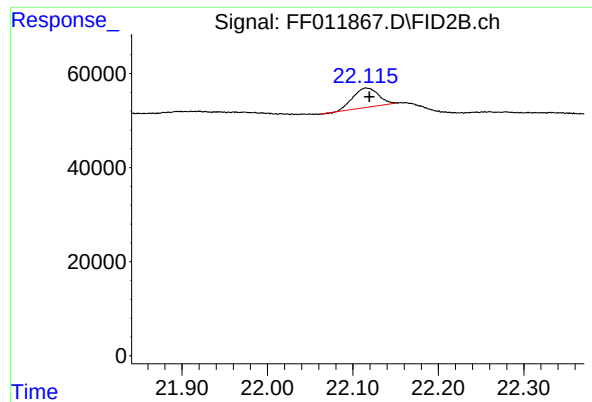

#18 N-TETRACONTANE

R.T.: 22.115 min
Delta R.T.: -0.004 min
Response: 84034
Conc: 0.65 ug/ml

Instrument :

FID_F

ClientSampleId :