

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011123\
Data File : FF011874.D
Signal(s) : FID2B.ch
Acq On : 11 Jan 2023 12:05
Operator : YP\AJ
Sample : 01080-01 200X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 12 02:47:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

2)	N-DECANE	4.648	35604	0.226 ug/ml
3)	N-DODECANE	6.786	152718	0.949 ug/ml
4)	N-TETRADECANE	8.579	117737	0.716 ug/ml
5)	N-HEXADECANE	10.206	79575	0.467 ug/ml
7)	N-EICOSANE	12.894f	64371	0.363 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011123\
Data File : FF011874.D
Signal(s) : FID2B.ch
Acq On : 11 Jan 2023 12:05
Operator : YP\AJ
Sample : 01080-01 200X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 12 02:47:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

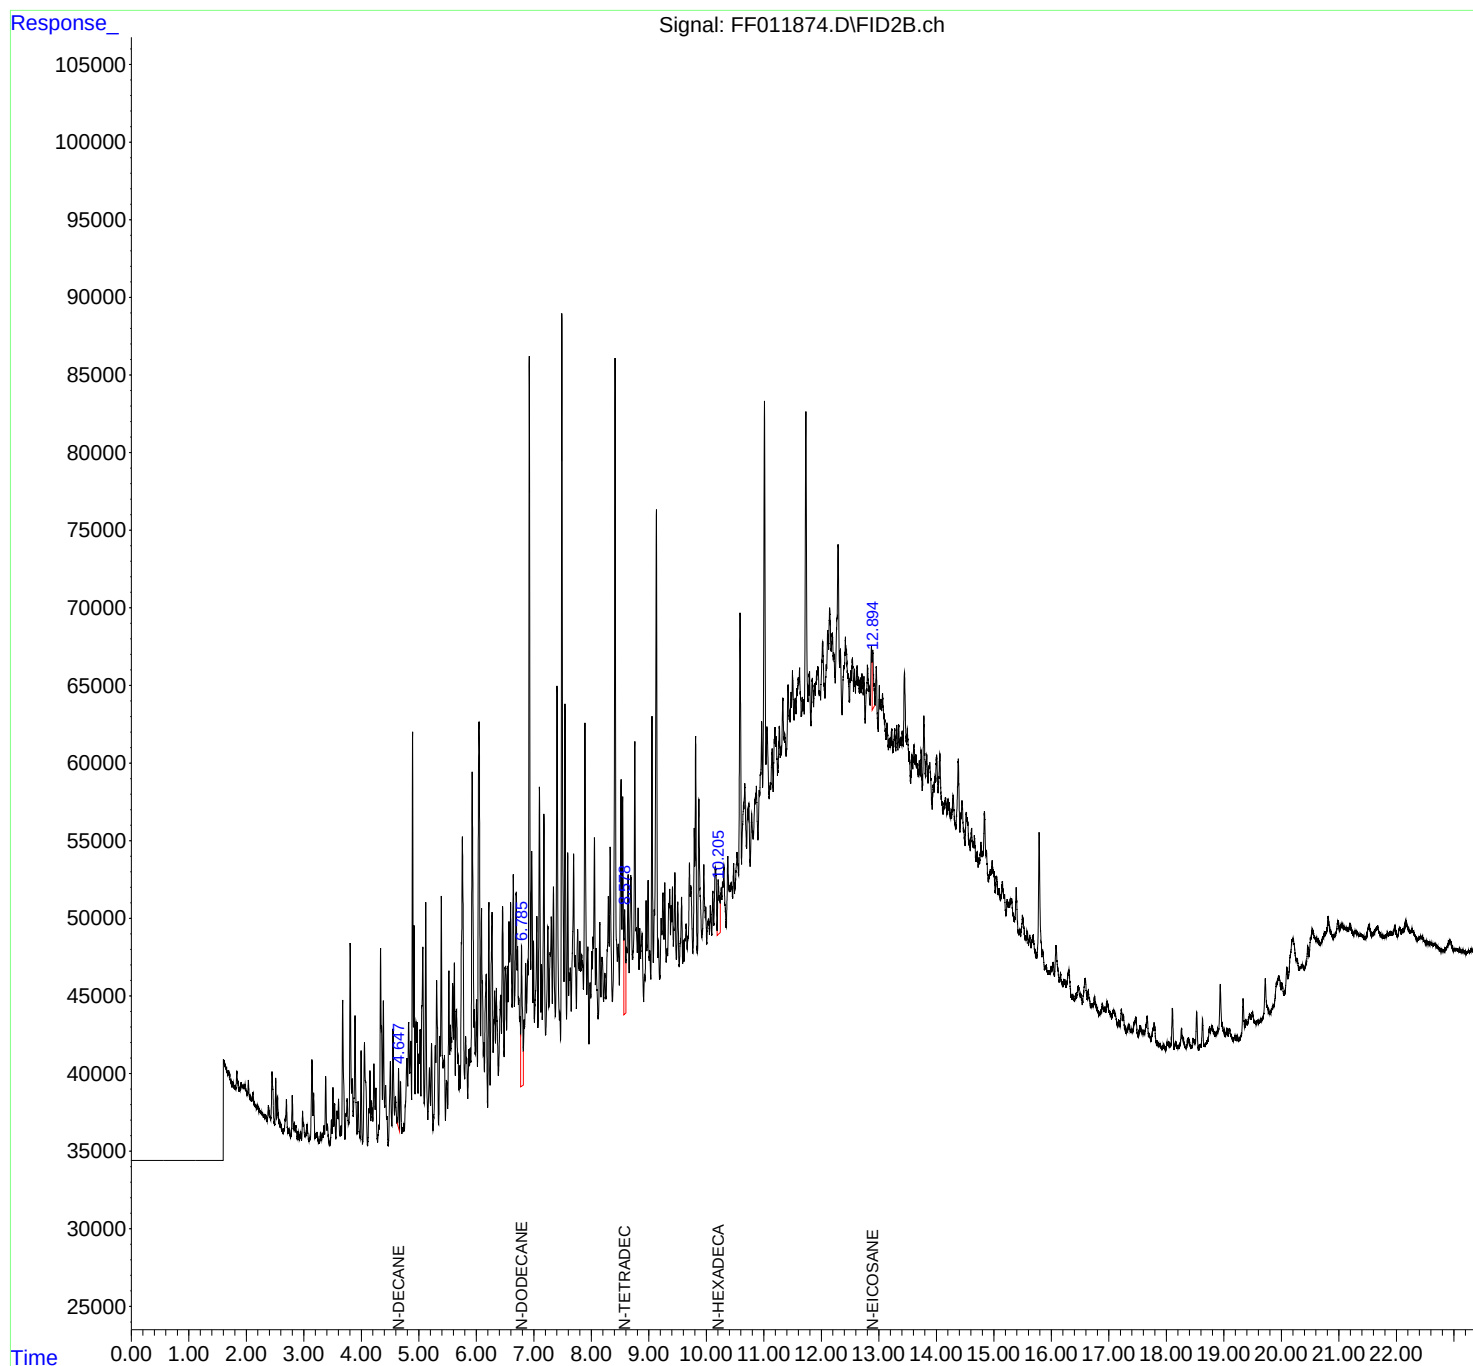


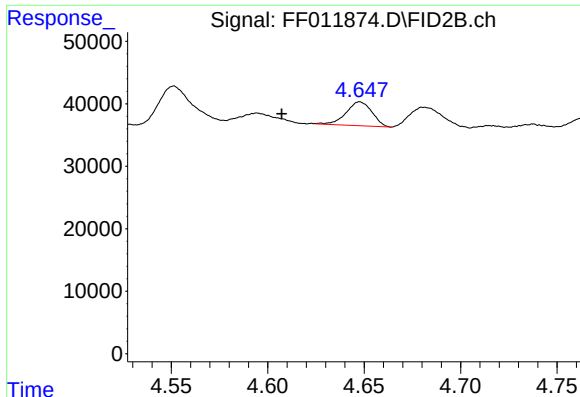

#2 N-DECANE


R.T.: 4.648 min
Delta R.T.: 0.041 min
Response: 35604
Conc: 0.23 ug/ml

Instrument :
FID_F
ClientSampleId :

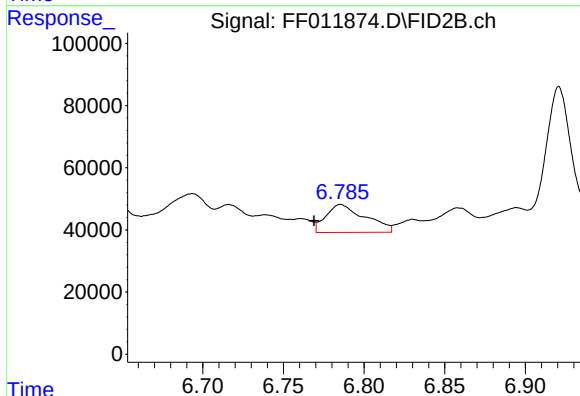


#3 N-DODECANE

R.T.: 6.786 min
Delta R.T.: 0.017 min
Response: 152718
Conc: 0.95 ug/ml

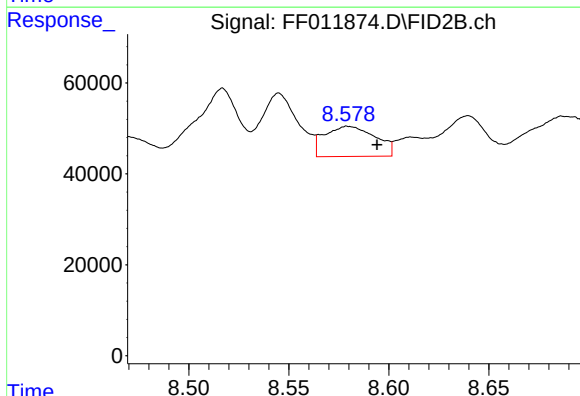


#4 N-TETRADECANE

R.T.: 8.579 min
Delta R.T.: -0.015 min
Response: 117737
Conc: 0.72 ug/ml

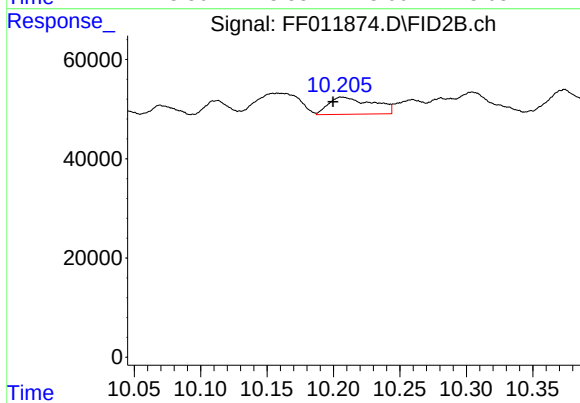

#5 N-HEXADECANE


R.T.: 10.206 min
Delta R.T.: 0.007 min
Response: 79575
Conc: 0.47 ug/ml

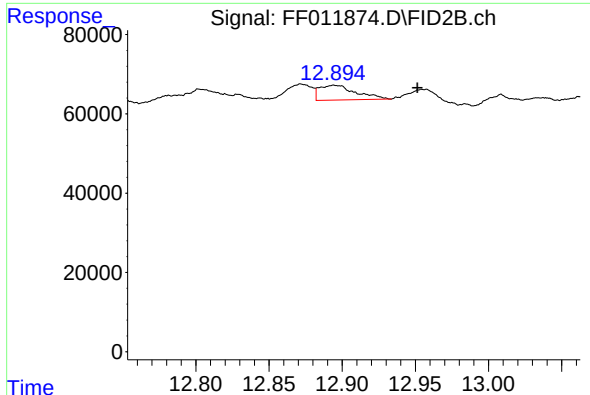

#7 N-EICOSANE

R.T.: 12.894 min
Delta R.T.: -0.057 min
Response: 64371
Conc: 0.36 ug/ml

Instrument :
FID_F
ClientSampleId :

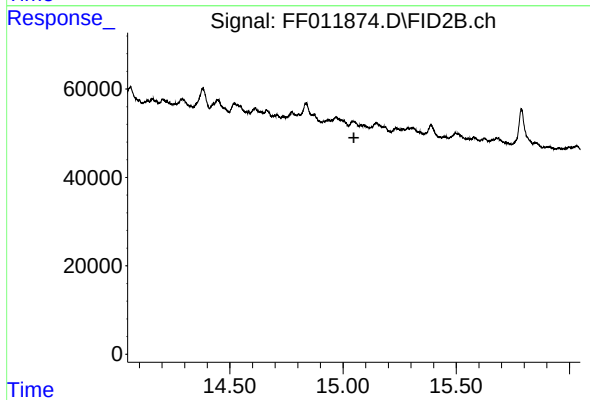

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.048 min
Response: 0
Conc: N.D.