

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011320\
 Data File : FF006176.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jan 2020 15:09
 Operator : DD\AJ
 Sample : L1070-05
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 14 07:54:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.623	1400492	12.925 ug/ml
Target Compounds			
4) N-TETRADECANE	8.250f	250709	1.986 ug/ml
7) N-EICOSANE	12.590f	171216	1.340 ug/ml
10) N-TETRACOSANE	14.801	146788	1.178 ug/ml
11) N-HEXACOSANE	15.842	87554	0.712 ug/ml
12) N-OCTACOSANE	16.789	156736	1.289 ug/ml
13) N-TRIACONTANE	17.672	329673	2.750 ug/ml
14) N-DOTRIACONTANE	18.495	198064	1.714 ug/ml
15) N-TETRATRIACONTANE	19.292	143222	1.271 ug/ml
16) N-HEXATRIACONTANE	20.024	252413	2.361 ug/ml
17) N-OCTATRIACONTANE	20.745	45790	0.495 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011320\
Data File : FF006176.D
Signal(s) : FID2B.ch
Acq On : 13 Jan 2020 15:09
Operator : DD\AJ
Sample : L1070-05
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 14 07:54:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

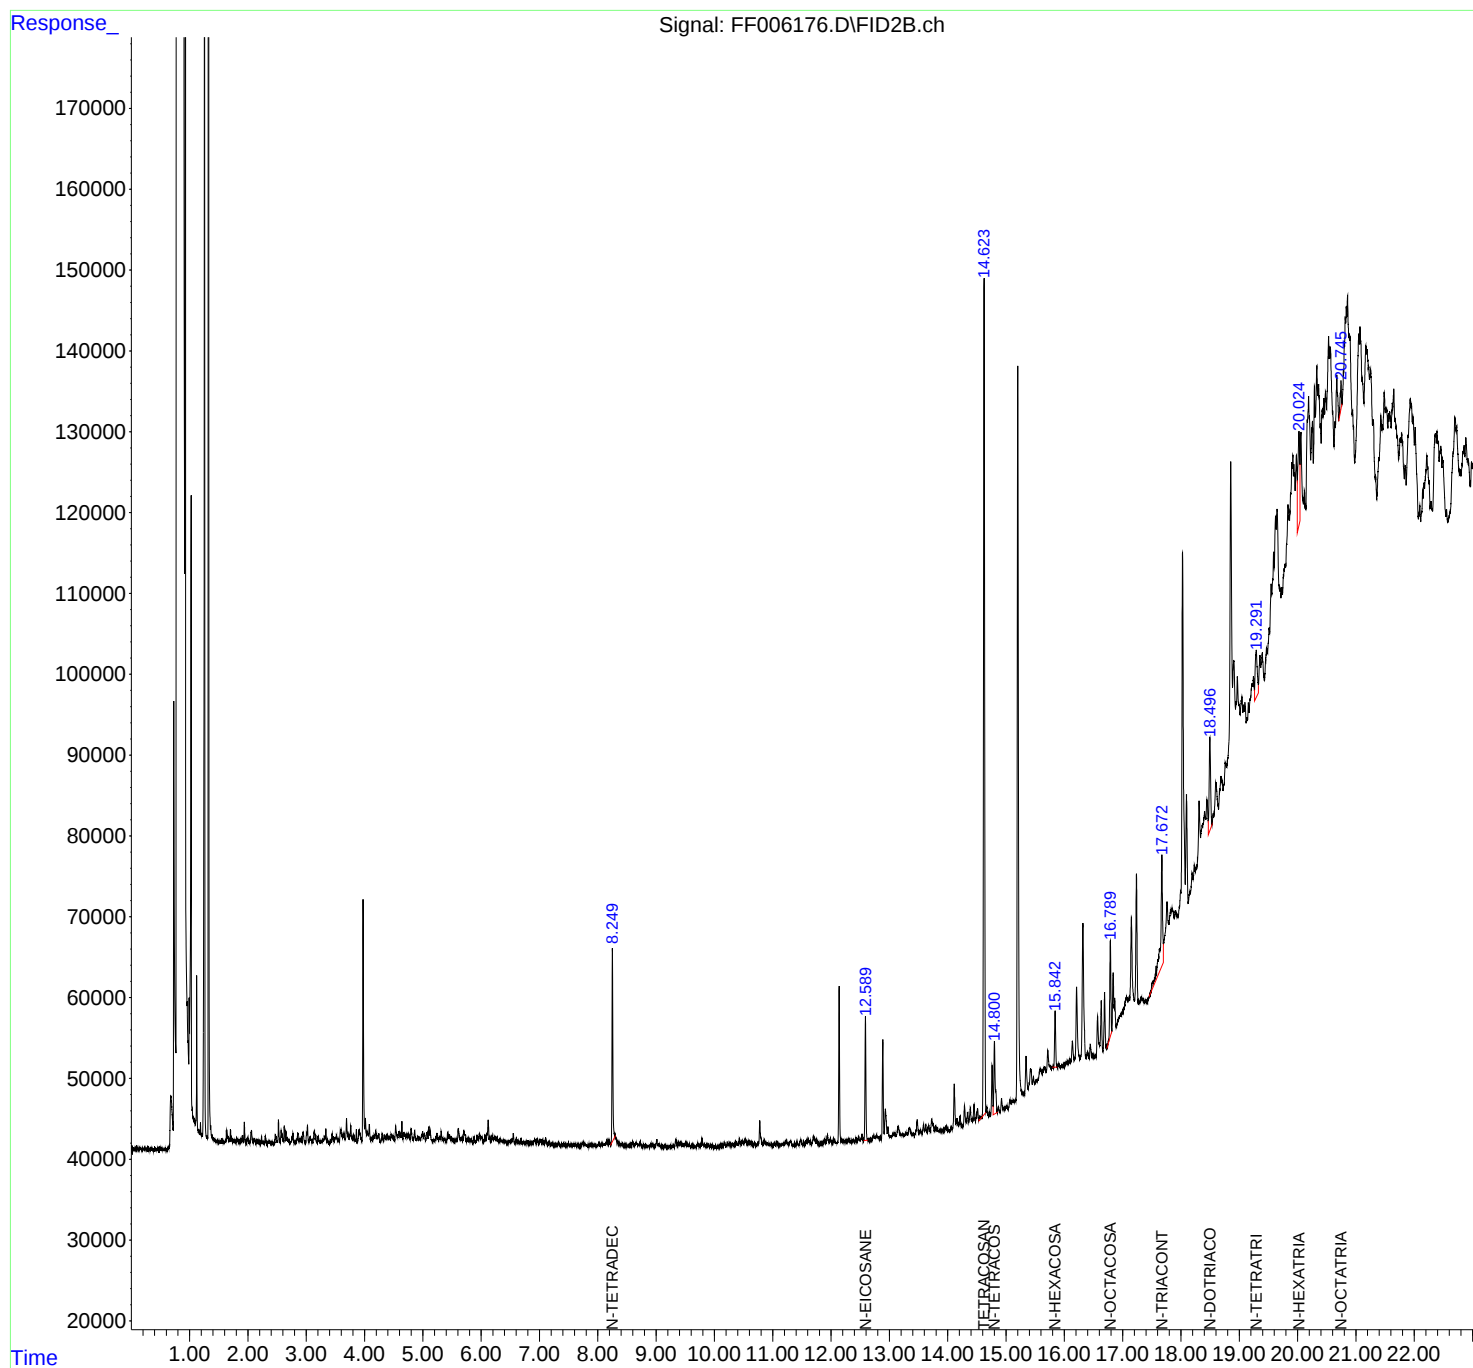

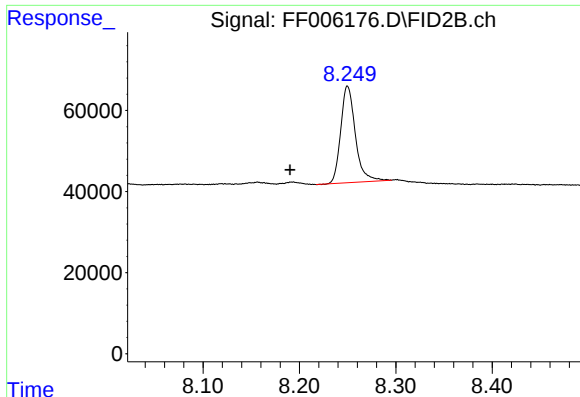


#4 N-TETRADECANE

R.T.: 8.250 min
Delta R.T.: 0.060 min
Response: 250709
Conc: 1.99 ug/ml

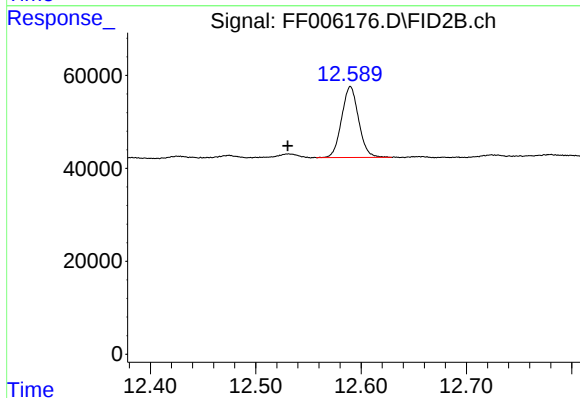


#7 N-EICOSANE

R.T.: 12.590 min
Delta R.T.: 0.060 min
Response: 171216
Conc: 1.34 ug/ml

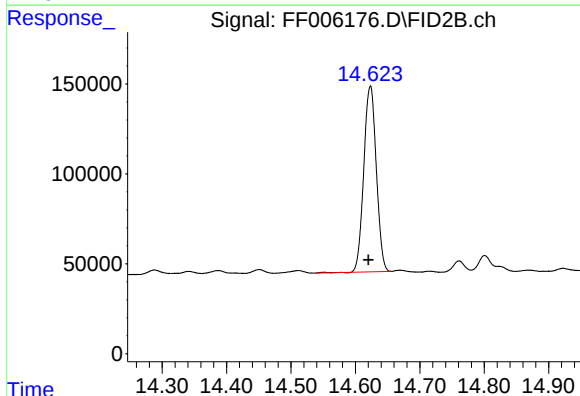


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.623 min
Delta R.T.: 0.003 min
Response: 1400492
Conc: 12.92 ug/ml

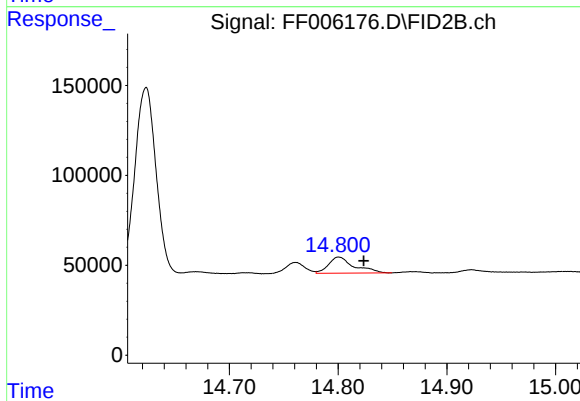


#10 N-TETRACOSANE

R.T.: 14.801 min
Delta R.T.: -0.023 min
Response: 146788
Conc: 1.18 ug/ml

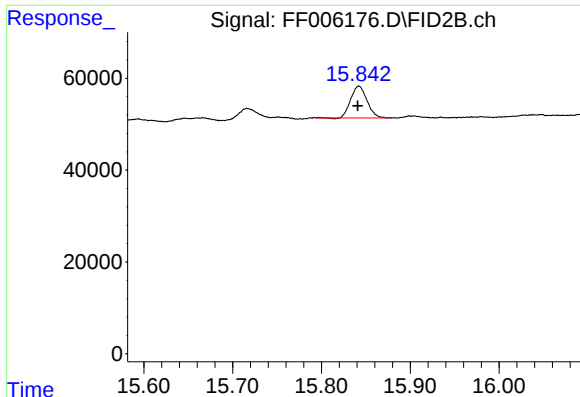


#11 N-HEXACOSANE

R.T.: 15.842 min
Delta R.T.: 0.001 min
Response: 87554
Conc: 0.71 ug/ml

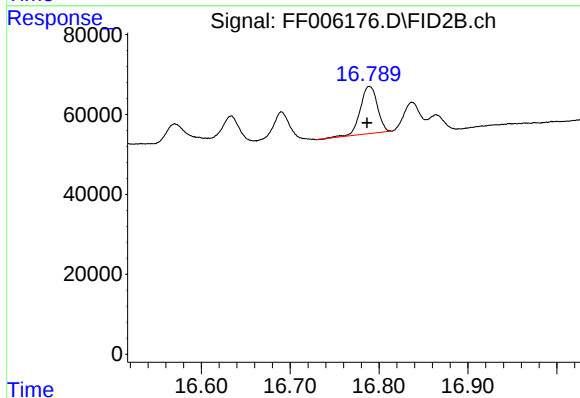


#12 N-OCTACOSANE

R.T.: 16.789 min
Delta R.T.: 0.003 min
Response: 156736
Conc: 1.29 ug/ml

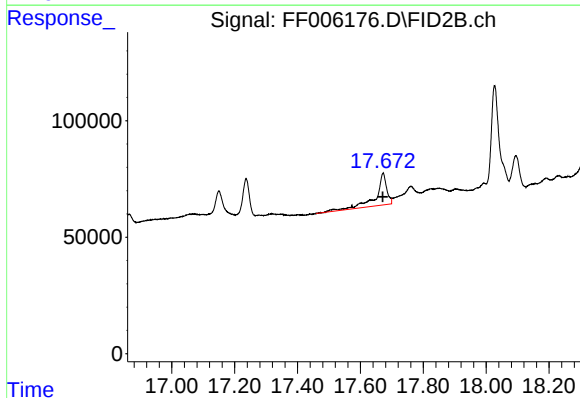


#13 N-TRIACONTANE

R.T.: 17.672 min
Delta R.T.: 0.000 min
Response: 329673
Conc: 2.75 ug/ml

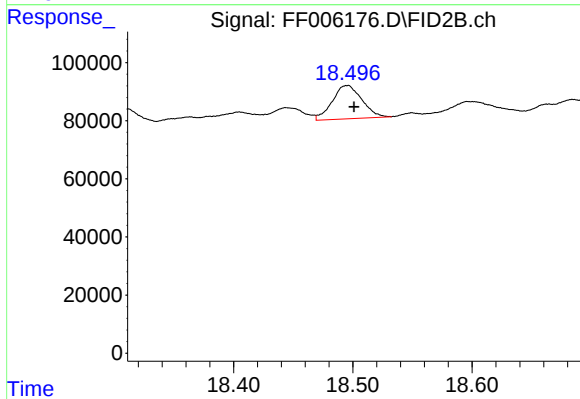


#14 N-DOTRIACONTANE

R.T.: 18.495 min
Delta R.T.: -0.006 min
Response: 198064
Conc: 1.71 ug/ml

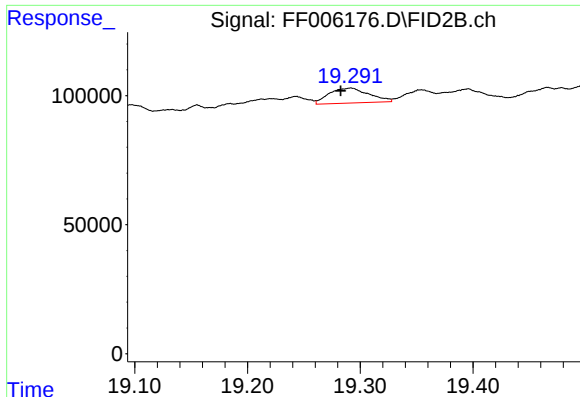


#15 N-TETRATRIACONTANE

R.T.: 19.292 min
Delta R.T.: 0.009 min
Response: 143222
Conc: 1.27 ug/ml

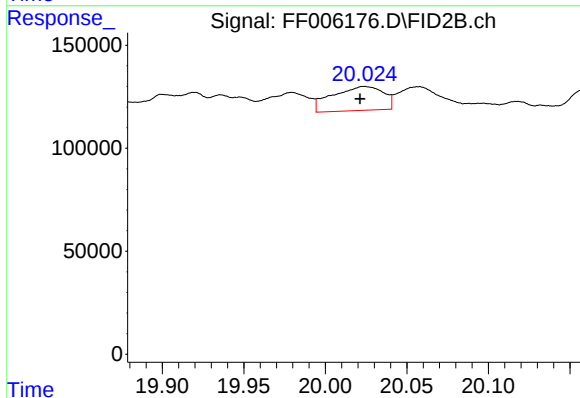

#16 N-HEXATRIACONTANE

R.T.: 20.024 min
Delta R.T.: 0.003 min
Response: 252413
Conc: 2.36 ug/ml

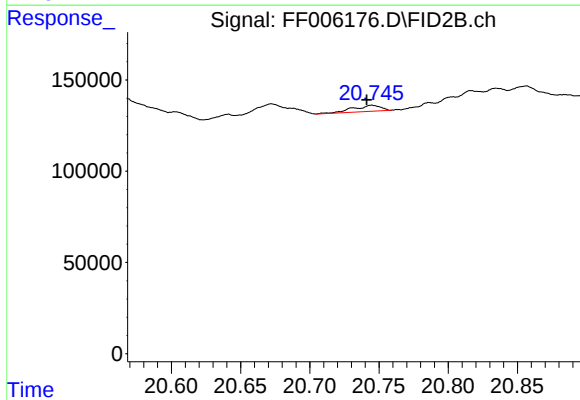

#17 N-OCTATRIACONTANE

R.T.: 20.745 min
Delta R.T.: 0.004 min
Response: 45790
Conc: 0.49 ug/ml