

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011419\
 Data File : FF003244.D
 Signal(s) : FID2B.ch
 Acq On : 14 Jan 2019 16:16
 Operator : AJ\SJ
 Sample : K1126-01 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 14 21:34:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.608	774442	5.825 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.153	454758	2.983 ug/ml
5)	N-HEXADECANE	9.753	367045	2.394 ug/ml
6)	N-OCTADECANE	11.195	363151	2.361 ug/ml
7)	N-EICOSANE	12.507	293628	1.928 ug/ml
8)	N-DOCOSANE	13.707	209057	1.387 ug/ml
10)	N-TETRACOSANE	14.780f	266956	1.792 ug/ml
12)	N-OCTACOSANE	16.788	187116	1.286 ug/ml
13)	N-TRIACONTANE	17.676	224871	1.575 ug/ml
14)	N-DOTRIACONTANE	18.512	192527	1.445 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011419\
Data File : FF003244.D
Signal(s) : FID2B.ch
Acq On : 14 Jan 2019 16:16
Operator : AJ\SJ
Sample : K1126-01 2X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 14 21:34:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

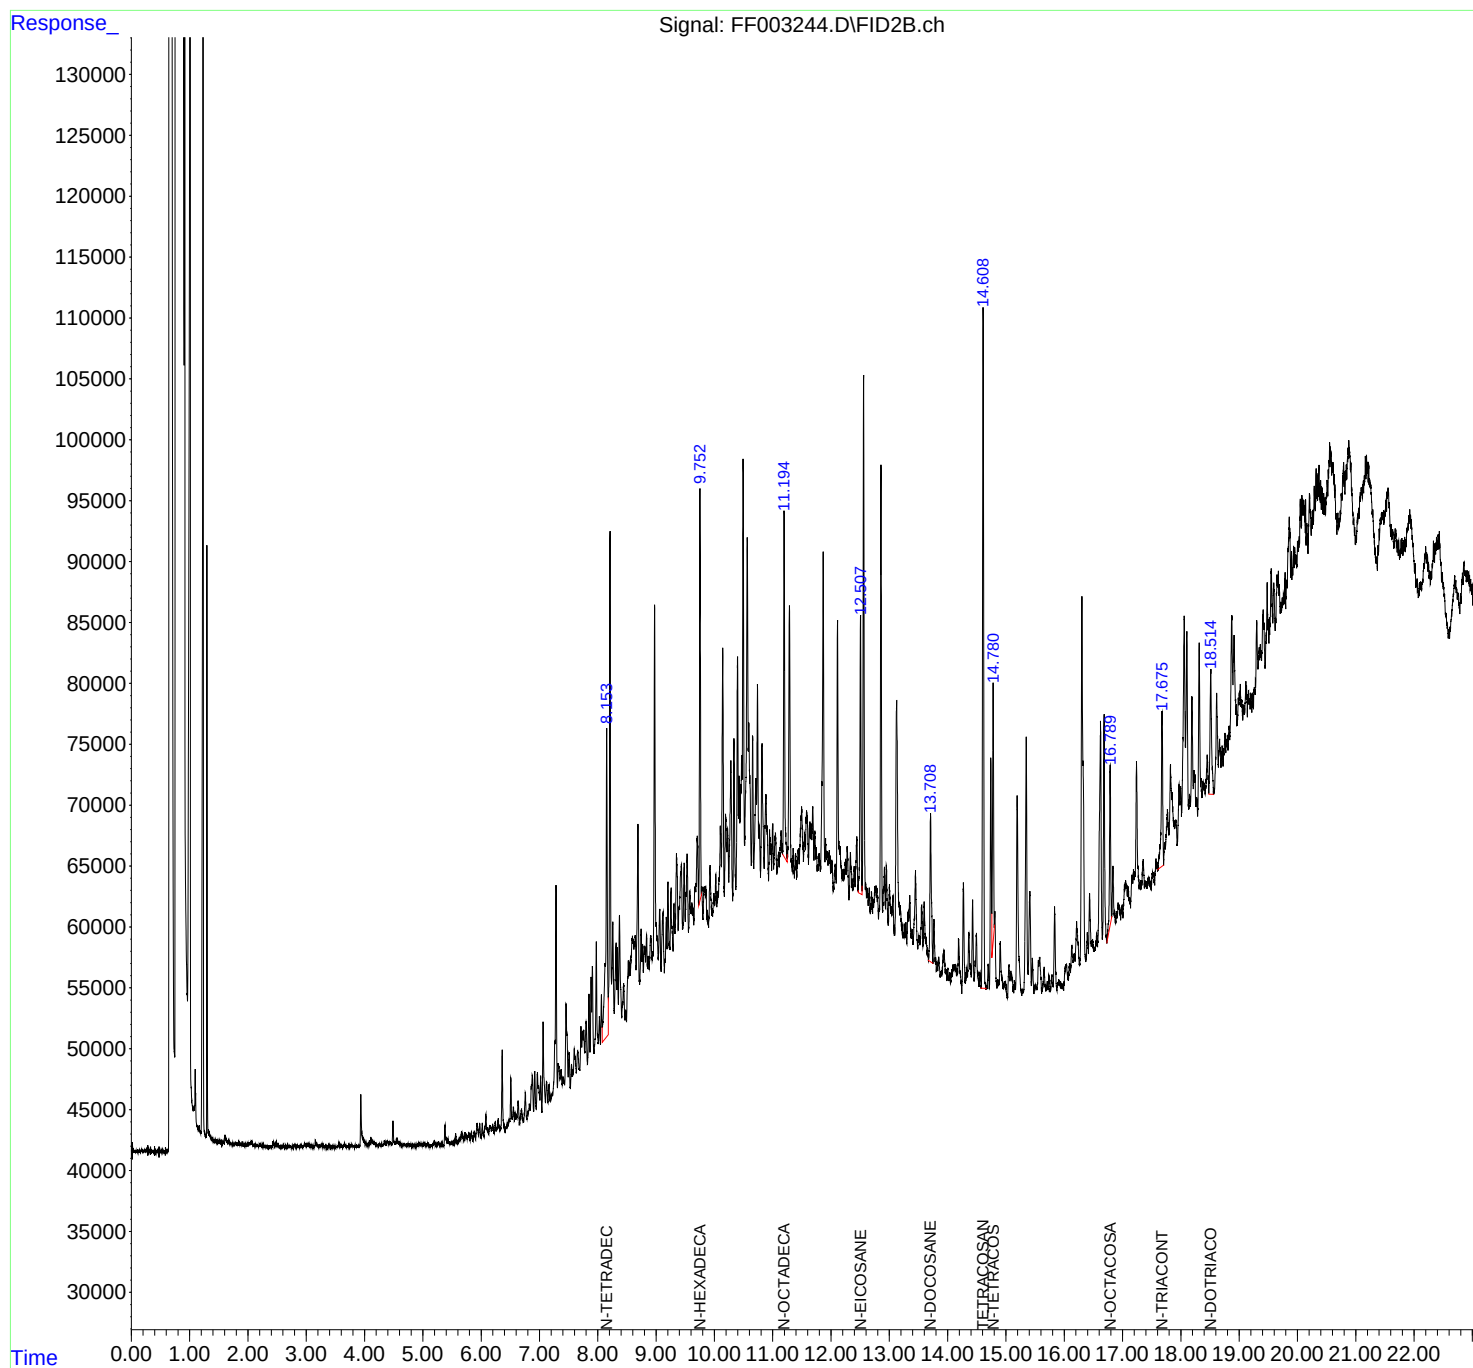

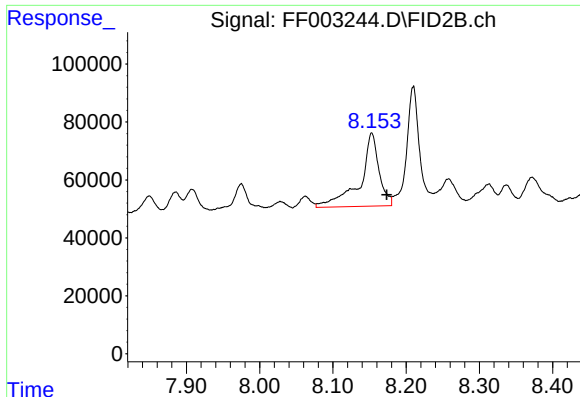


#4 N-TETRADECANE

R.T.: 8.153 min
Delta R.T.: -0.020 min
Response: 454758
Conc: 2.98 ug/ml

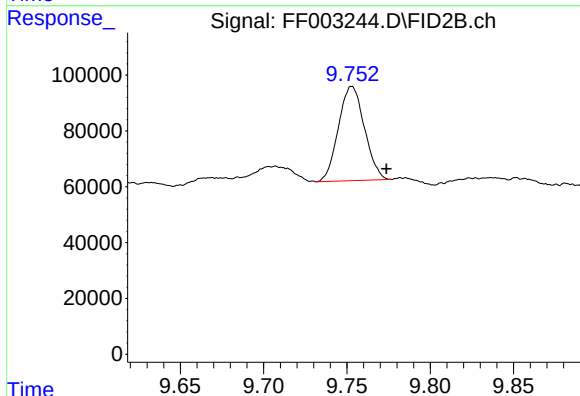


#5 N-HEXADECANE

R.T.: 9.753 min
Delta R.T.: -0.021 min
Response: 367045
Conc: 2.39 ug/ml

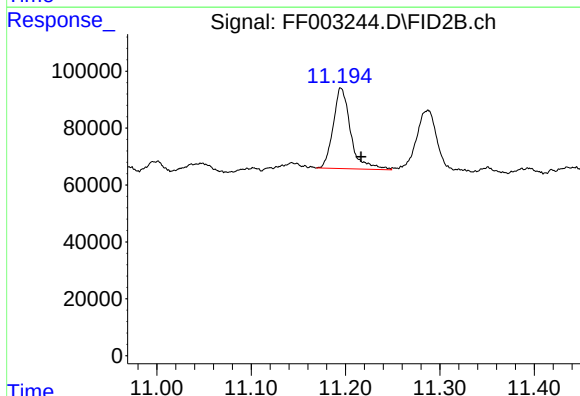


#6 N-OCTADECANE

R.T.: 11.195 min
Delta R.T.: -0.021 min
Response: 363151
Conc: 2.36 ug/ml

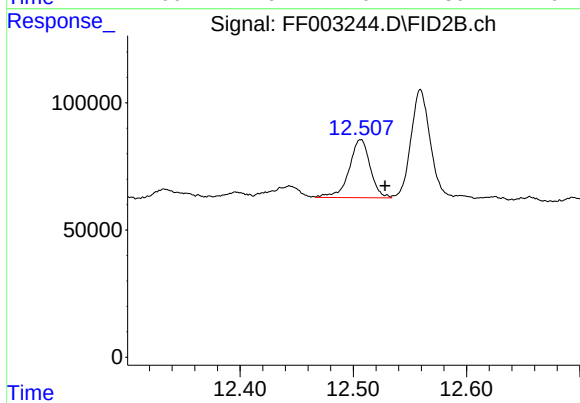


#7 N-EICOSANE

R.T.: 12.507 min
Delta R.T.: -0.021 min
Response: 293628
Conc: 1.93 ug/ml

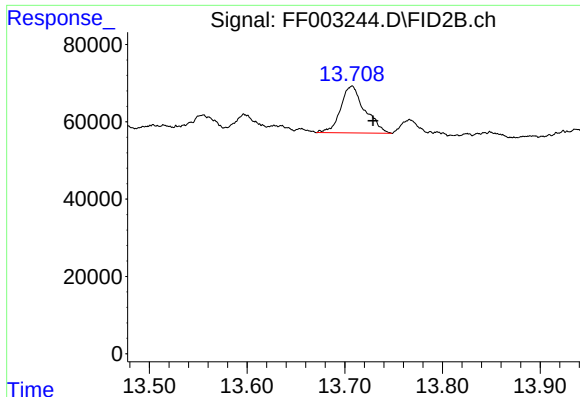


#8 N-DOCOSANE

R.T.: 13.707 min
Delta R.T.: -0.021 min
Response: 209057
Conc: 1.39 ug/ml

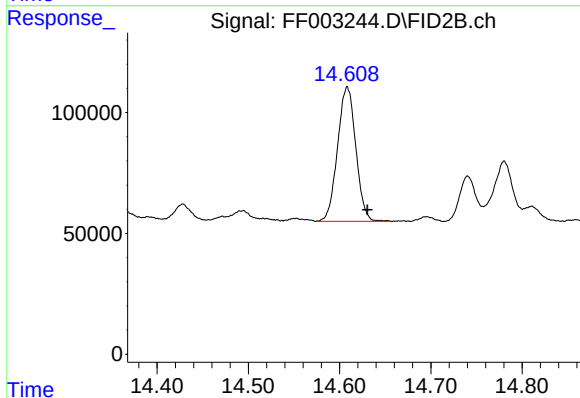


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.608 min
Delta R.T.: -0.022 min
Response: 774442
Conc: 5.83 ug/ml

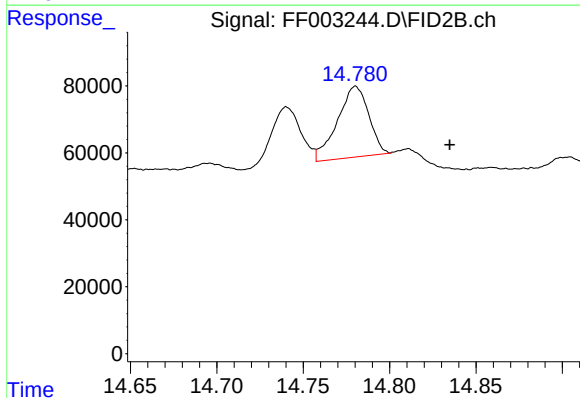


#10 N-TETRACOSANE

R.T.: 14.780 min
Delta R.T.: -0.055 min
Response: 266956
Conc: 1.79 ug/ml

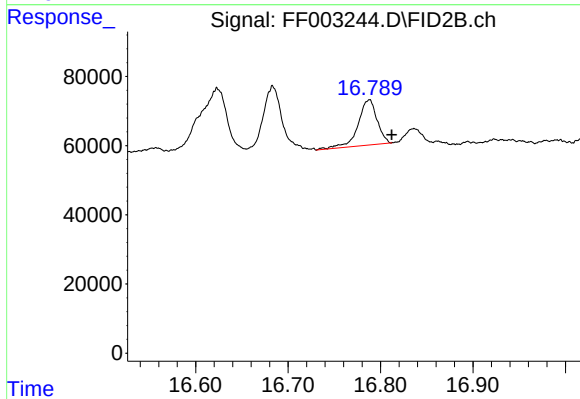


#12 N-OCTACOSANE

R.T.: 16.788 min
Delta R.T.: -0.024 min
Response: 187116
Conc: 1.29 ug/ml

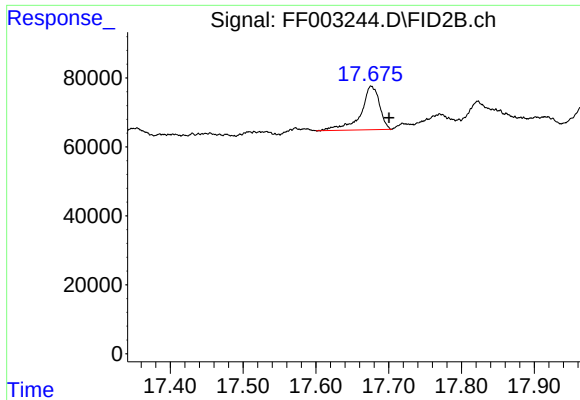

#13 N-TRIACONTANE

R.T.: 17.676 min
Delta R.T.: -0.025 min
Response: 224871
Conc: 1.57 ug/ml

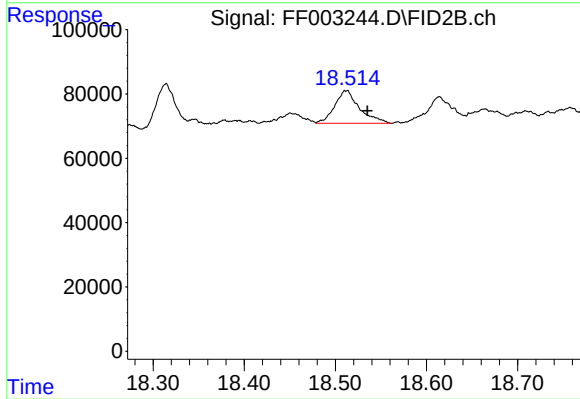

#14 N-DOTRIACONTANE

R.T.: 18.512 min
Delta R.T.: -0.023 min
Response: 192527
Conc: 1.45 ug/ml