

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011419\
 Data File : FF003242.D
 Signal(s) : FID2B.ch
 Acq On : 14 Jan 2019 15:03
 Operator : AJ\SJ
 Sample : K1128-01MSD
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 14 21:33:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.608	2117986	15.931 ug/mlm
Target Compounds			
2) N-DECANE	4.349	2415203	16.083 ug/ml
3) N-DODECANE	6.367	2531105	16.725 ug/ml
4) N-TETRADECANE	8.158	2573817	16.883 ug/ml
5) N-HEXADECANE	9.757	2608836	17.018 ug/ml
6) N-OCTADECANE	11.199	2589760	16.838 ug/ml
7) N-EICOSANE	12.508	2527488	16.598 ug/ml
8) N-DOCOSANE	13.708	2504964	16.616 ug/ml
10) N-TETRACOSANE	14.813	2622144	17.598 ug/ml
11) N-HEXACOSANE	15.836	2481049	16.863 ug/ml
12) N-OCTACOSANE	16.788	2590143	17.797 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011419\
Data File : FF003242.D
Signal(s) : FID2B.ch
Acq On : 14 Jan 2019 15:03
Operator : AJ\SJ
Sample : K1128-01MSD
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 14 21:33:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

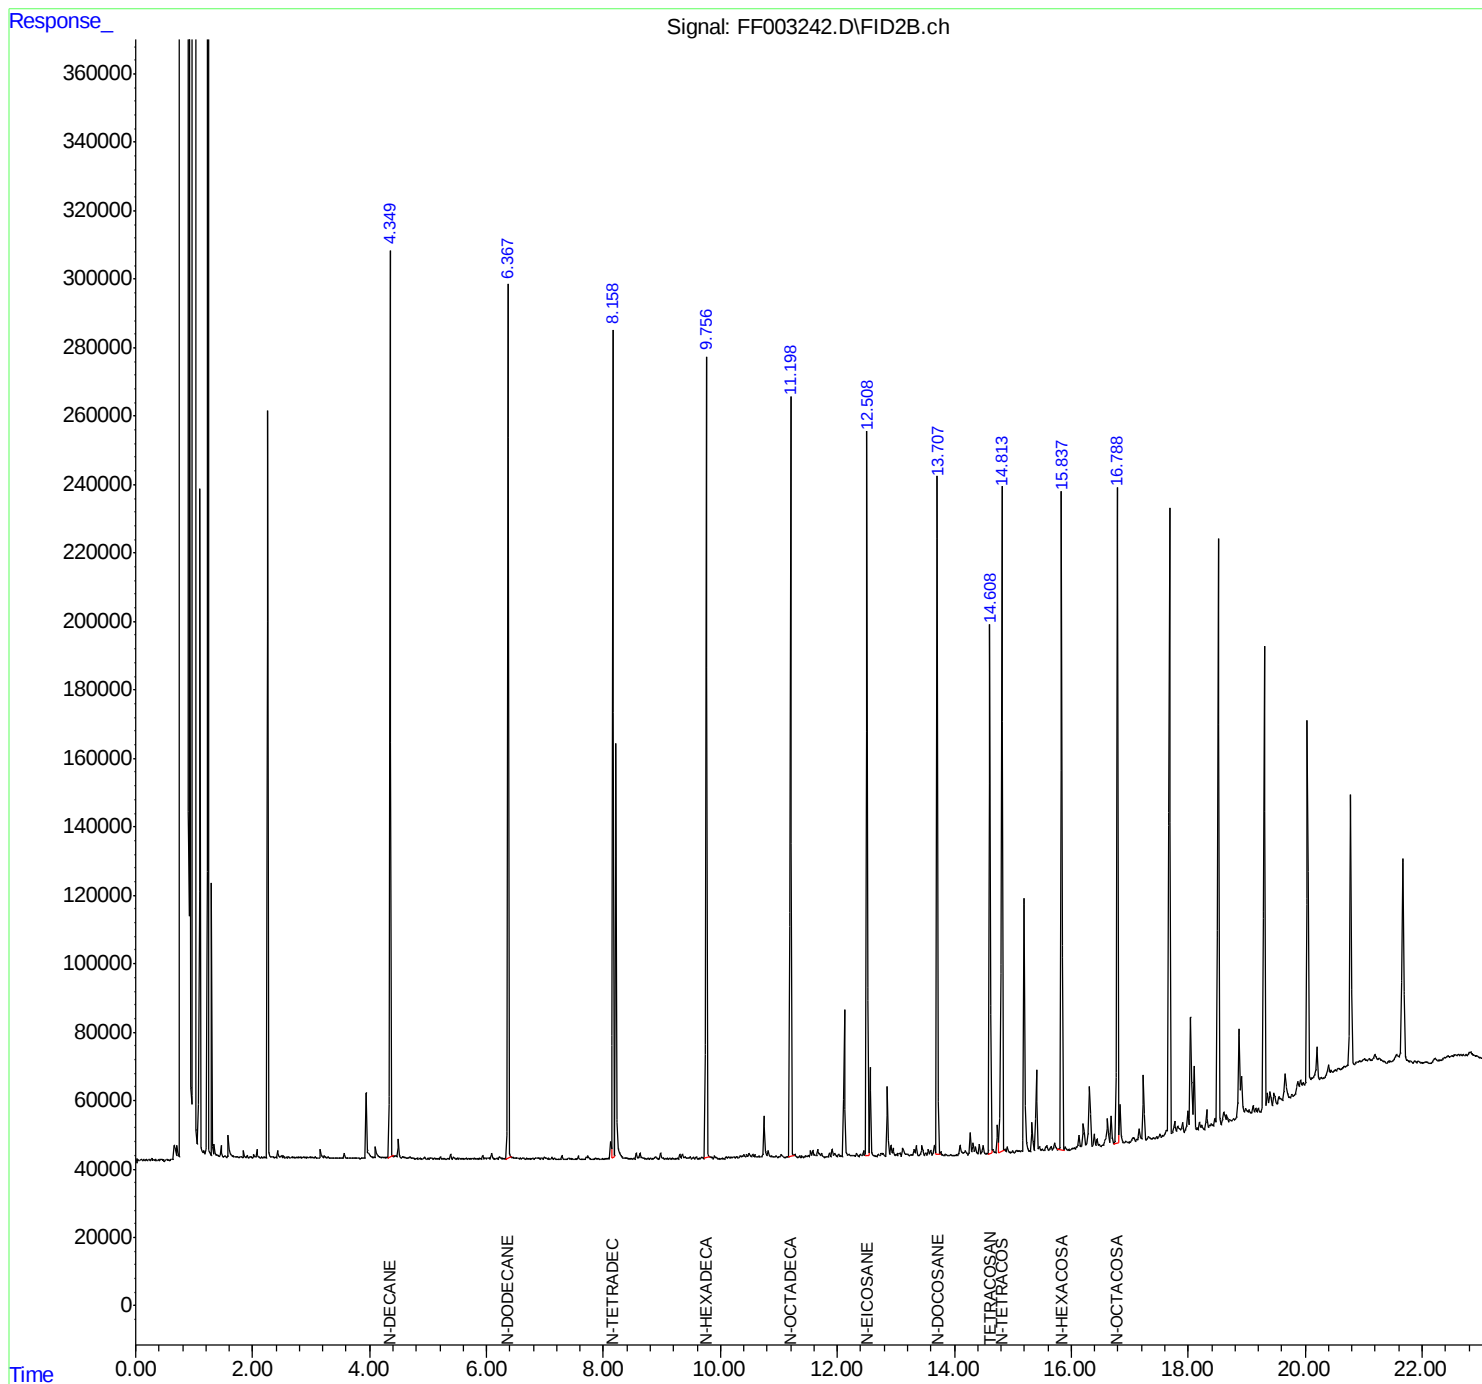

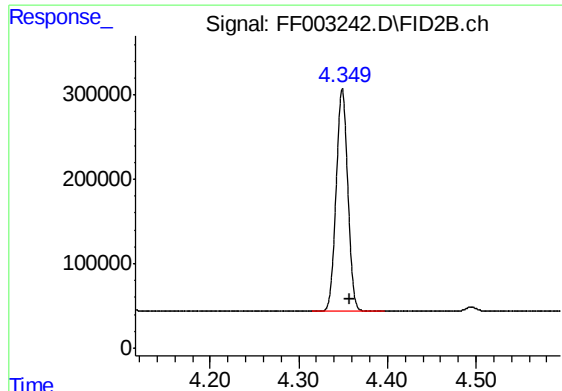


#2 N-DECANE

R.T.: 4.349 min
Delta R.T.: -0.009 min
Response: 2415203
Conc: 16.08 ug/ml

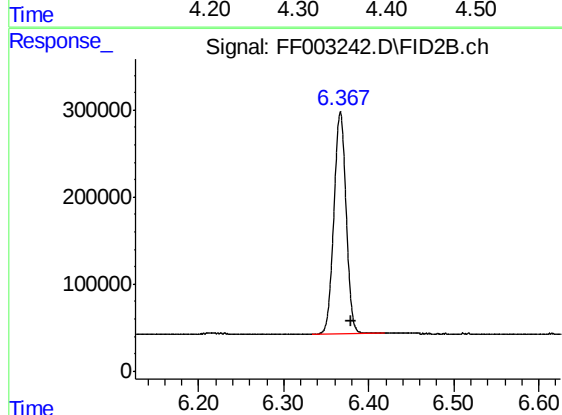


#3 N-DODECANE

R.T.: 6.367 min
Delta R.T.: -0.013 min
Response: 2531105
Conc: 16.72 ug/ml

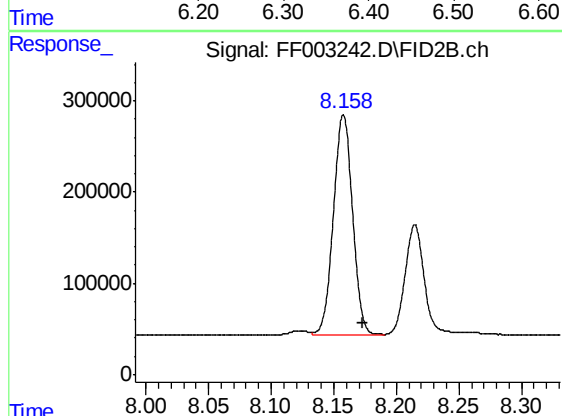


#4 N-TETRADECANE

R.T.: 8.158 min
Delta R.T.: -0.016 min
Response: 2573817
Conc: 16.88 ug/ml

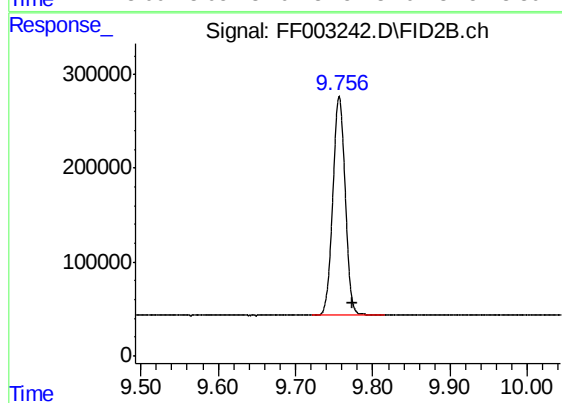


#5 N-HEXADECANE

R.T.: 9.757 min
Delta R.T.: -0.017 min
Response: 2608836
Conc: 17.02 ug/ml

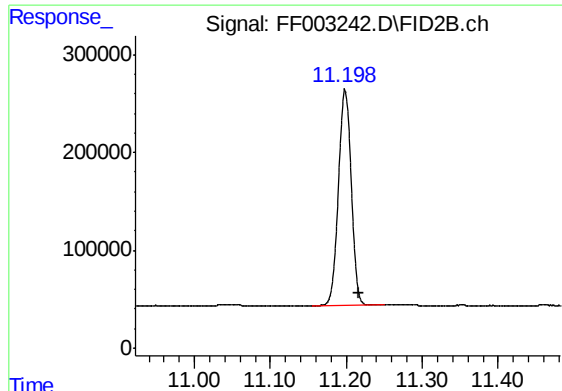


#6 N-OCTADECANE

R.T.: 11.199 min
Delta R.T.: -0.018 min
Response: 2589760
Conc: 16.84 ug/ml

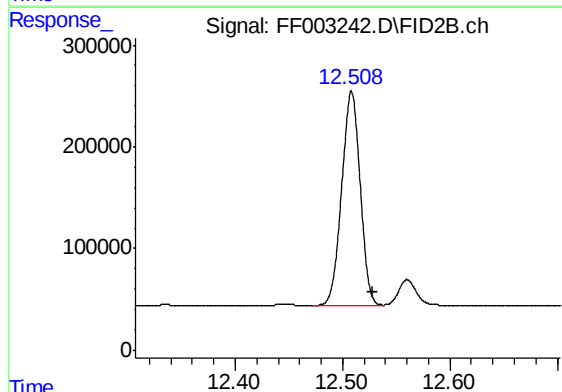


#7 N-EICOSANE

R.T.: 12.508 min
Delta R.T.: -0.020 min
Response: 2527488
Conc: 16.60 ug/ml

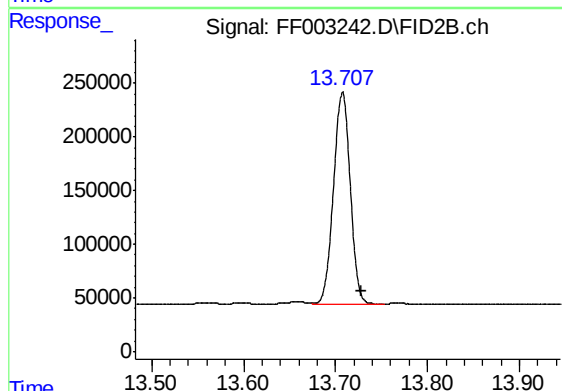


#8 N-DOCOSANE

R.T.: 13.708 min
Delta R.T.: -0.021 min
Response: 2504964
Conc: 16.62 ug/ml

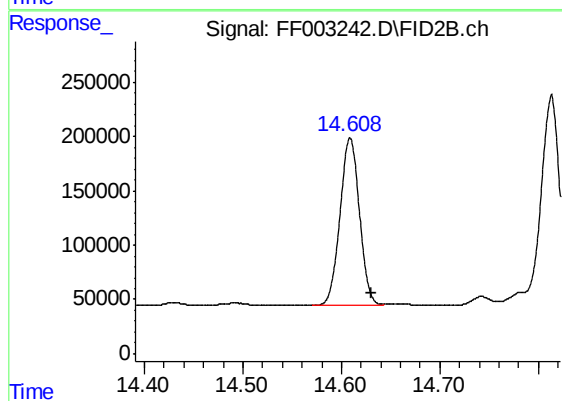


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.608 min
Delta R.T.: -0.022 min
Response: 2117986
Conc: 15.93 ug/ml m

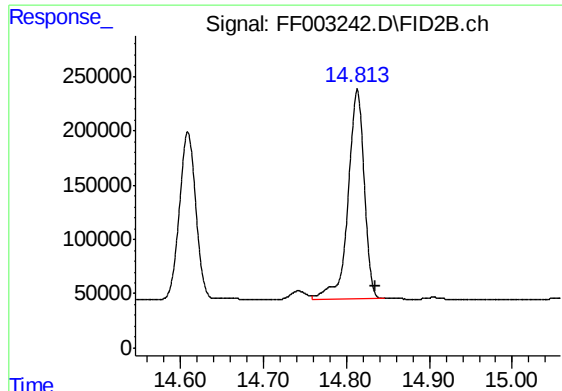


#10 N-TETRACOSANE

R.T.: 14.813 min
Delta R.T.: -0.022 min
Response: 2622144
Conc: 17.60 ug/ml

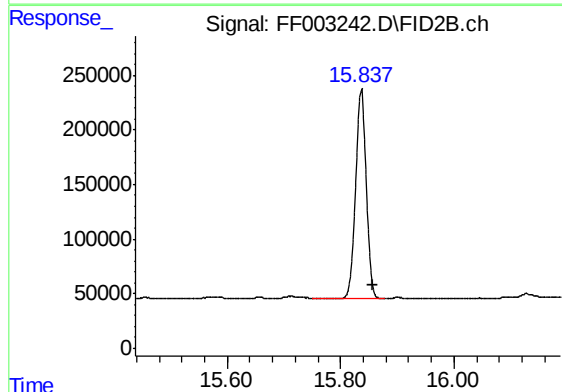

#11 N-HEXACOSANE

R.T.: 15.836 min
Delta R.T.: -0.021 min
Response: 2481049
Conc: 16.86 ug/ml

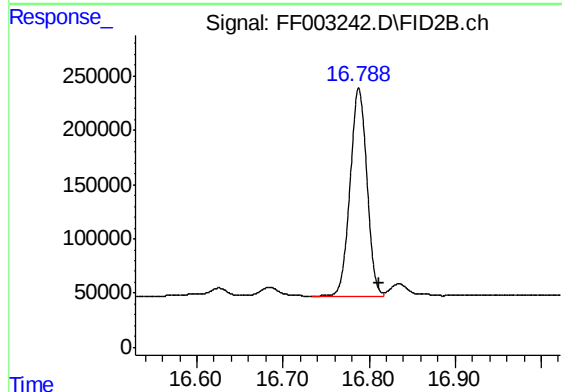

#12 N-OCTACOSANE

R.T.: 16.788 min
Delta R.T.: -0.024 min
Response: 2590143
Conc: 17.80 ug/ml m