

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF011519\
Data File : FF003247.D
Signal(s) : FID2B.ch
Acq On : 15 Jan 2019 08:44
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 15 14:04:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
7)	N-EICOSANE	12.493	123278	0.751 ug/ml
8)	N-DOCOSANE	13.701	154968	0.954 ug/ml
10)	N-TETRACOSANE	14.782f	719831	4.488 ug/ml
11)	N-HEXACOSANE	15.833	88286	0.558 ug/ml
12)	N-OCTACOSANE	16.786	106758	0.678 ug/ml
13)	N-TRIACONTANE	17.676	120815	0.770 ug/ml
14)	N-DOTRIACONTANE	18.514	239995	1.650 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF011519\
Data File : FF003247.D
Signal(s) : FID2B.ch
Acq On : 15 Jan 2019 08:44
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 15 14:04:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

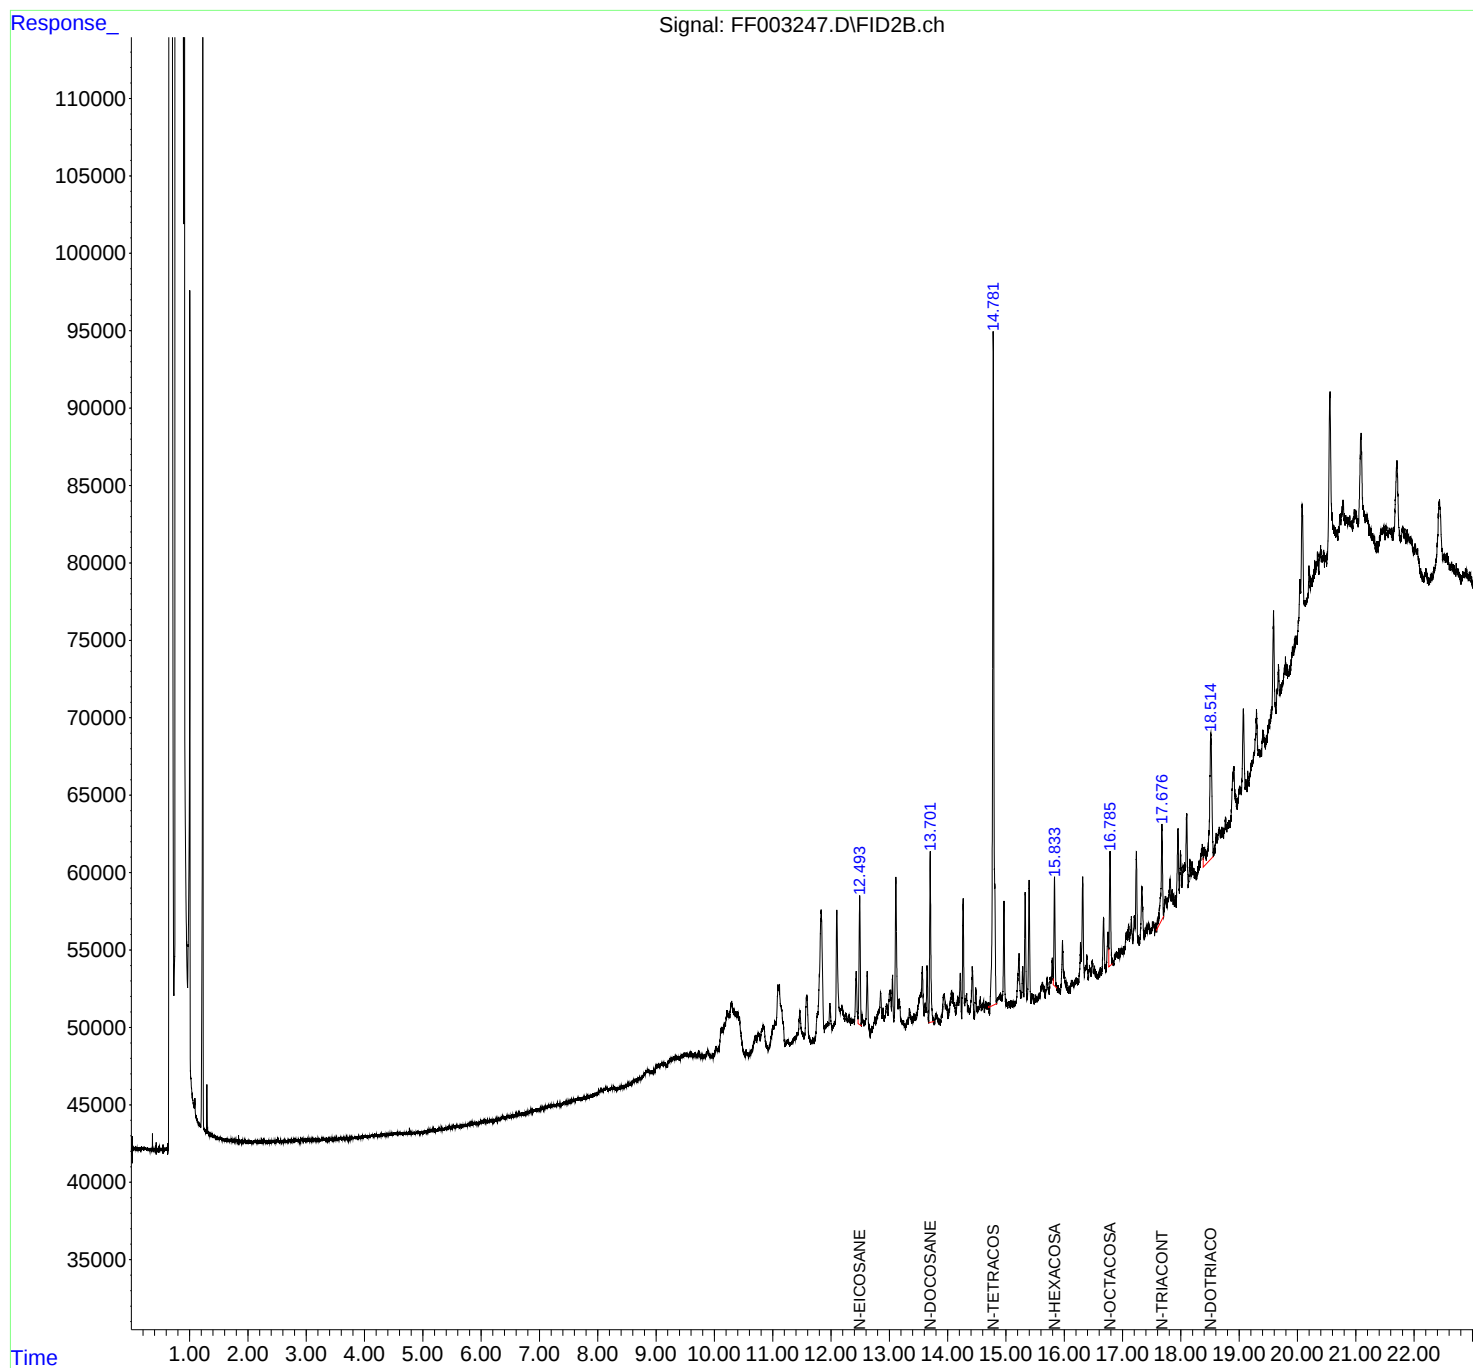


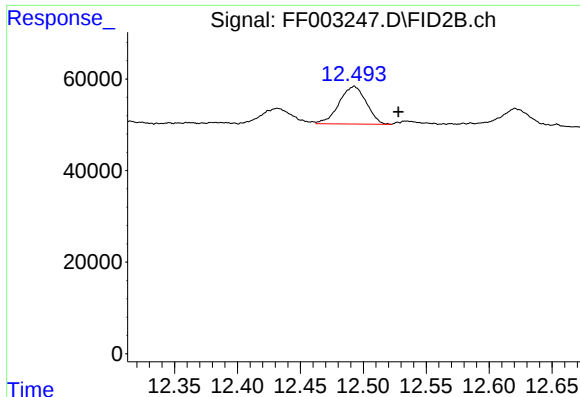

#7 N-EICOSANE


R.T.: 12.493 min
Delta R.T.: -0.035 min
Response: 123278
Conc: 0.75 ug/ml

Instrument :
FID_F
ClientSampleId :

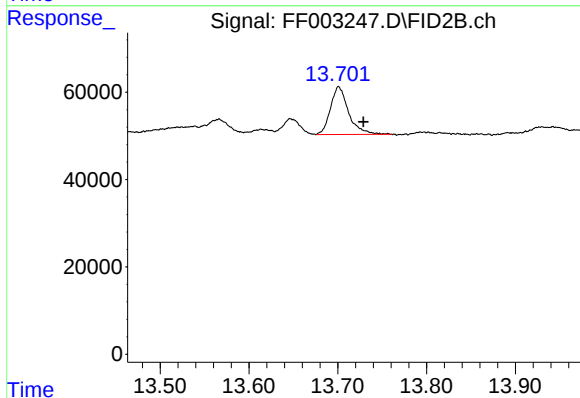


#8 N-DOCOSANE

R.T.: 13.701 min
Delta R.T.: -0.028 min
Response: 154968
Conc: 0.95 ug/ml

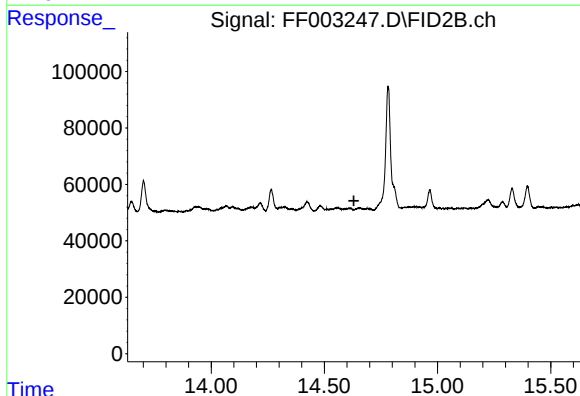


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.630 min
Response: 0
Conc: N.D.

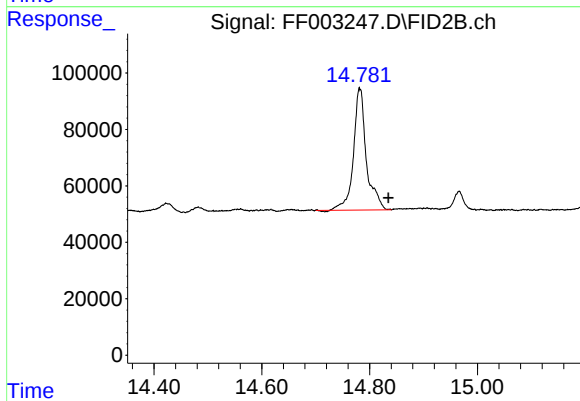

#10 N-TETRACOSANE


R.T.: 14.782 min
Delta R.T.: -0.053 min
Response: 719831
Conc: 4.49 ug/ml

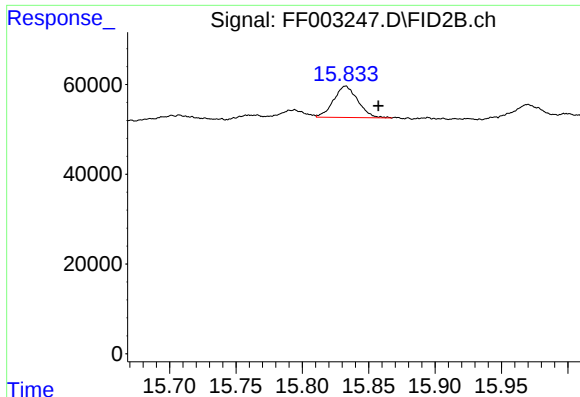

#11 N-HEXACOSANE


R.T.: 15.833 min
Delta R.T.: -0.025 min
Response: 88286
Conc: 0.56 ug/ml

Instrument :
FID_F
ClientSampleId :

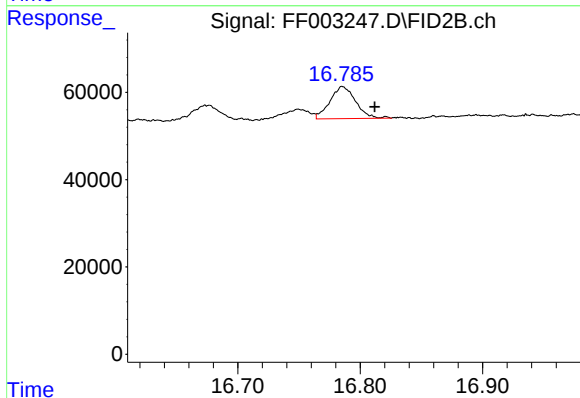


#12 N-OCTACOSANE

R.T.: 16.786 min
Delta R.T.: -0.026 min
Response: 106758
Conc: 0.68 ug/ml

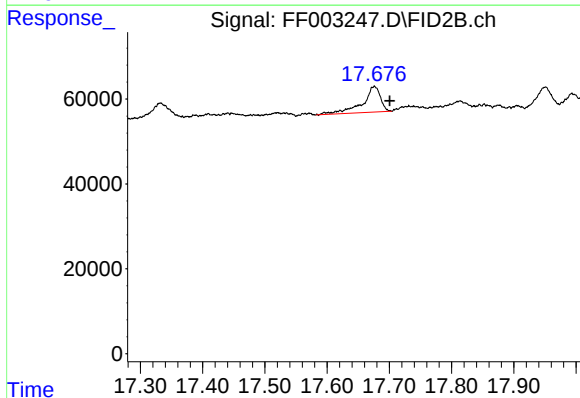

#13 N-TRIACONTANE

R.T.: 17.676 min
Delta R.T.: -0.025 min
Response: 120815
Conc: 0.77 ug/ml

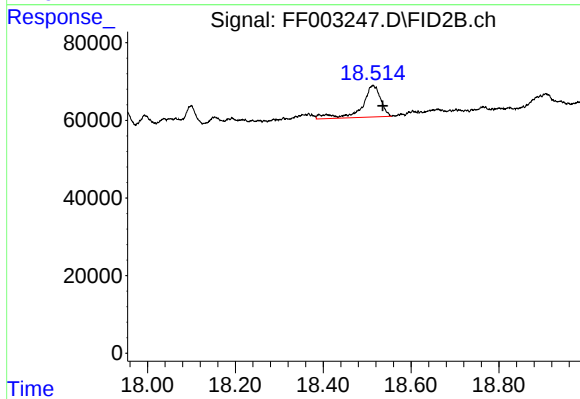

#14 N-DOTRIACONTANE

R.T.: 18.514 min
Delta R.T.: -0.022 min
Response: 239995
Conc: 1.65 ug/ml