

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF011519\
 Data File : FF003250.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jan 2019 10:13
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 15 14:04:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.368	3105734	19.146 ug/ml
12) N-OCTACOSANE	16.789	2746968	17.440 ug/ml
13) N-TRIACONTANE	17.678	114382	0.729 ug/ml
14) N-DOTRIACONTANE	18.512	107414	0.739 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF011519\
Data File : FF003250.D
Signal(s) : FID2B.ch
Acq On : 15 Jan 2019 10:13
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 15 14:04:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

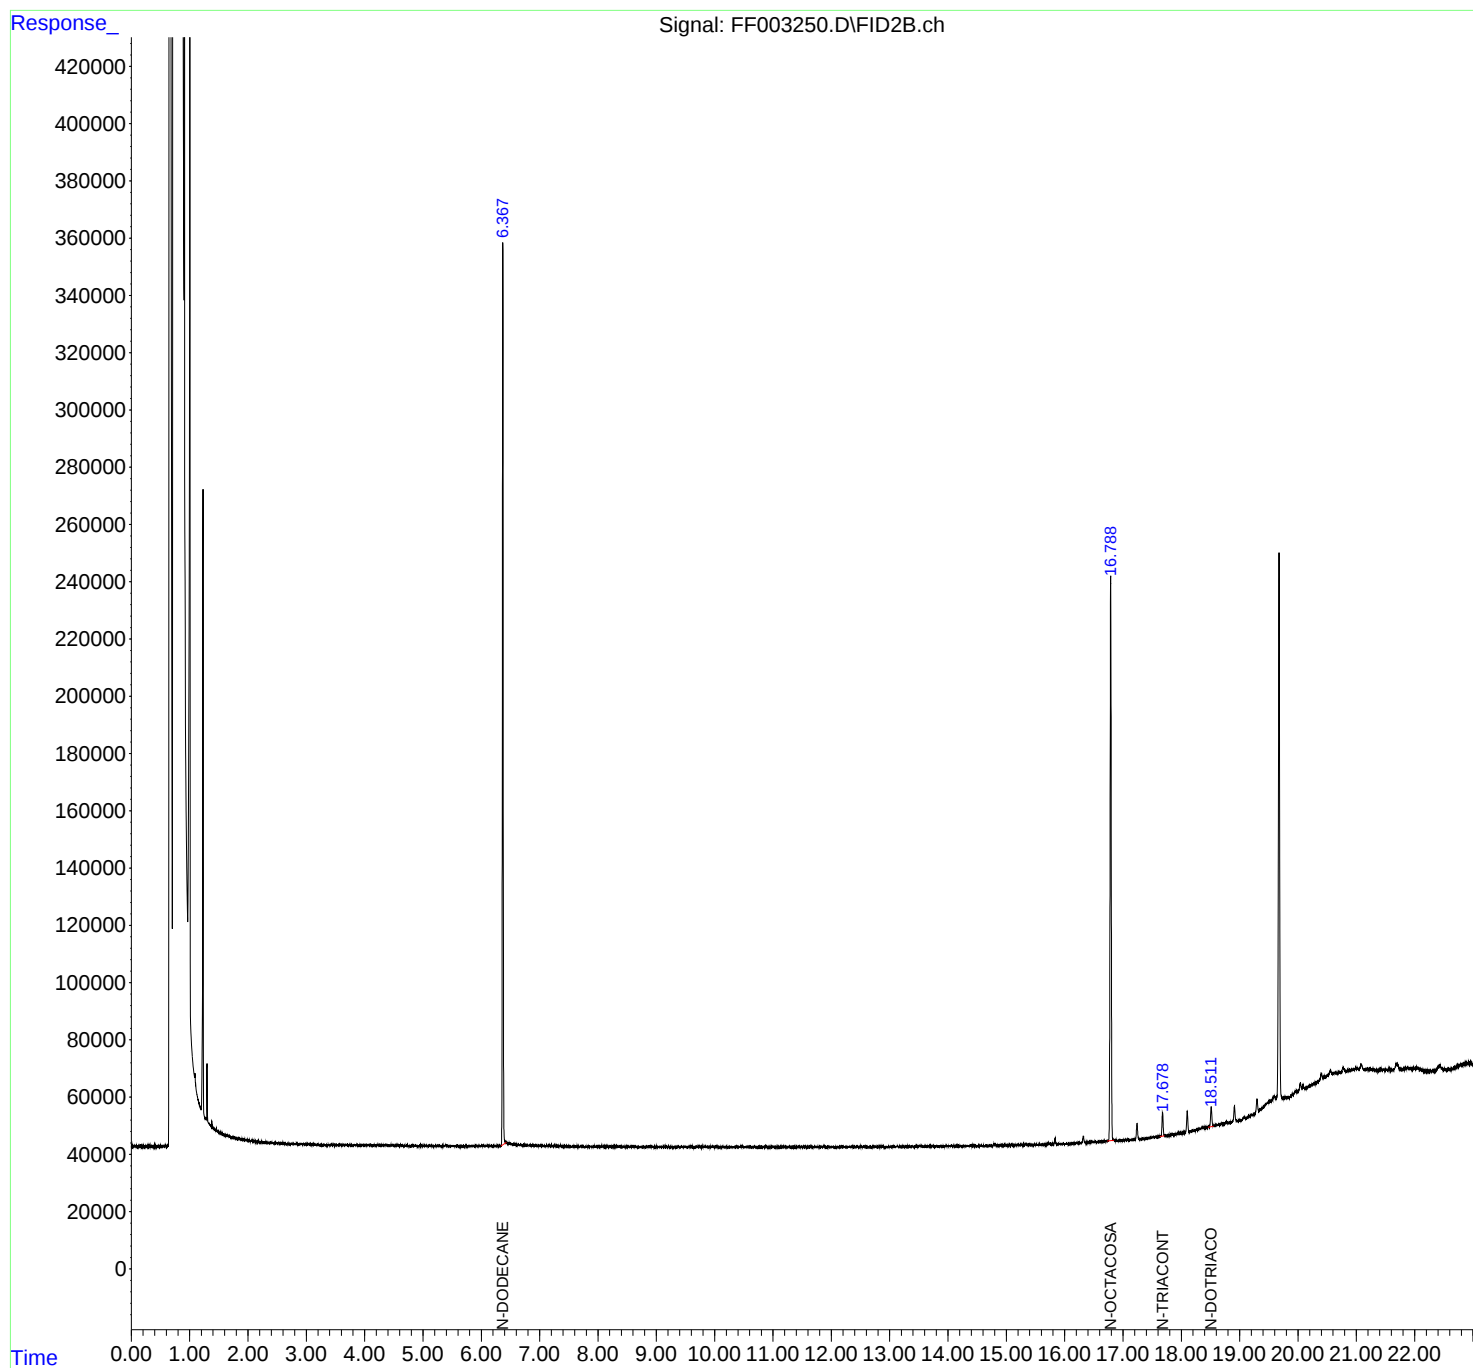


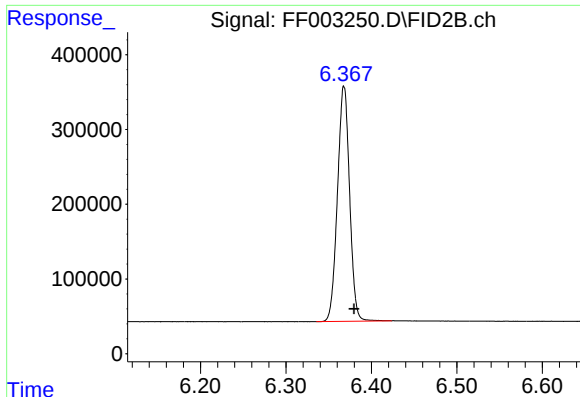

#3 N-DODECANE


R.T.: 6.368 min
Delta R.T.: -0.012 min
Response: 3105734
Conc: 19.15 ug/ml

Instrument :
FID_F
ClientSampleId :

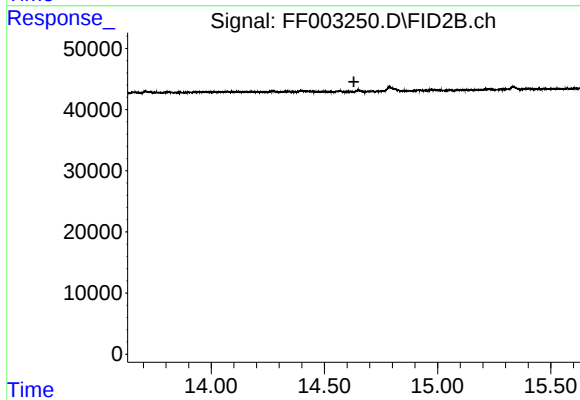


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.630 min
Response: 0
Conc: N.D.

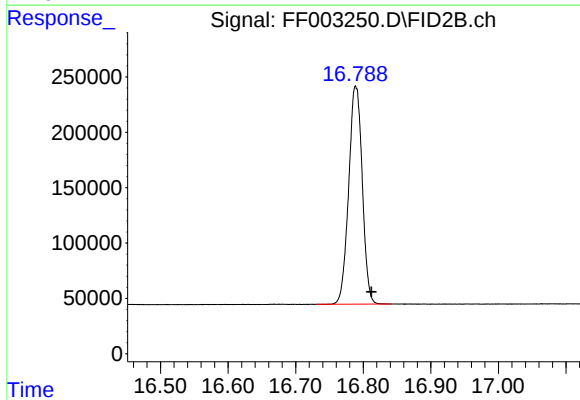


#12 N-OCTACOSANE

R.T.: 16.789 min
Delta R.T.: -0.023 min
Response: 2746968
Conc: 17.44 ug/ml

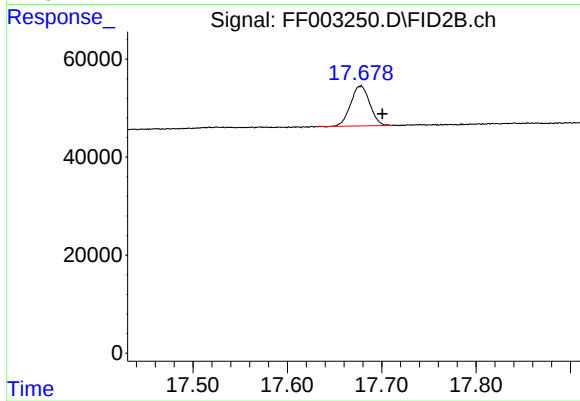

#13 N-TRIACONTANE

R.T.: 17.678 min
Delta R.T.: -0.023 min
Response: 114382
Conc: 0.73 ug/ml

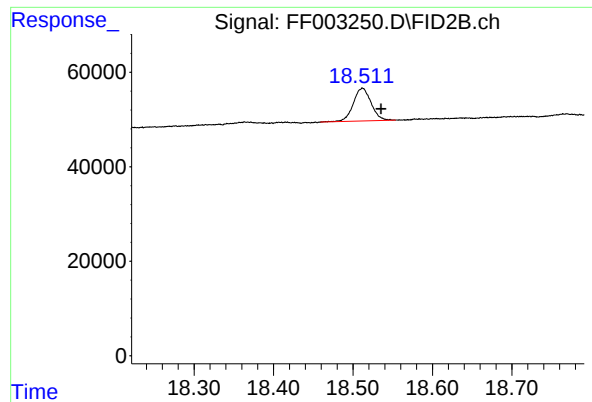

#14 N-DOTRIACONTANE

R.T.: 18.512 min
Delta R.T.: -0.023 min
Response: 107414
Conc: 0.74 ug/ml

Instrument :
FID_F
ClientSampleId :