

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011519\
 Data File : FF003252.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jan 2019 12:05
 Operator : AJ\SJ
 Sample : PB116288BSD
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB116288BSD

Integration File: autoint1.e
 Quant Time: Jan 15 14:05:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.609	2309442	16.140 ug/ml
Target Compounds			
2) N-DECANE	4.340	3244484	20.062 ug/ml
3) N-DODECANE	6.360	3295014	20.312 ug/ml
4) N-TETRADECANE	8.153	3225284	19.752 ug/ml
5) N-HEXADECANE	9.753	3175173	19.337 ug/ml
6) N-OCTADECANE	11.196	3119871	18.867 ug/ml
7) N-EICOSANE	12.508	3037273	18.498 ug/ml
8) N-DOCOSANE	13.707	2965346	18.249 ug/ml
10) N-TETRACOSANE	14.812	2927406	18.253 ug/ml
11) N-HEXACOSANE	15.836	2865079	18.114 ug/ml
12) N-OCTACOSANE	16.789	2868576	18.212 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011519\
Data File : FF003252.D
Signal(s) : FID2B.ch
Acq On : 15 Jan 2019 12:05
Operator : AJ\SJ
Sample : PB116288BSD
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB116288BSD

Integration File: autoint1.e
Quant Time: Jan 15 14:05:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

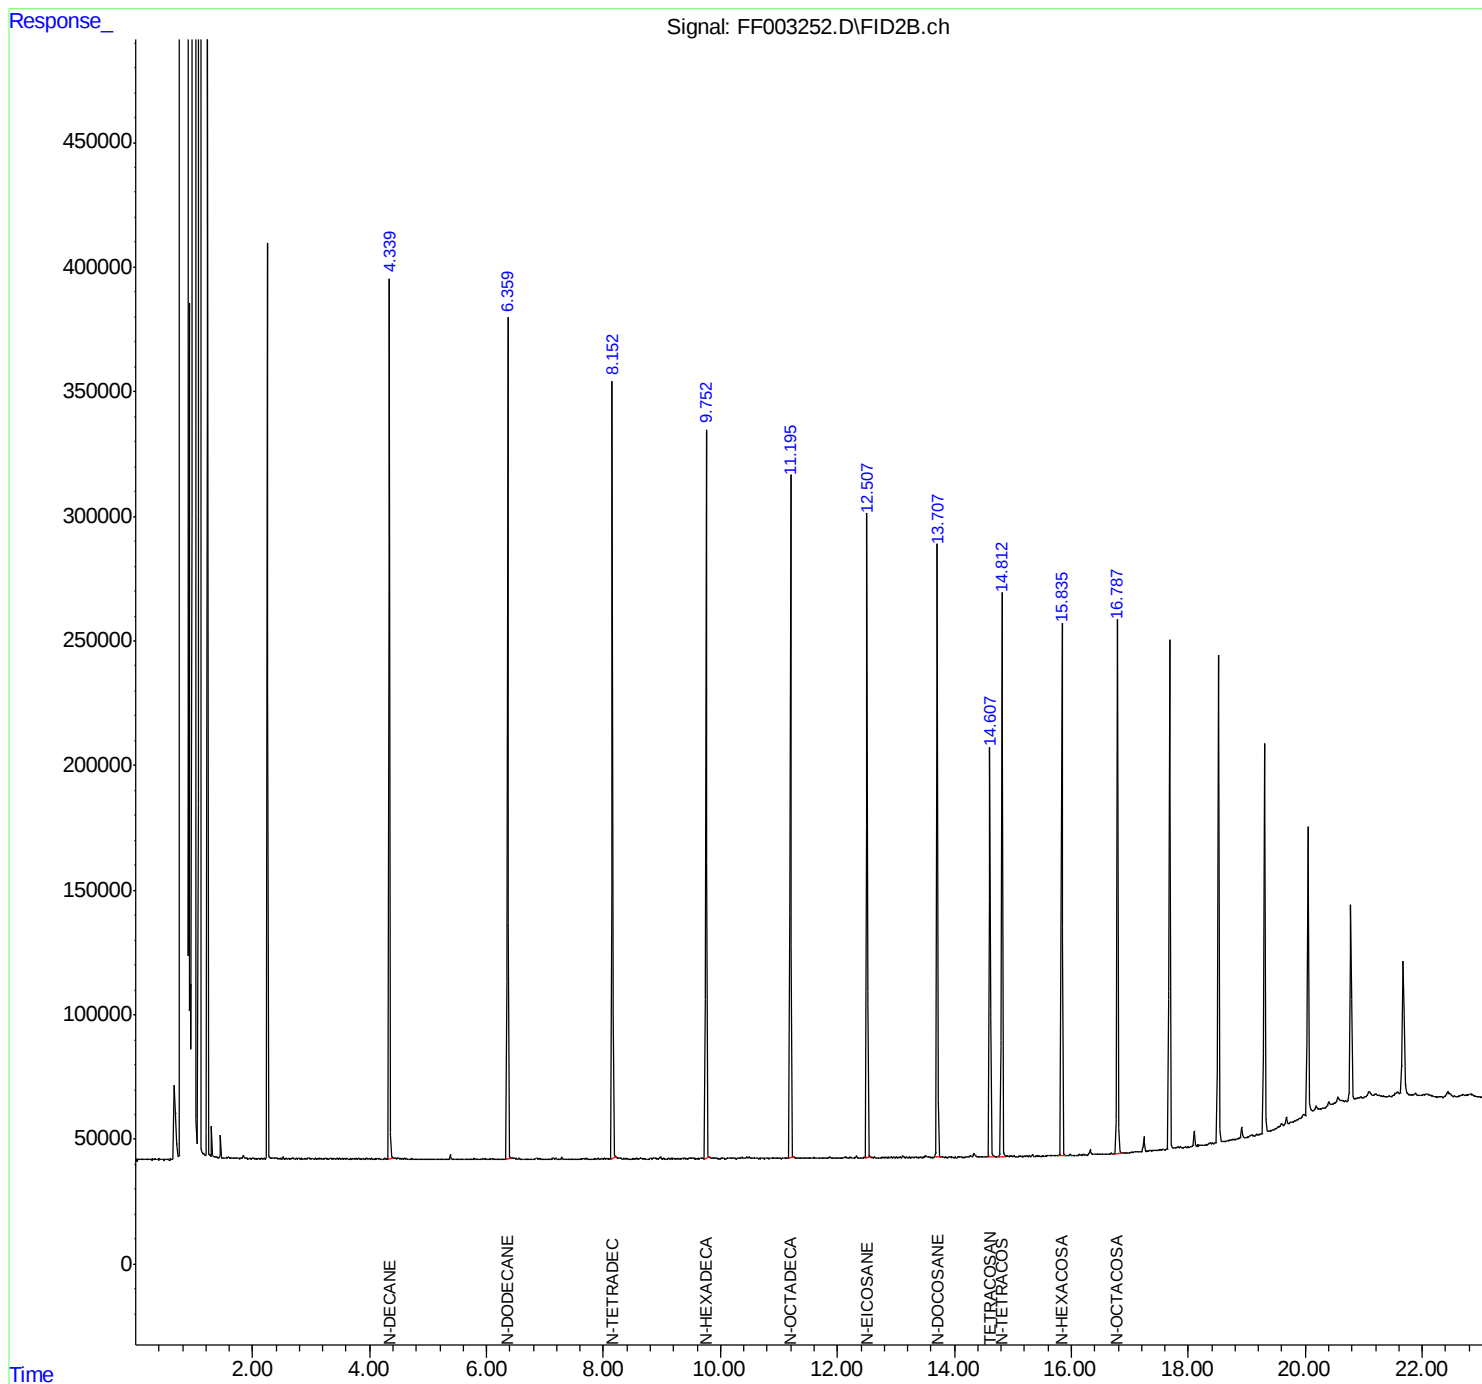


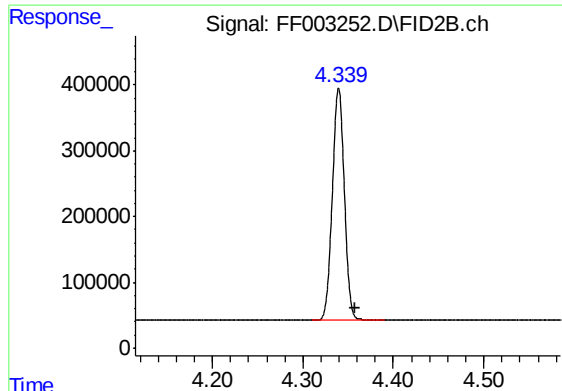

#2 N-DECANE


R.T.: 4.340 min
Delta R.T.: -0.018 min
Response: 3244484
Conc: 20.06 ug/ml

Instrument :
FID_F
ClientSampleId :
PB116288BSD

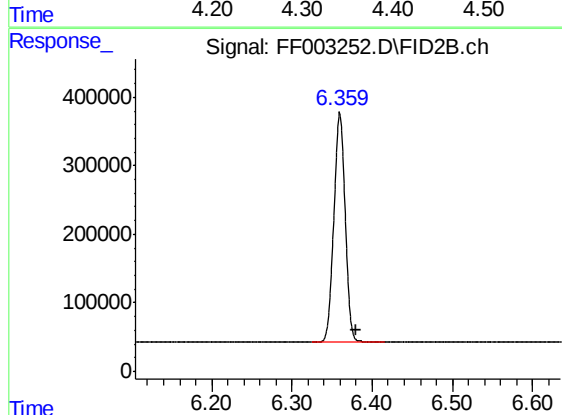


#3 N-DODECANE

R.T.: 6.360 min
Delta R.T.: -0.020 min
Response: 3295014
Conc: 20.31 ug/ml

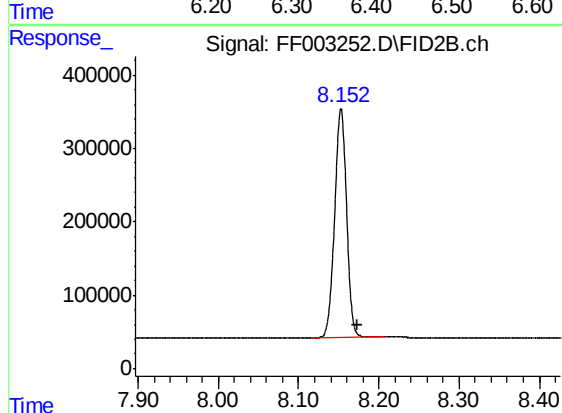


#4 N-TETRADECANE

R.T.: 8.153 min
Delta R.T.: -0.021 min
Response: 3225284
Conc: 19.75 ug/ml

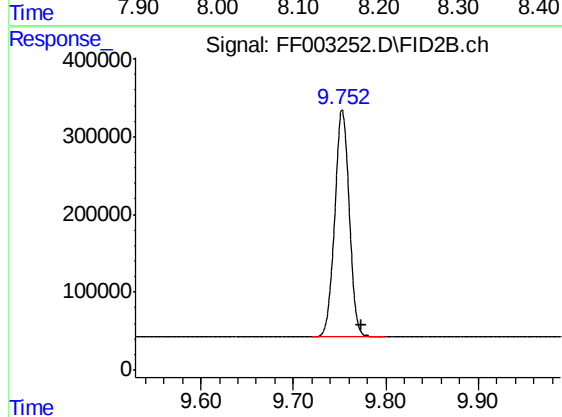

#5 N-HEXADECANE


R.T.: 9.753 min
Delta R.T.: -0.021 min
Response: 3175173
Conc: 19.34 ug/ml

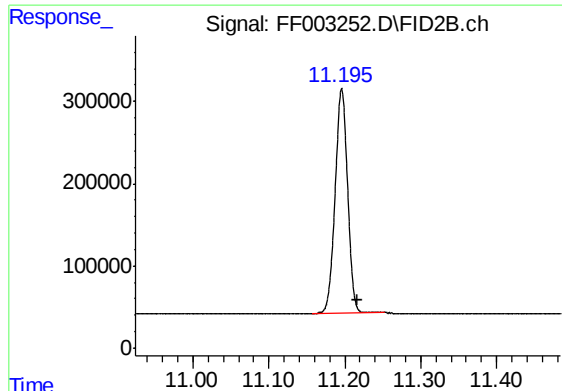

#6 N-OCTADECANE


R.T.: 11.196 min
Delta R.T.: -0.020 min
Response: 3119871
Conc: 18.87 ug/ml

Instrument :
FID_F
ClientSampleId :
PB116288BSD

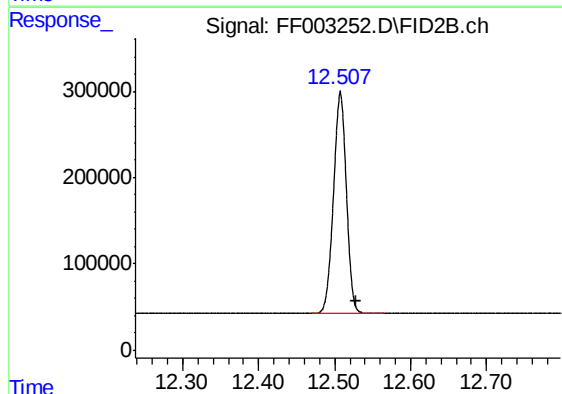


#7 N-EICOSANE

R.T.: 12.508 min
Delta R.T.: -0.020 min
Response: 3037273
Conc: 18.50 ug/ml

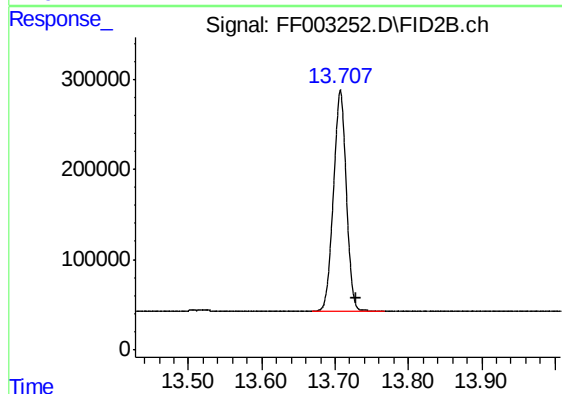


#8 N-DOCOSANE

R.T.: 13.707 min
Delta R.T.: -0.021 min
Response: 2965346
Conc: 18.25 ug/ml

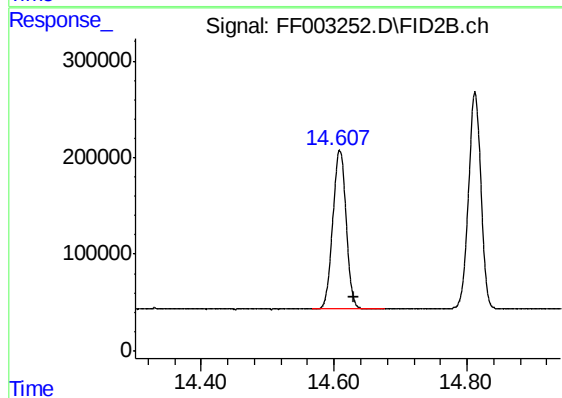

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.609 min
Delta R.T.: -0.022 min
Response: 2309442
Conc: 16.14 ug/ml

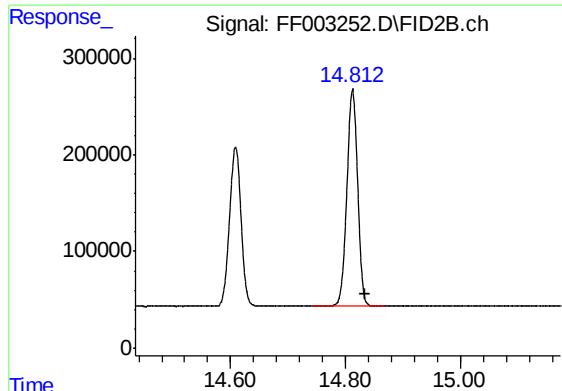

#10 N-TETRACOSANE


R.T.: 14.812 min
Delta R.T.: -0.023 min
Response: 2927406
Conc: 18.25 ug/ml

Instrument :
FID_F
ClientSampleId :
PB116288BSD

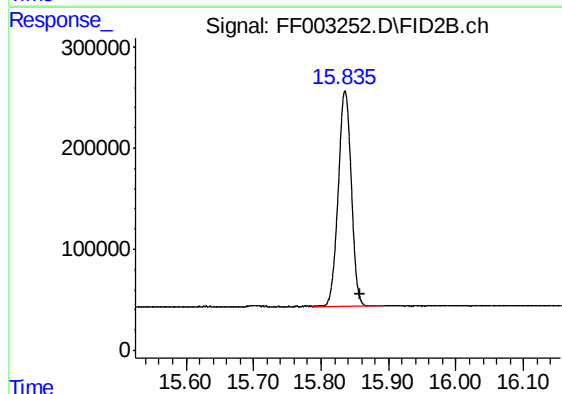

#11 N-HEXACOSANE

R.T.: 15.836 min
Delta R.T.: -0.022 min
Response: 2865079
Conc: 18.11 ug/ml

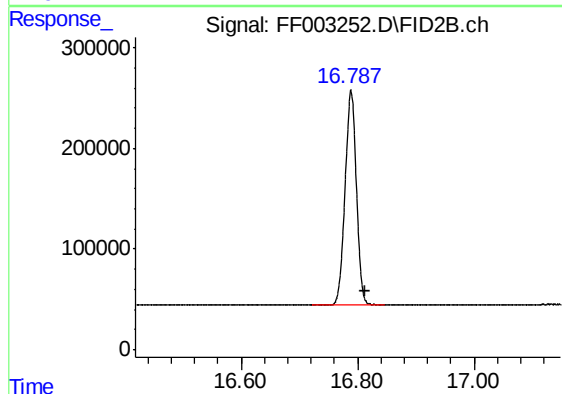

#12 N-OCTACOSANE

R.T.: 16.789 min
Delta R.T.: -0.023 min
Response: 2868576
Conc: 18.21 ug/ml