

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011521\
 Data File : FF008093.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jan 2021 11:10
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Jan 15 22:03:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010421.M
 Quant Title :
 QLast Update : Tue Jan 05 12:03:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.419	3558313	27.679 ug/ml
12) N-OCTACOSANE	16.853	3530136	25.823 ug/ml
13) N-TRIACONTANE	17.740	291709	2.224 ug/ml
14) N-DOTRIACONTANE	18.575	386189	3.281 ug/ml
15) N-TETRATRIACONTANE	19.358	271169	2.864 ug/ml
16) N-HEXATRIACONTANE	20.099	175044	2.415 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011521\
Data File : FF008093.D
Signal(s) : FID2B.ch
Acq On : 15 Jan 2021 11:10
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jan 15 22:03:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010421.M
Quant Title :
QLast Update : Tue Jan 05 12:03:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

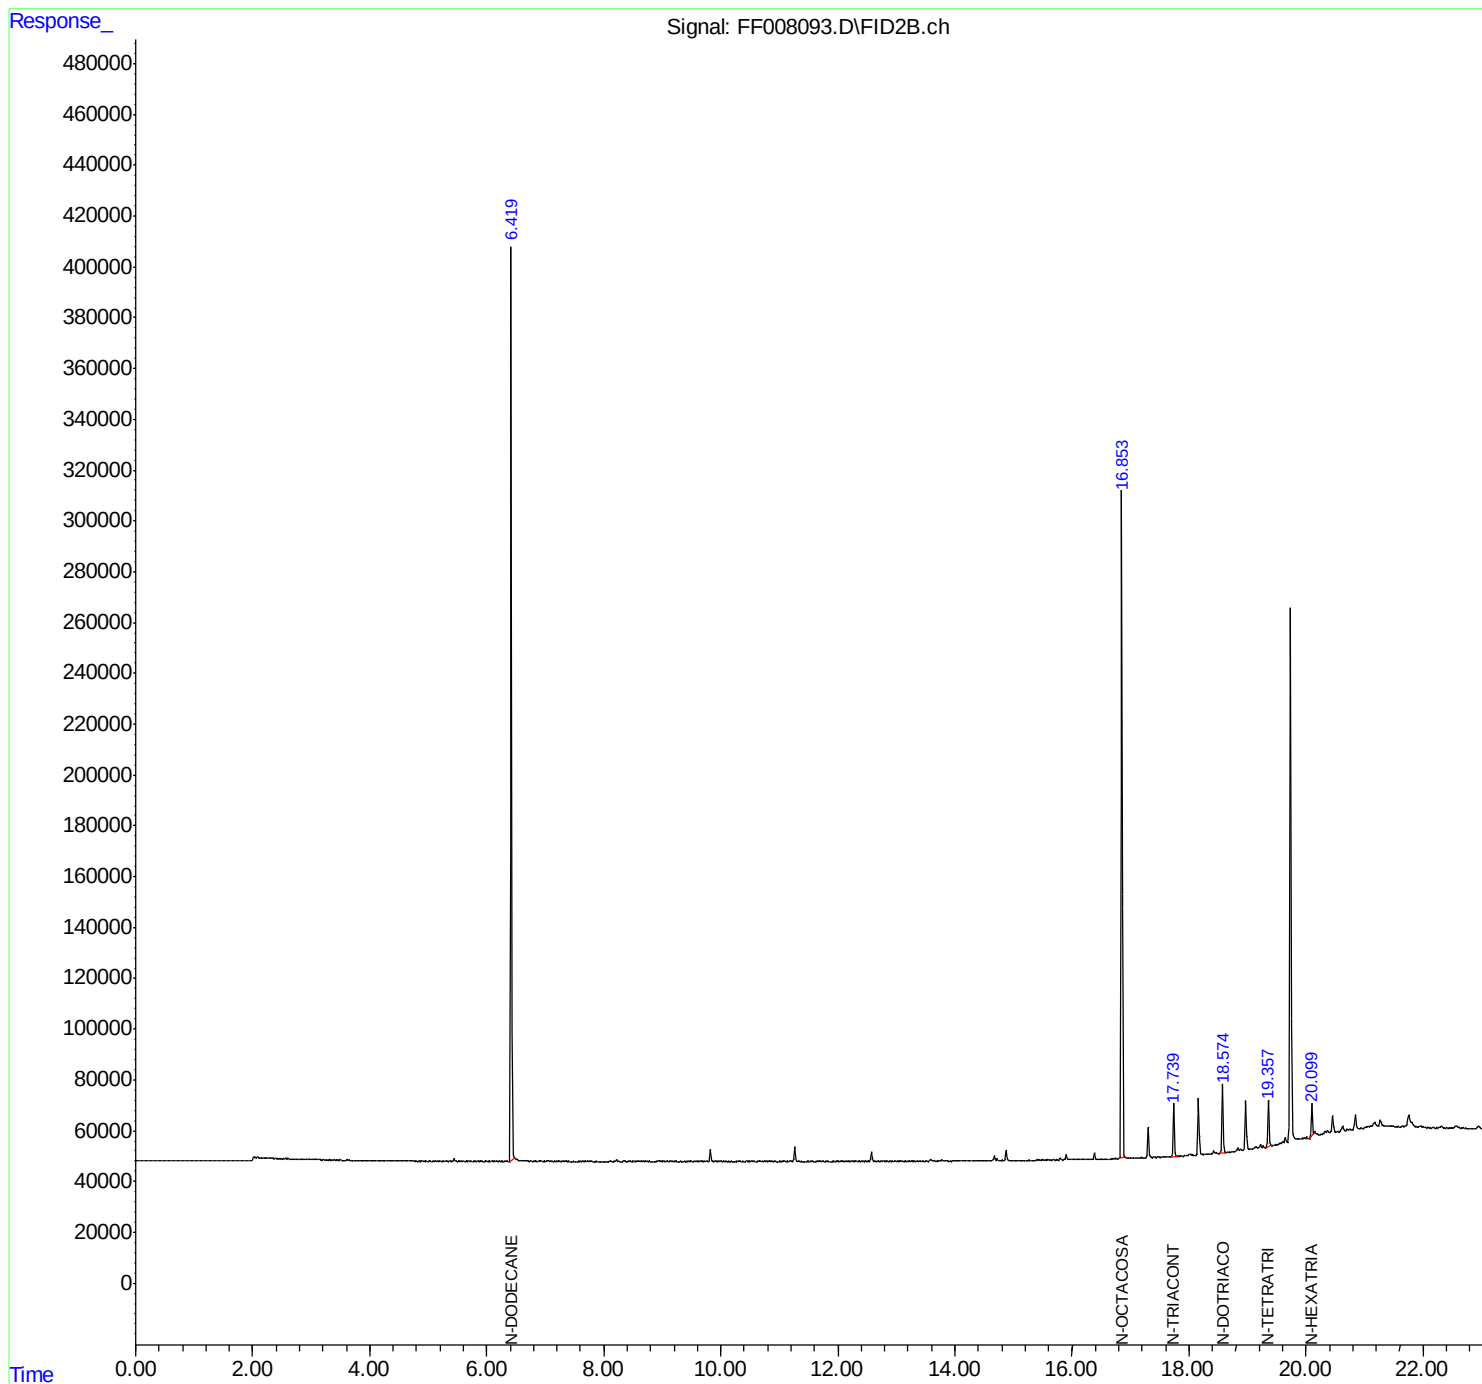


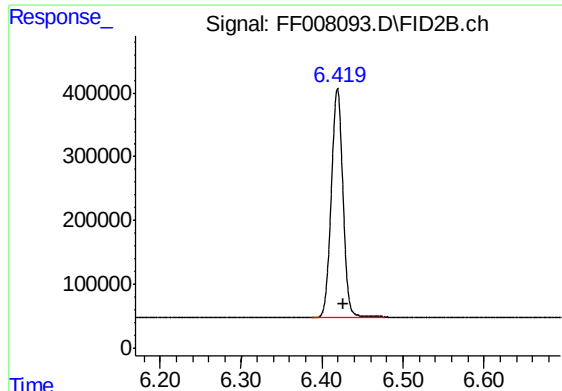

#3 N-DODECANE


R.T.: 6.419 min
Delta R.T.: -0.007 min
Response: 3558313
Conc: 27.68 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

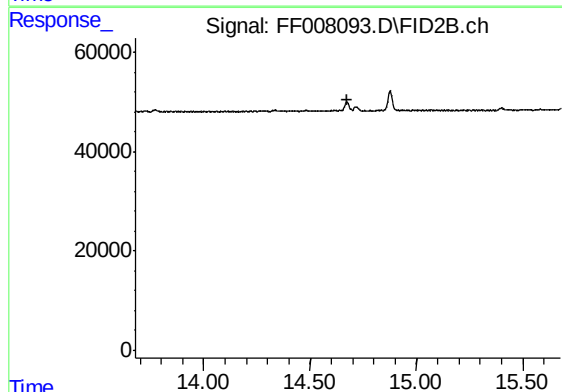


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.678 min
Response: 0
Conc: N.D.

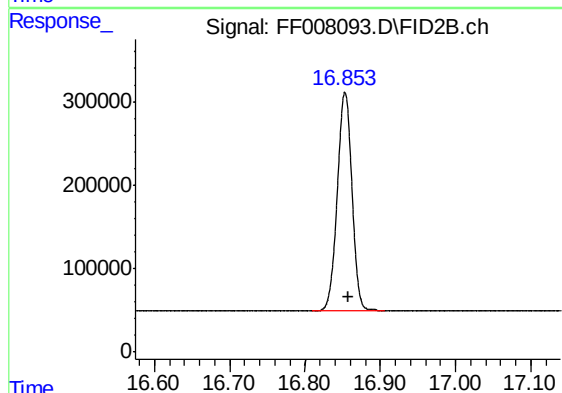


#12 N-OCTACOSANE

R.T.: 16.853 min
Delta R.T.: -0.004 min
Response: 3530136
Conc: 25.82 ug/ml

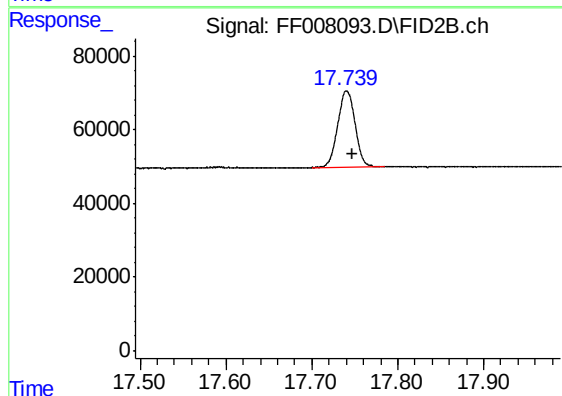

#13 N-TRIACONTANE


R.T.: 17.740 min
Delta R.T.: -0.007 min
Response: 291709
Conc: 2.22 ug/ml

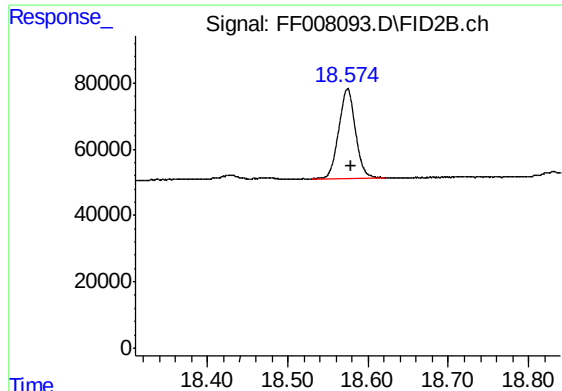

#14 N-DOTRIACONTANE


R.T.: 18.575 min
Delta R.T.: -0.005 min
Response: 386189
Conc: 3.28 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

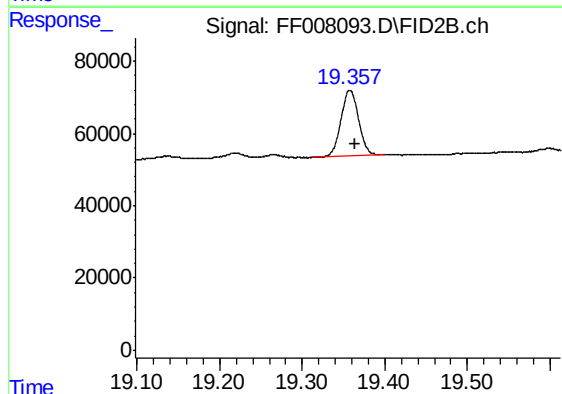

#15 N-TETRATRIACONTANE

R.T.: 19.358 min
Delta R.T.: -0.007 min
Response: 271169
Conc: 2.86 ug/ml

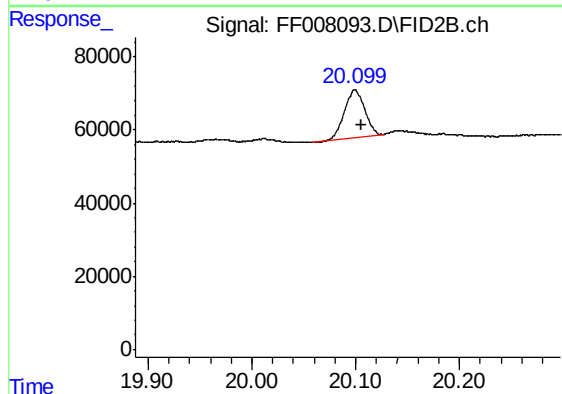

#16 N-HEXATRIACONTANE

R.T.: 20.099 min
Delta R.T.: -0.006 min
Response: 175044
Conc: 2.42 ug/ml