

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011521\
Data File : FF008096.D
Signal(s) : FID2B.ch
Acq On : 15 Jan 2021 13:27
Operator : DD\AJ
Sample : M1146-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
520-Z

Integration File: autoint1.e
Quant Time: Jan 15 22:03:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010421.M
Quant Title :
QLast Update : Tue Jan 05 12:03:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.673	2472354	19.967 ug/ml
Target Compounds			
4) N-TETRADECANE	8.183	640971	4.741 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011521\
Data File : FF008096.D
Signal(s) : FID2B.ch
Acq On : 15 Jan 2021 13:27
Operator : DD\AJ
Sample : M1146-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
520-Z

Integration File: autoint1.e
Quant Time: Jan 15 22:03:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010421.M
Quant Title :
QLast Update : Tue Jan 05 12:03:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

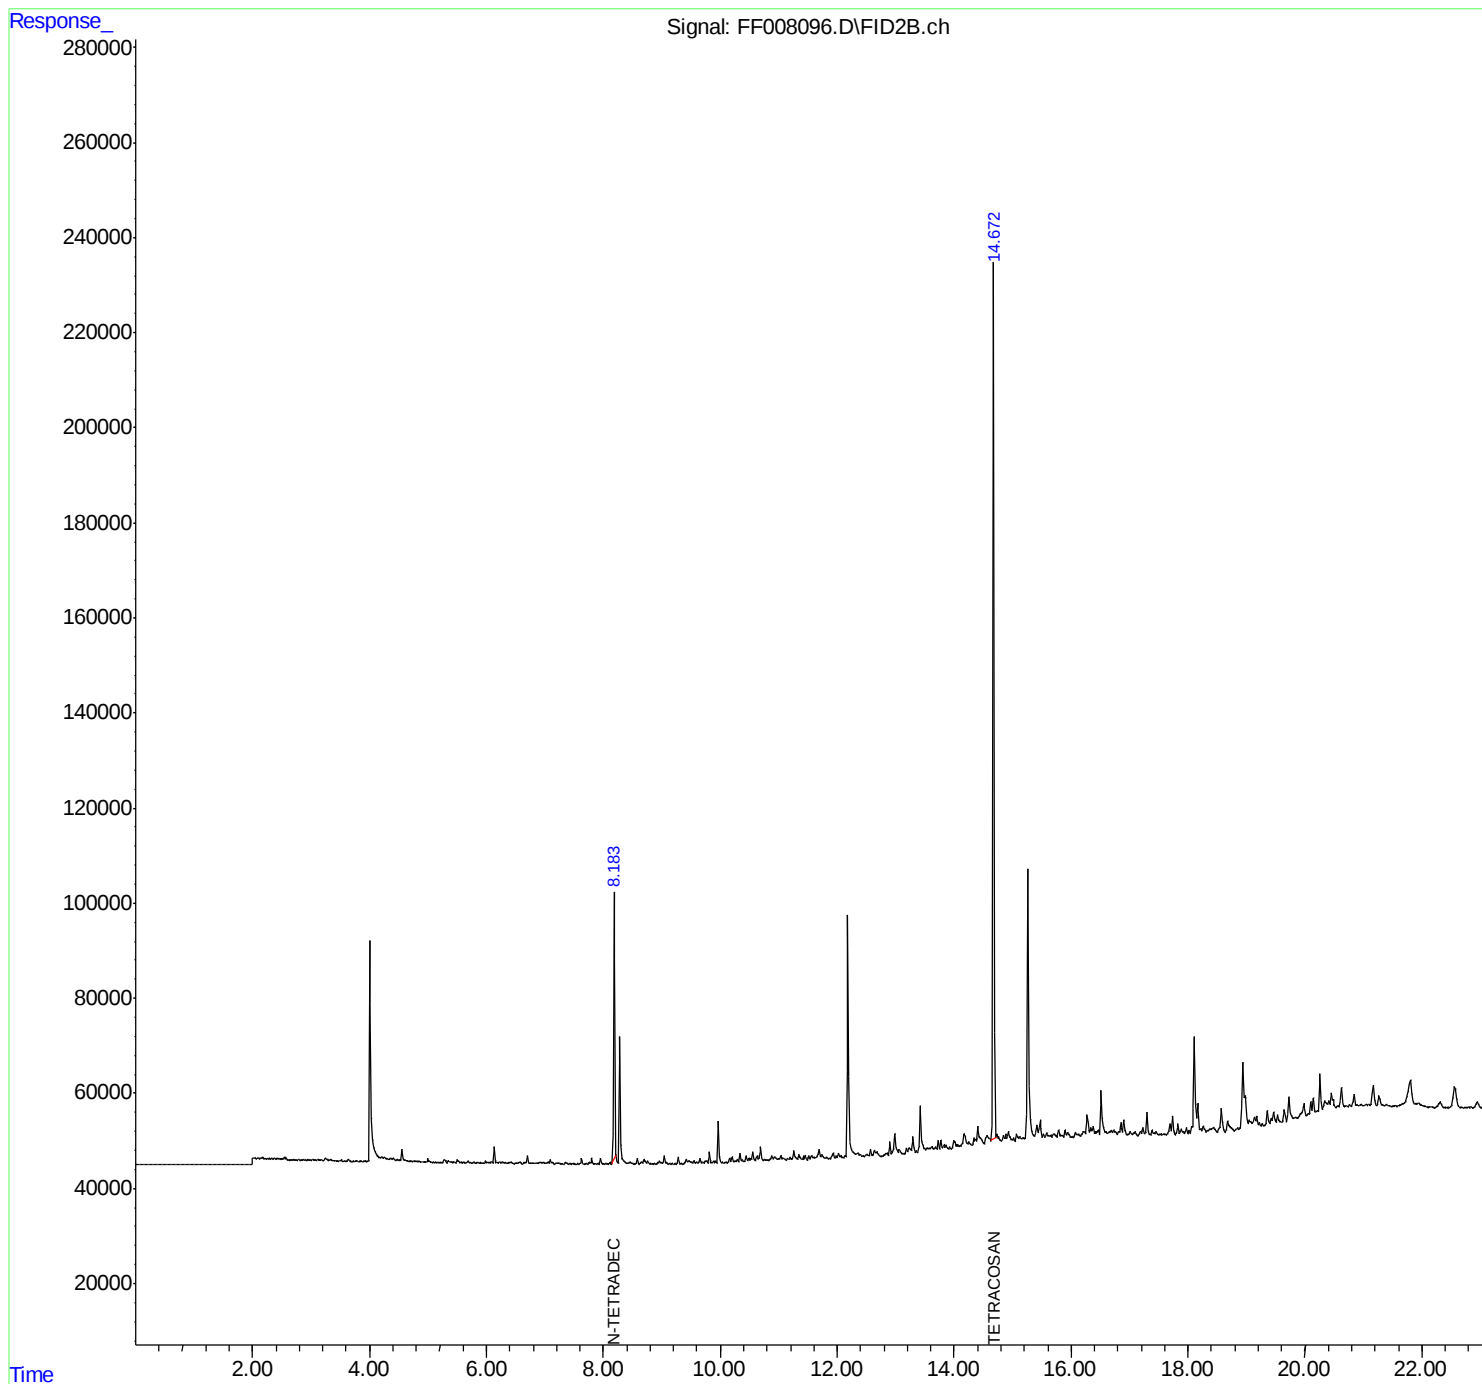


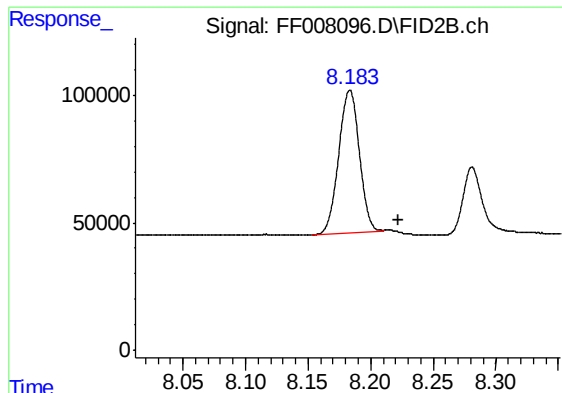

#4 N-TETRADECANE

R.T.: 8.183 min
Delta R.T.: -0.038 min
Response: 640971
Conc: 4.74 ug/ml

Instrument :
FID_F
ClientSampleId :
520-Z

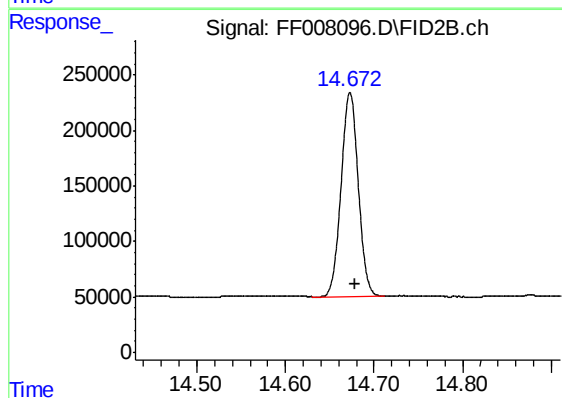

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.673 min
Delta R.T.: -0.005 min
Response: 2472354
Conc: 19.97 ug/ml