

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011619\
Data File : FF003258.D
Signal(s) : FID2B.ch
Acq On : 16 Jan 2019 11:47
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 16 23:47:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.366	3343950	20.614 ug/ml
12)	N-OCTACOSANE	16.787	2968399	18.846 ug/ml
13)	N-TRIACONTANE	17.676	199798	1.273 ug/ml
14)	N-DOTRIACONTANE	18.510	210070	1.445 ug/ml
15)	N-TETRATRIACONTANE	19.296	91183	0.690 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011619\
Data File : FF003258.D
Signal(s) : FID2B.ch
Acq On : 16 Jan 2019 11:47
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 16 23:47:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

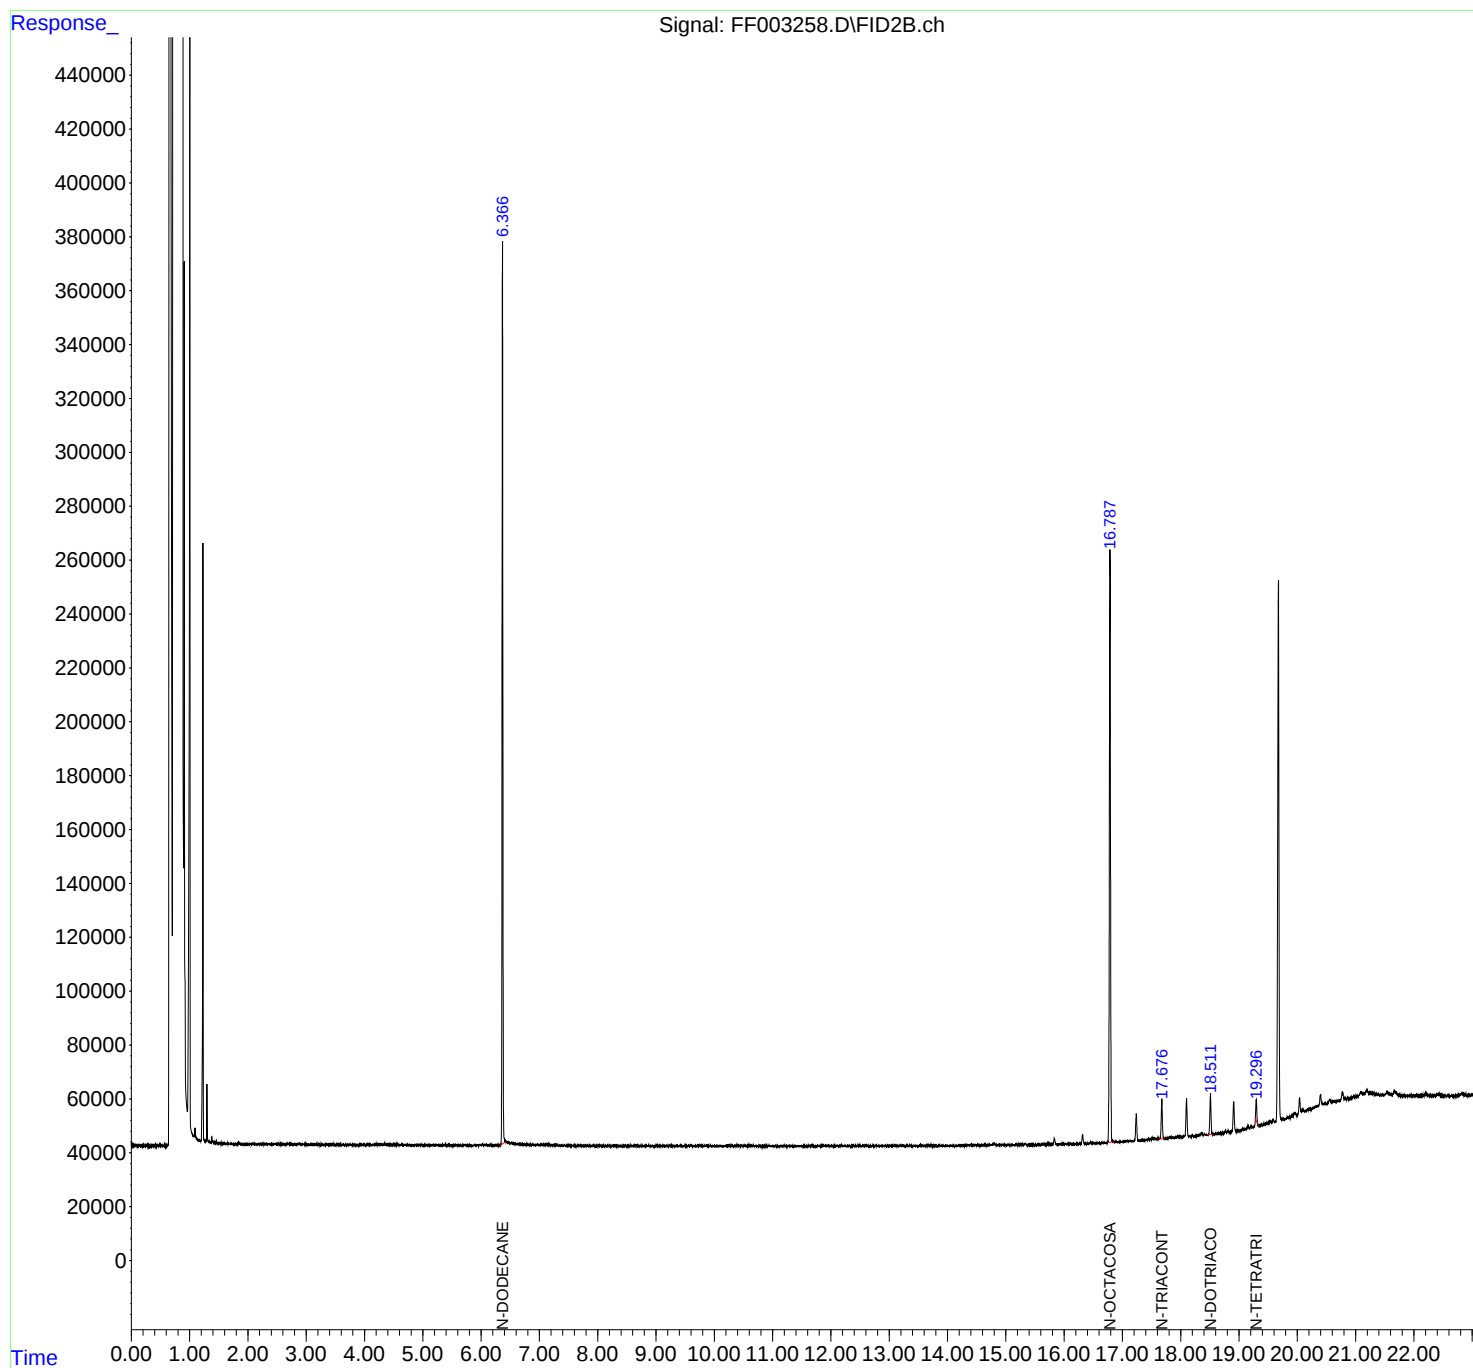

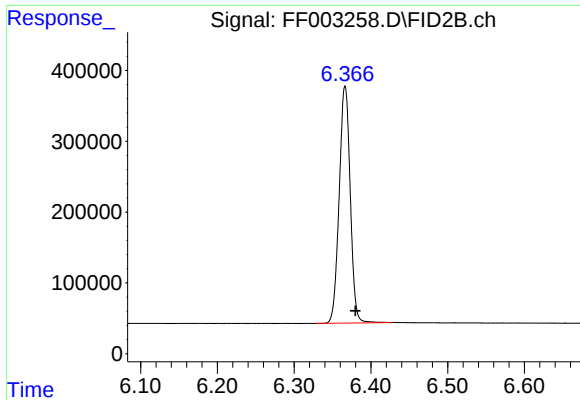


#3 N-DODECANE

R.T.: 6.366 min
Delta R.T.: -0.013 min
Response: 3343950
Conc: 20.61 ug/ml

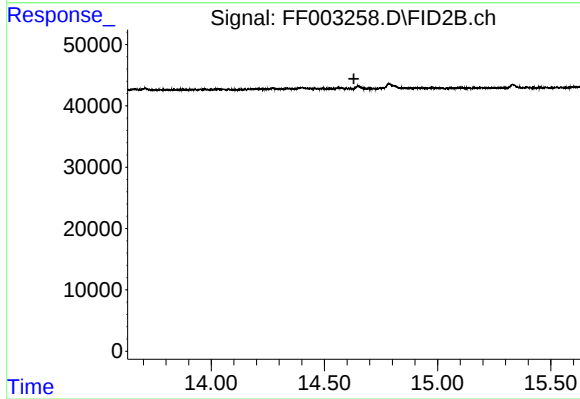


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.630 min
Response: 0
Conc: N.D.

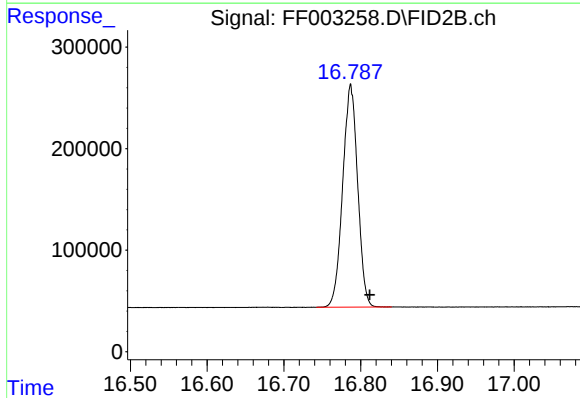


#12 N-OCTACOSANE

R.T.: 16.787 min
Delta R.T.: -0.025 min
Response: 2968399
Conc: 18.85 ug/ml

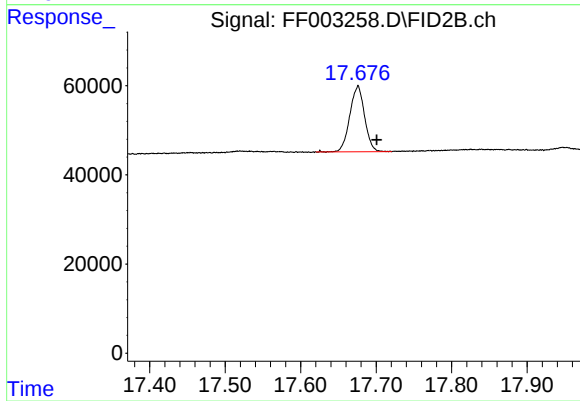


#13 N-TRIACONTANE

R.T.: 17.676 min
Delta R.T.: -0.025 min
Response: 199798
Conc: 1.27 ug/ml

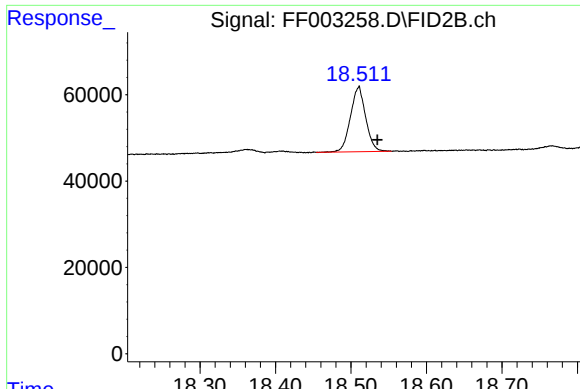

#14 N-DOTRIACONTANE

R.T.: 18.510 min
Delta R.T.: -0.025 min
Response: 210070
Conc: 1.44 ug/ml

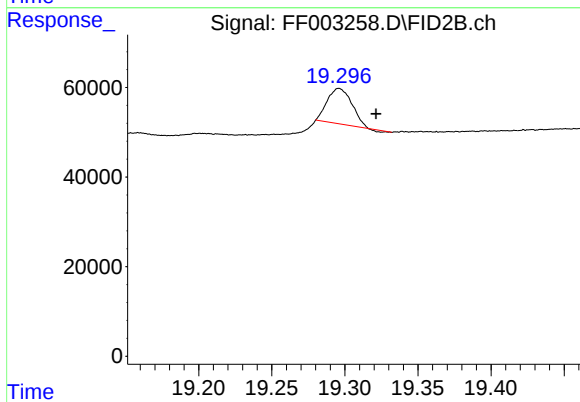

#15 N-TETRATRIACONTANE

R.T.: 19.296 min
Delta R.T.: -0.025 min
Response: 91183
Conc: 0.69 ug/ml