

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
 Data File : FF003268.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jan 2019 09:25
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 17 23:38:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.612	2113863	14.773 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.678	131961	0.841 ug/ml
14) N-DOTRIACONTANE	18.514	165685	1.139 ug/ml
15) N-TETRATRIACONTANE	19.301	97146	0.735 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
Data File : FF003268.D
Signal(s) : FID2B.ch
Acq On : 17 Jan 2019 09:25
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 17 23:38:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

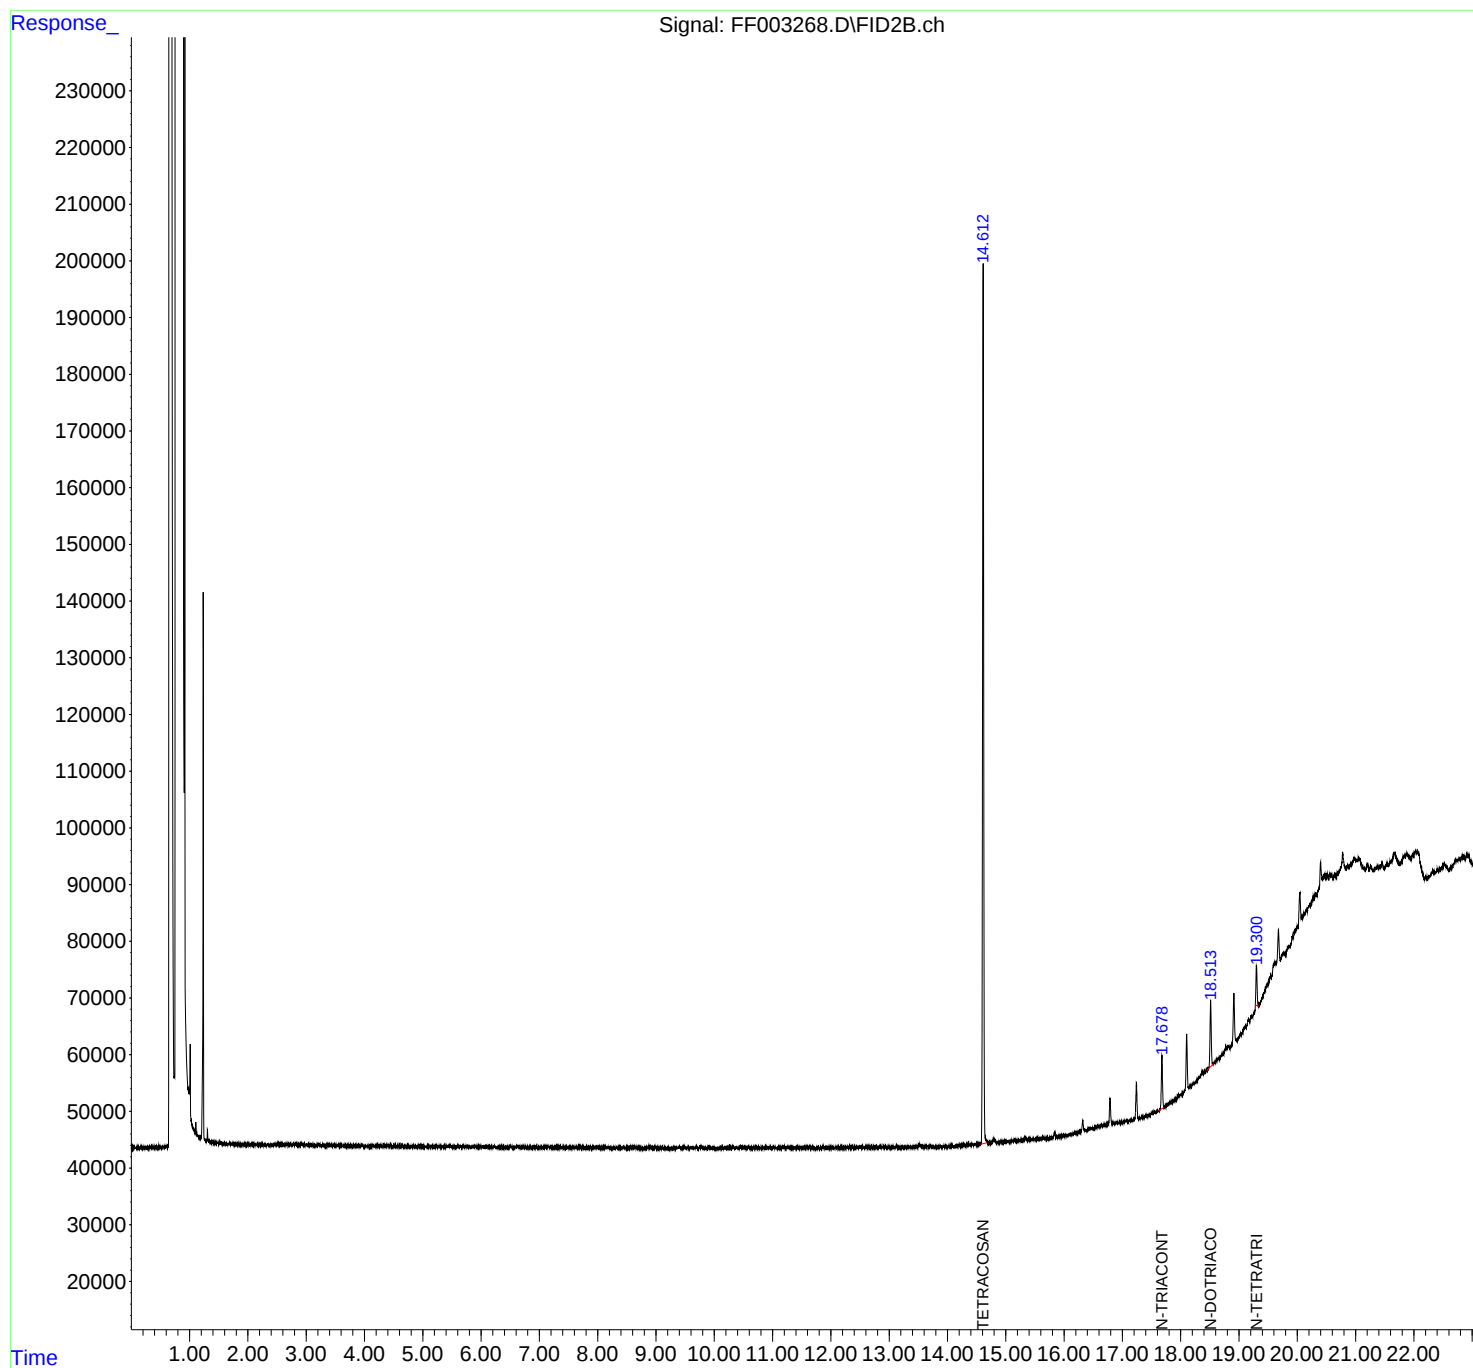


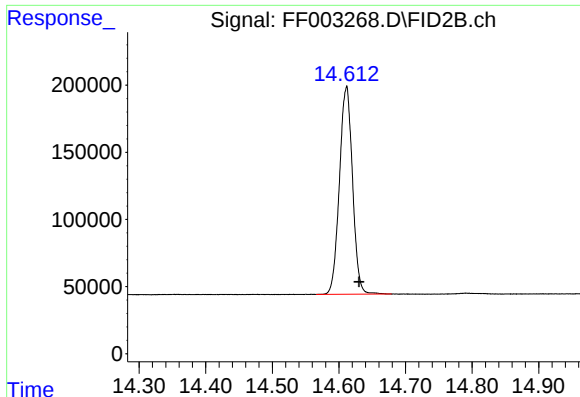

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.612 min
Delta R.T.: -0.019 min
Response: 2113863
Conc: 14.77 ug/ml

Instrument :
FID_F
ClientSampleId :

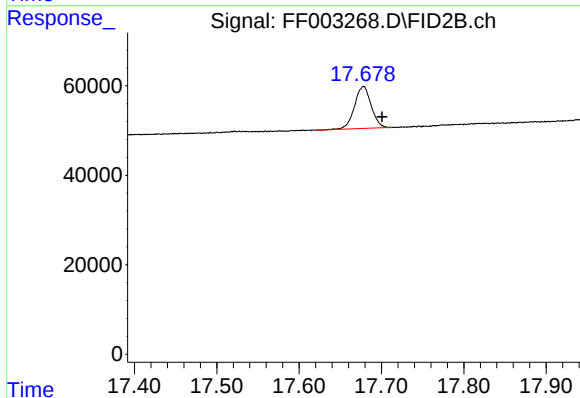


#13 N-TRIACONTANE

R.T.: 17.678 min
Delta R.T.: -0.022 min
Response: 131961
Conc: 0.84 ug/ml

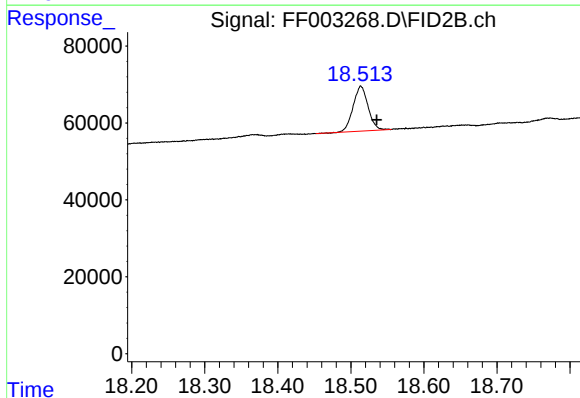

#14 N-DOTRIACONTANE

R.T.: 18.514 min
Delta R.T.: -0.021 min
Response: 165685
Conc: 1.14 ug/ml

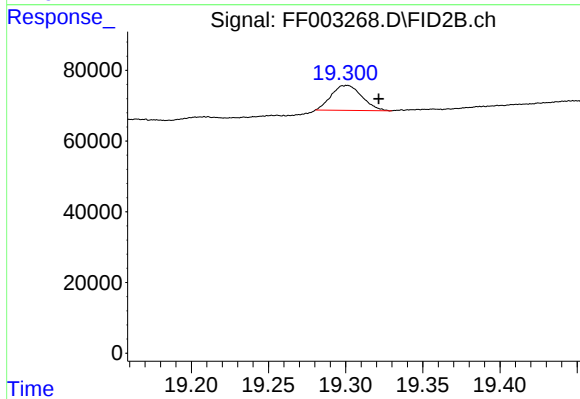

#15 N-TETRATRIACONTANE

R.T.: 19.301 min
Delta R.T.: -0.021 min
Response: 97146
Conc: 0.73 ug/ml