

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
Data File : FF003270.D
Signal(s) : FID2B.ch
Acq On : 17 Jan 2019 10:37
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 17 23:41:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.361	3468909	21.384 ug/ml
12)	N-OCTACOSANE	16.789	3220420	20.446 ug/ml
13)	N-TRIACONTANE	17.678	306609	1.953 ug/ml
14)	N-DOTRIACONTANE	18.512	340174	2.339 ug/ml
15)	N-TETRATRIACONTANE	19.300	202492	1.532 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
Data File : FF003270.D
Signal(s) : FID2B.ch
Acq On : 17 Jan 2019 10:37
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 17 23:41:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

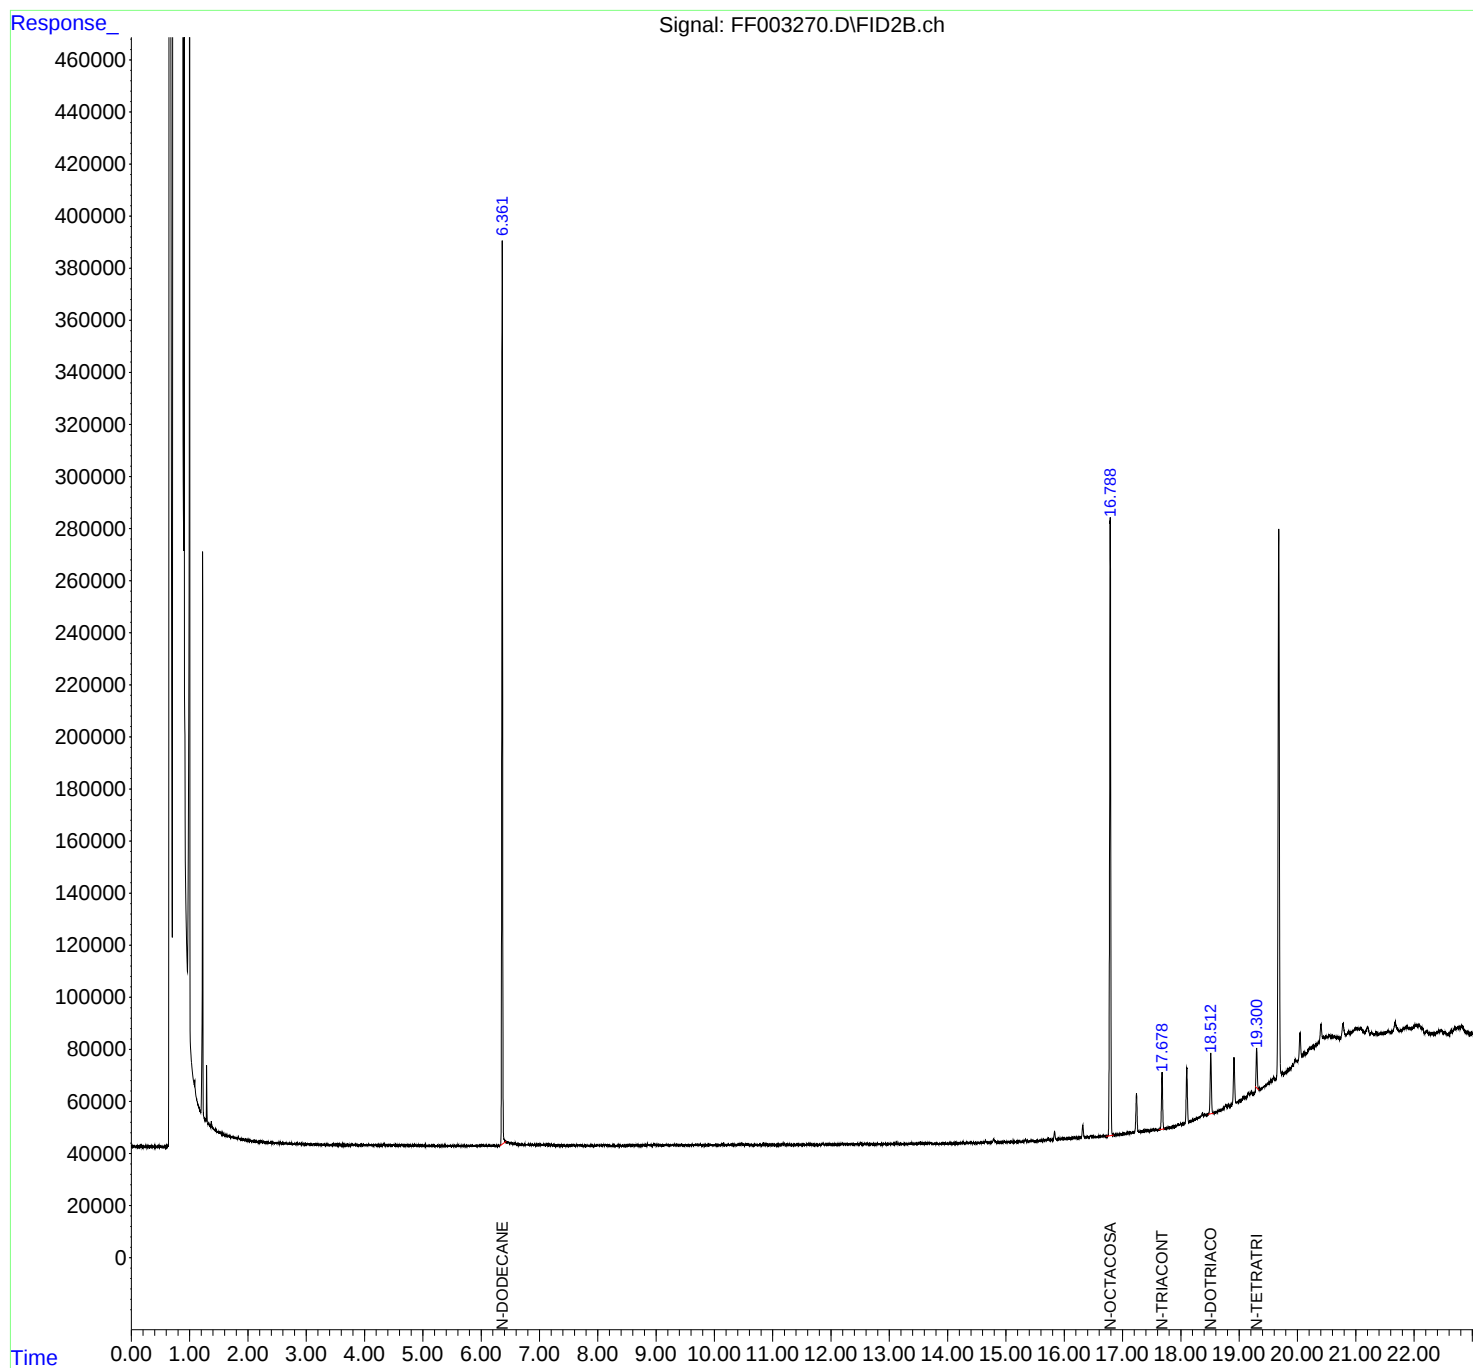


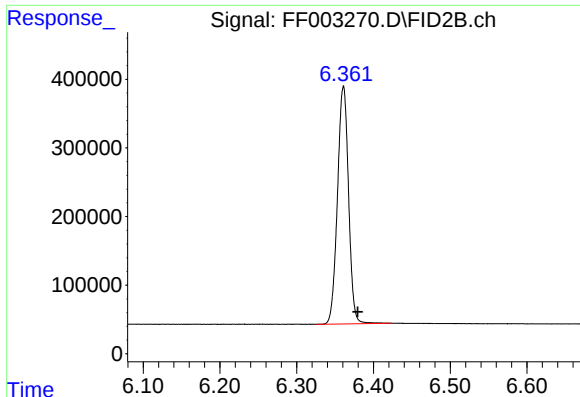

#3 N-DODECANE


R.T.: 6.361 min
Delta R.T.: -0.019 min
Response: 3468909
Conc: 21.38 ug/ml

Instrument :
FID_F
ClientSampleId :

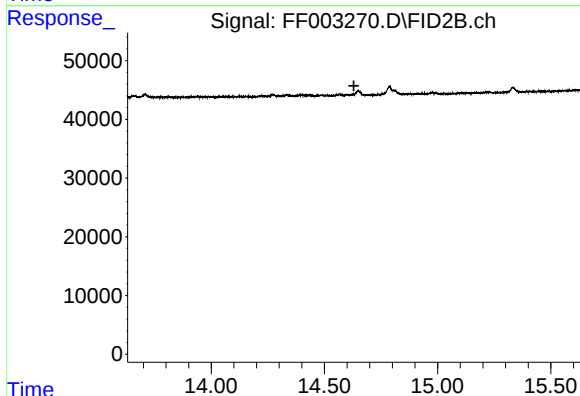


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.630 min
Response: 0
Conc: N.D.

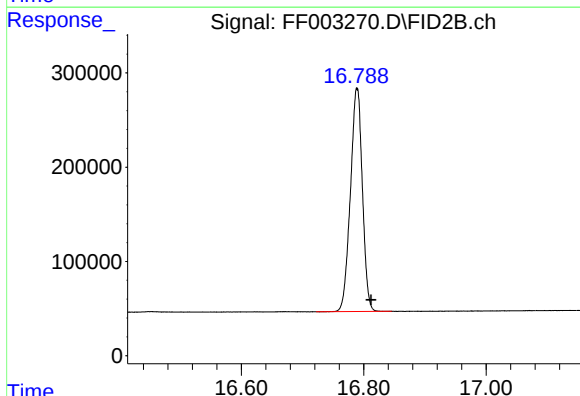


#12 N-OCTACOSANE

R.T.: 16.789 min
Delta R.T.: -0.023 min
Response: 3220420
Conc: 20.45 ug/ml

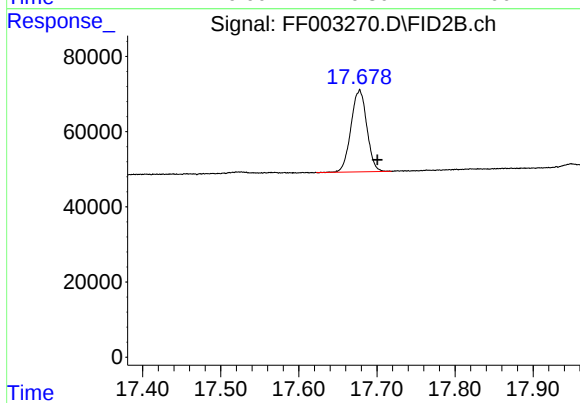

#13 N-TRIACONTANE


R.T.: 17.678 min
Delta R.T.: -0.023 min
Response: 306609
Conc: 1.95 ug/ml

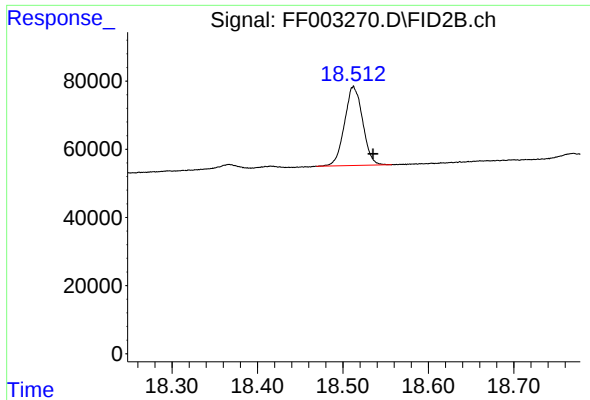

#14 N-DOTRIACONTANE

R.T.: 18.512 min
Delta R.T.: -0.023 min
Response: 340174
Conc: 2.34 ug/ml

Instrument :
FID_F
ClientSampleId :

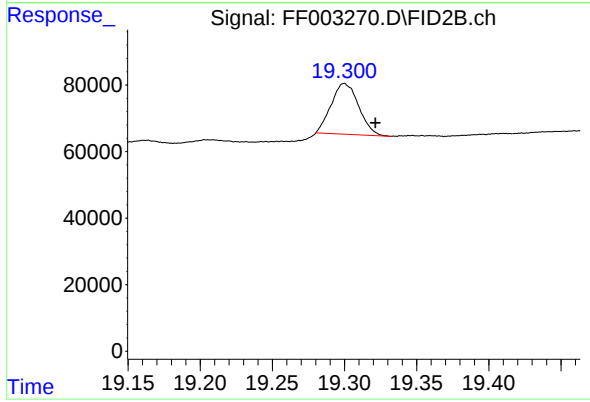

#15 N-TETRATRIACONTANE

R.T.: 19.300 min
Delta R.T.: -0.022 min
Response: 202492
Conc: 1.53 ug/ml