

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
 Data File : FF003274.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jan 2019 14:42
 Operator : AJ\SJ
 Sample : K1157-05
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 17 23:42:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.608	1717795	12.005 ug/ml
Target Compounds			
4) N-TETRADECANE	8.213	933798	5.719 ug/ml
6) N-OCTADECANE	11.213	92165	0.557 ug/ml
7) N-EICOSANE	12.560	335519	2.043 ug/ml
10) N-TETRACOSANE	14.781f	136992	0.854 ug/ml
11) N-HEXACOSANE	15.835	149718	0.947 ug/ml
12) N-OCTACOSANE	16.833	410651	2.607 ug/ml
13) N-TRIACONTANE	17.677	312106	1.988 ug/ml
14) N-DOTRIACONTANE	18.510	457488	3.146 ug/ml
15) N-TETRATRIACONTANE	19.355	83729	0.633 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
Data File : FF003274.D
Signal(s) : FID2B.ch
Acq On : 17 Jan 2019 14:42
Operator : AJ\SJ
Sample : K1157-05
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 17 23:42:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

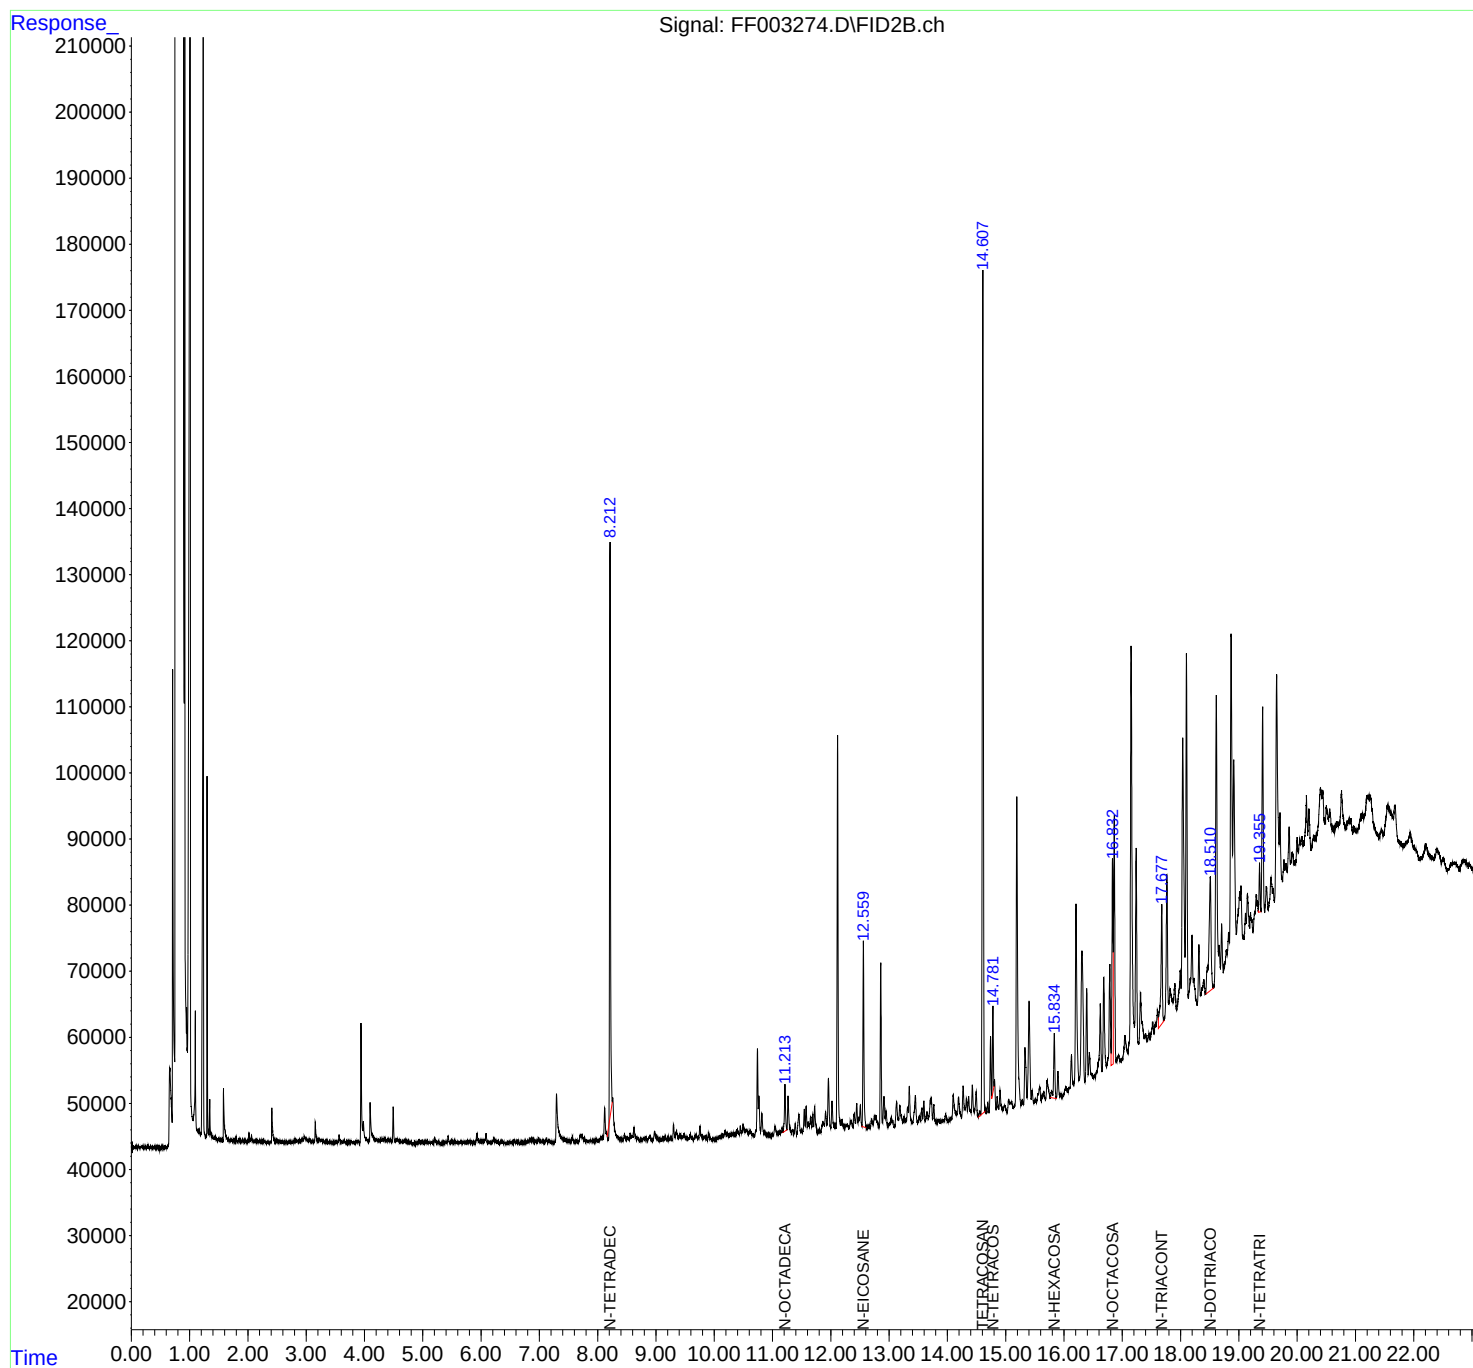


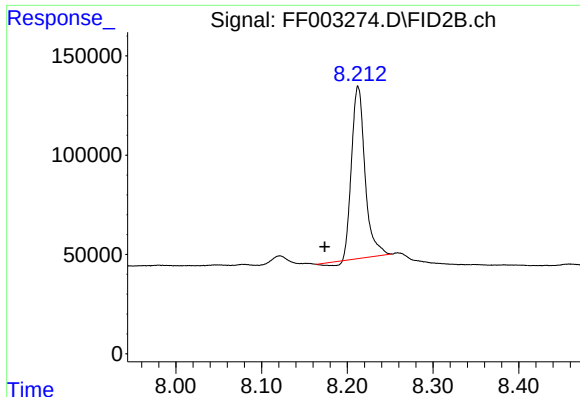

#4 N-TETRADECANE


R.T.: 8.213 min
Delta R.T.: 0.039 min
Response: 933798
Conc: 5.72 ug/ml

Instrument :
FID_F
ClientSampleId :

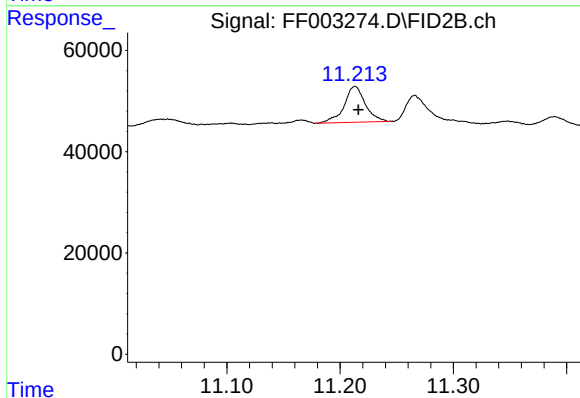


#6 N-OCTADECANE

R.T.: 11.213 min
Delta R.T.: -0.003 min
Response: 92165
Conc: 0.56 ug/ml

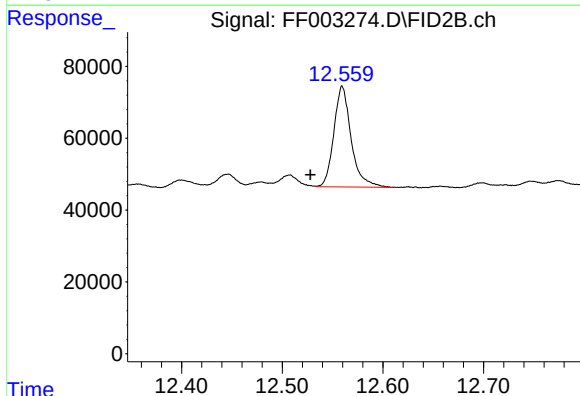


#7 N-EICOSANE

R.T.: 12.560 min
Delta R.T.: 0.032 min
Response: 335519
Conc: 2.04 ug/ml

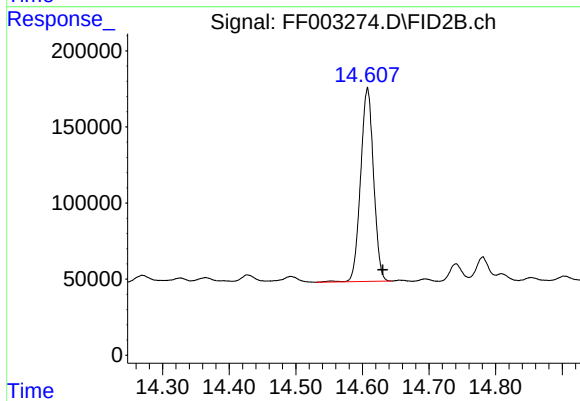

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.608 min
Delta R.T.: -0.023 min
Response: 1717795
Conc: 12.01 ug/ml

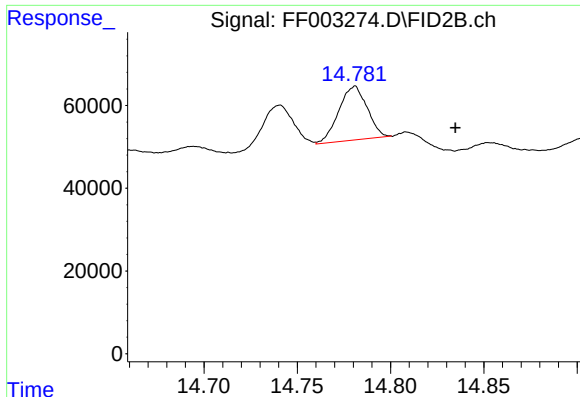

#10 N-TETRACOSANE


R.T.: 14.781 min
Delta R.T.: -0.054 min
Response: 136992
Conc: 0.85 ug/ml

Instrument :
FID_F
ClientSampleId :

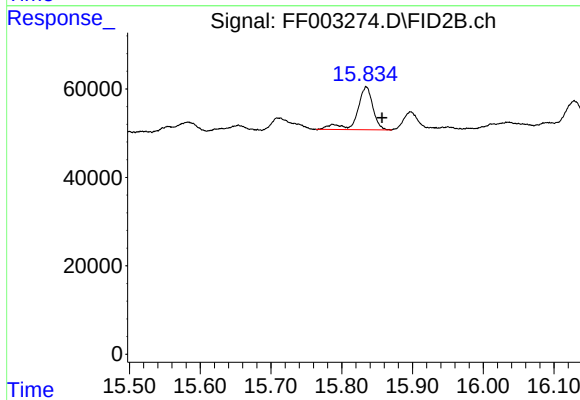


#11 N-HEXACOSANE

R.T.: 15.835 min
Delta R.T.: -0.023 min
Response: 149718
Conc: 0.95 ug/ml

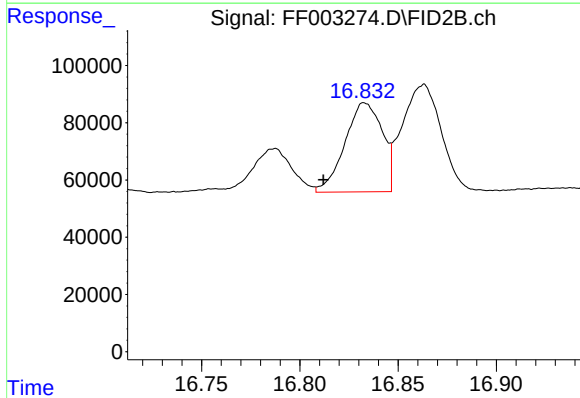


#12 N-OCTACOSANE

R.T.: 16.833 min
Delta R.T.: 0.021 min
Response: 410651
Conc: 2.61 ug/ml

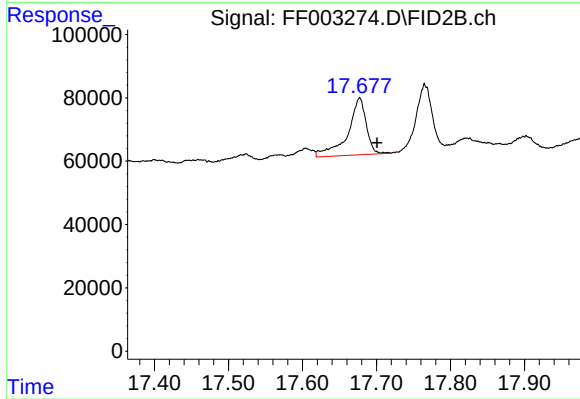

#13 N-TRIACONTANE


R.T.: 17.677 min
Delta R.T.: -0.023 min
Response: 312106
Conc: 1.99 ug/ml

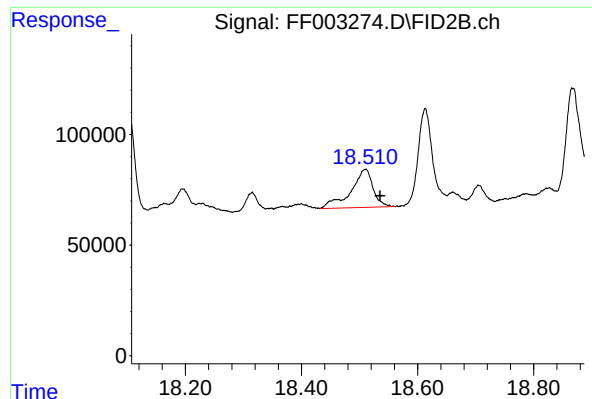

#14 N-DOTRIACONTANE

R.T.: 18.510 min
Delta R.T.: -0.025 min
Response: 457488
Conc: 3.15 ug/ml

Instrument :
FID_F
ClientSampleId :

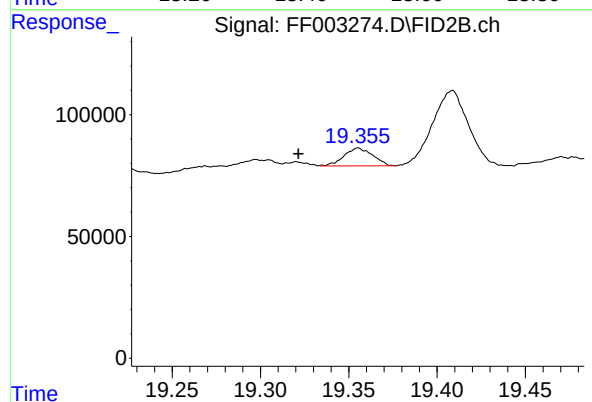

#15 N-TETRATRIACONTANE

R.T.: 19.355 min
Delta R.T.: 0.034 min
Response: 83729
Conc: 0.63 ug/ml