

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
 Data File : FF003276.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jan 2019 15:41
 Operator : AJ\SJ
 Sample : K1157-09
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 17 23:42:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.610	1710265	11.953 ug/ml
Target Compounds			
4) N-TETRADECANE	8.213	1127747	6.907 ug/ml
7) N-EICOSANE	12.508	123620	0.753 ug/ml
8) N-DOCOSANE	13.727	360008	2.216 ug/ml
10) N-TETRACOSANE	14.784f	1507740	9.401 ug/ml
11) N-HEXACOSANE	15.836	230120	1.455 ug/ml
12) N-OCTACOSANE	16.836	330396	2.098 ug/ml
13) N-TRIACONTANE	17.678	461836	2.942 ug/ml
14) N-DOTRIACONTANE	18.510	529303	3.640 ug/ml
15) N-TETRATRIACONTANE	19.361	125794	0.951 ug/ml
16) N-HEXATRIACONTANE	20.009f	44602	0.378 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
Data File : FF003276.D
Signal(s) : FID2B.ch
Acq On : 17 Jan 2019 15:41
Operator : AJ\SJ
Sample : K1157-09
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 17 23:42:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

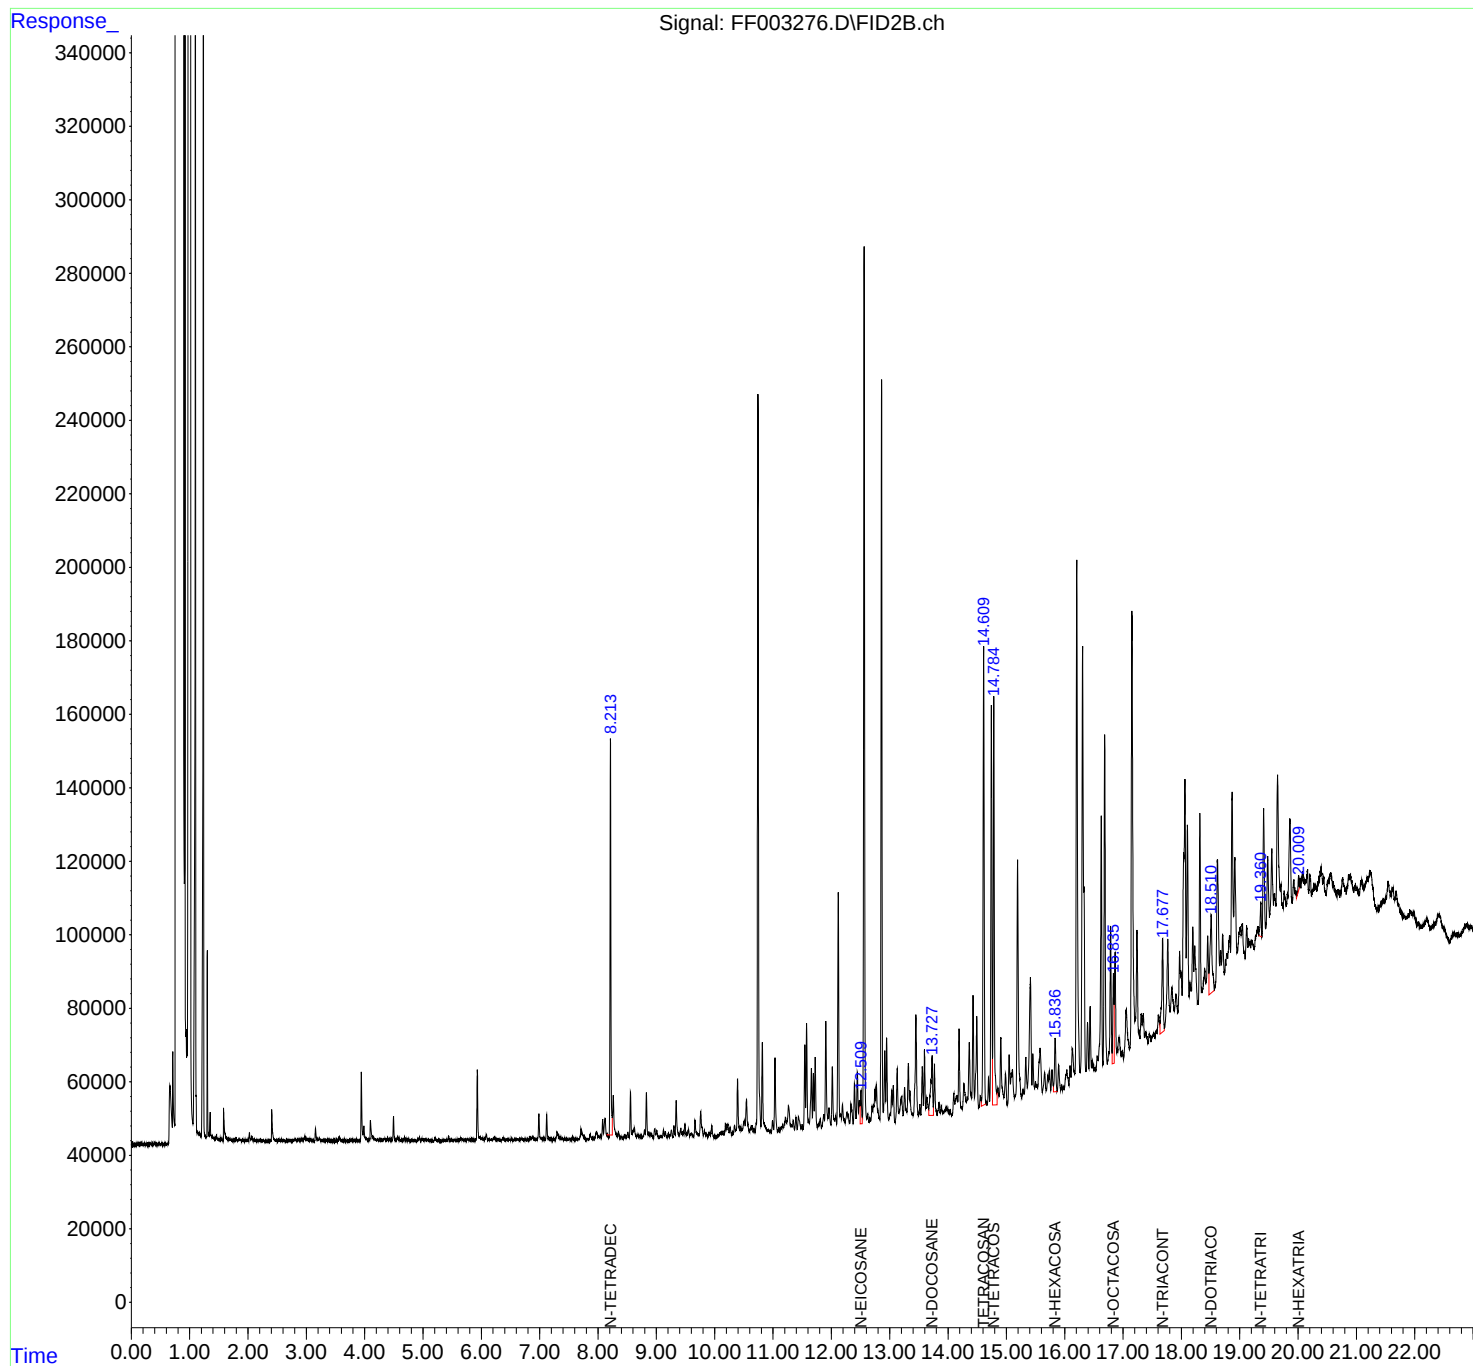


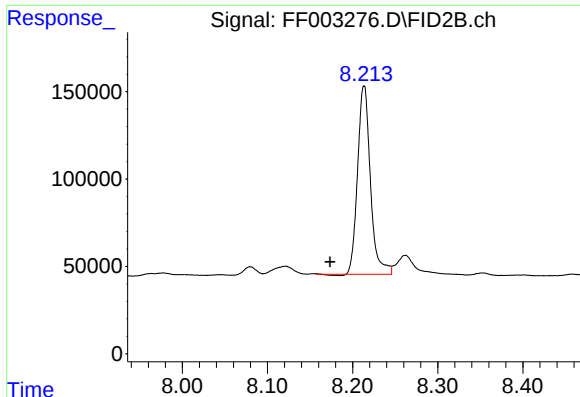

#4 N-TETRADECANE


R.T.: 8.213 min
Delta R.T.: 0.040 min
Response: 1127747
Conc: 6.91 ug/ml

Instrument :
FID_F
ClientSampleId :

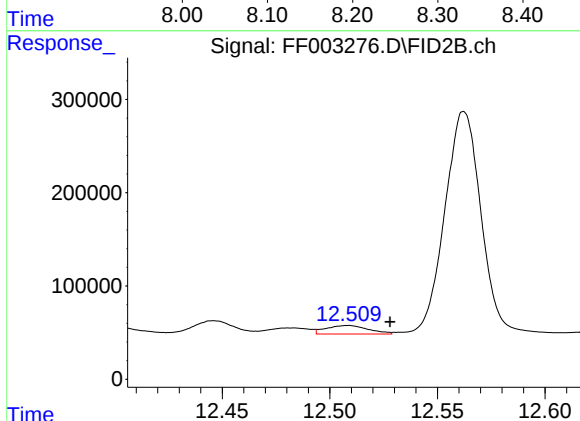


#7 N-EICOSANE

R.T.: 12.508 min
Delta R.T.: -0.020 min
Response: 123620
Conc: 0.75 ug/ml

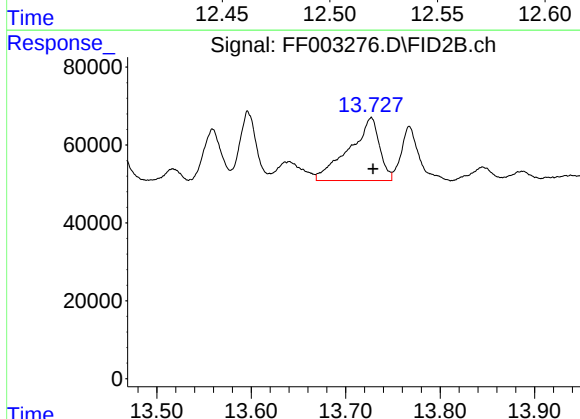


#8 N-DOCOSANE

R.T.: 13.727 min
Delta R.T.: -0.002 min
Response: 360008
Conc: 2.22 ug/ml

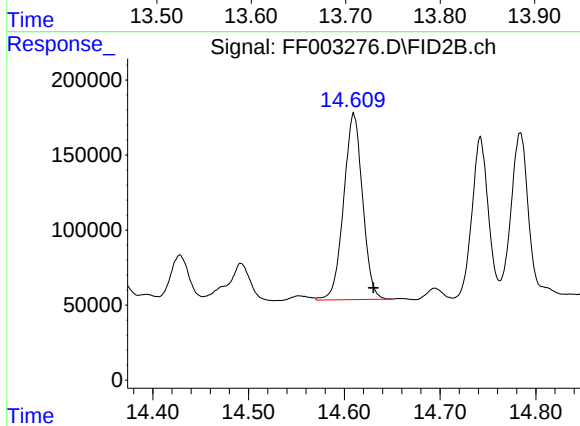

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.610 min
Delta R.T.: -0.021 min
Response: 1710265
Conc: 11.95 ug/ml

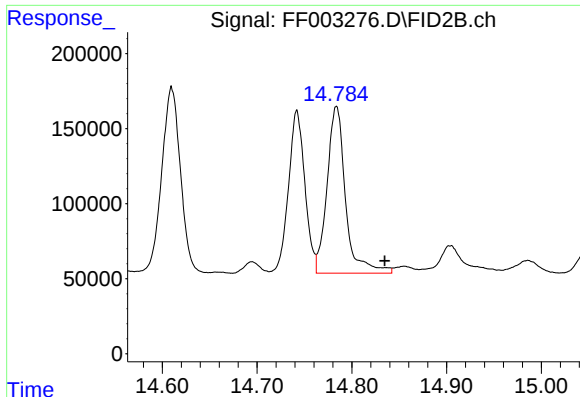

#10 N-TETRACOSANE


R.T.: 14.784 min
Delta R.T.: -0.051 min
Response: 1507740
Conc: 9.40 ug/ml

Instrument :
FID_F
ClientSampleId :

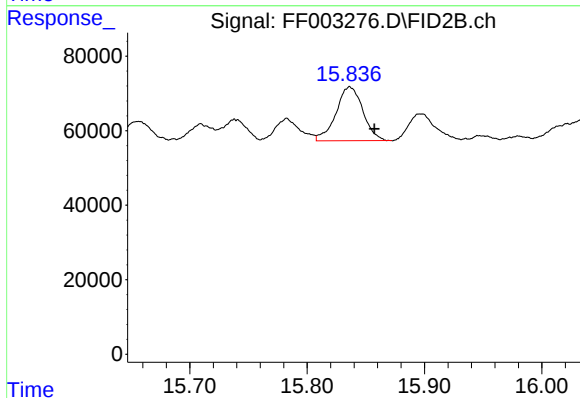


#11 N-HEXACOSANE

R.T.: 15.836 min
Delta R.T.: -0.021 min
Response: 230120
Conc: 1.45 ug/ml

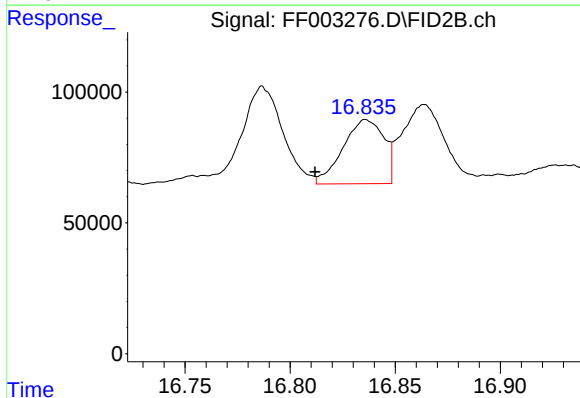


#12 N-OCTACOSANE

R.T.: 16.836 min
Delta R.T.: 0.024 min
Response: 330396
Conc: 2.10 ug/ml

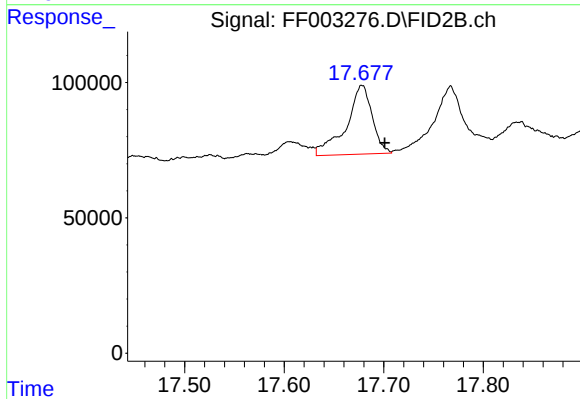

#13 N-TRIACONTANE


R.T.: 17.678 min
Delta R.T.: -0.023 min
Response: 461836
Conc: 2.94 ug/ml

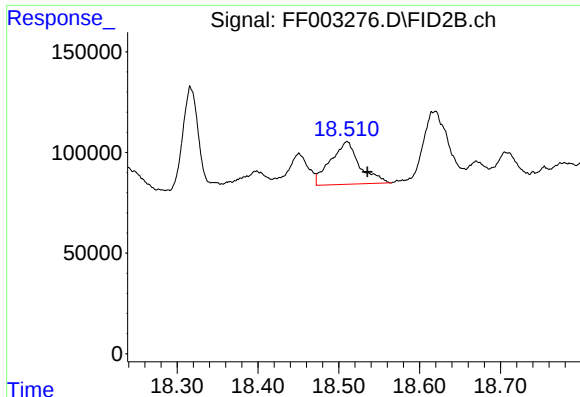

#14 N-DOTRIACONTANE


R.T.: 18.510 min
Delta R.T.: -0.025 min
Response: 529303
Conc: 3.64 ug/ml

Instrument :
FID_F
ClientSampleId :

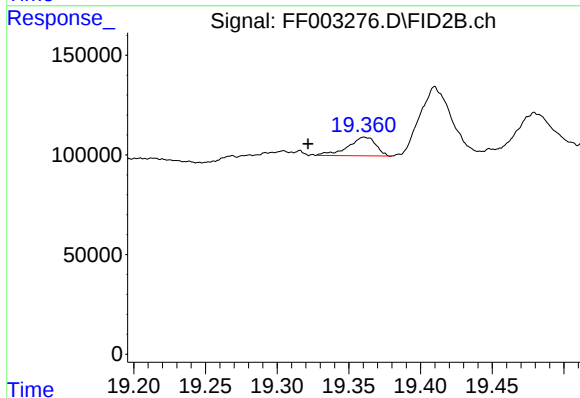

#15 N-TETRATRIACONTANE

R.T.: 19.361 min
Delta R.T.: 0.039 min
Response: 125794
Conc: 0.95 ug/ml

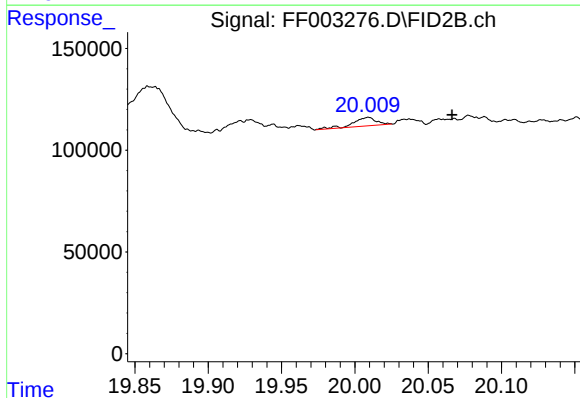

#16 N-HEXATRIACONTANE

R.T.: 20.009 min
Delta R.T.: -0.057 min
Response: 44602
Conc: 0.38 ug/ml