

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
 Data File : FF003277.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jan 2019 16:11
 Operator : AJ\SJ
 Sample : K1157-11
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 17 23:42:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.609	2265096	15.830 ug/ml
Target Compounds			
4) N-TETRADECANE	8.213	381538	2.337 ug/ml
7) N-EICOSANE	12.561	930128	5.665 ug/ml
8) N-DOCOSANE	13.727	172659	1.063 ug/ml
10) N-TETRACOSANE	14.783f	488867	3.048 ug/ml
11) N-HEXACOSANE	15.835	222529	1.407 ug/ml
12) N-OCTACOSANE	16.835	287955	1.828 ug/ml
13) N-TRIACONTANE	17.678	555550	3.539 ug/ml
14) N-DOTRIACONTANE	18.513	593664	4.082 ug/ml
15) N-TETRATRIACONTANE	19.360	139589	1.056 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
Data File : FF003277.D
Signal(s) : FID2B.ch
Acq On : 17 Jan 2019 16:11
Operator : AJ\SJ
Sample : K1157-11
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 17 23:42:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

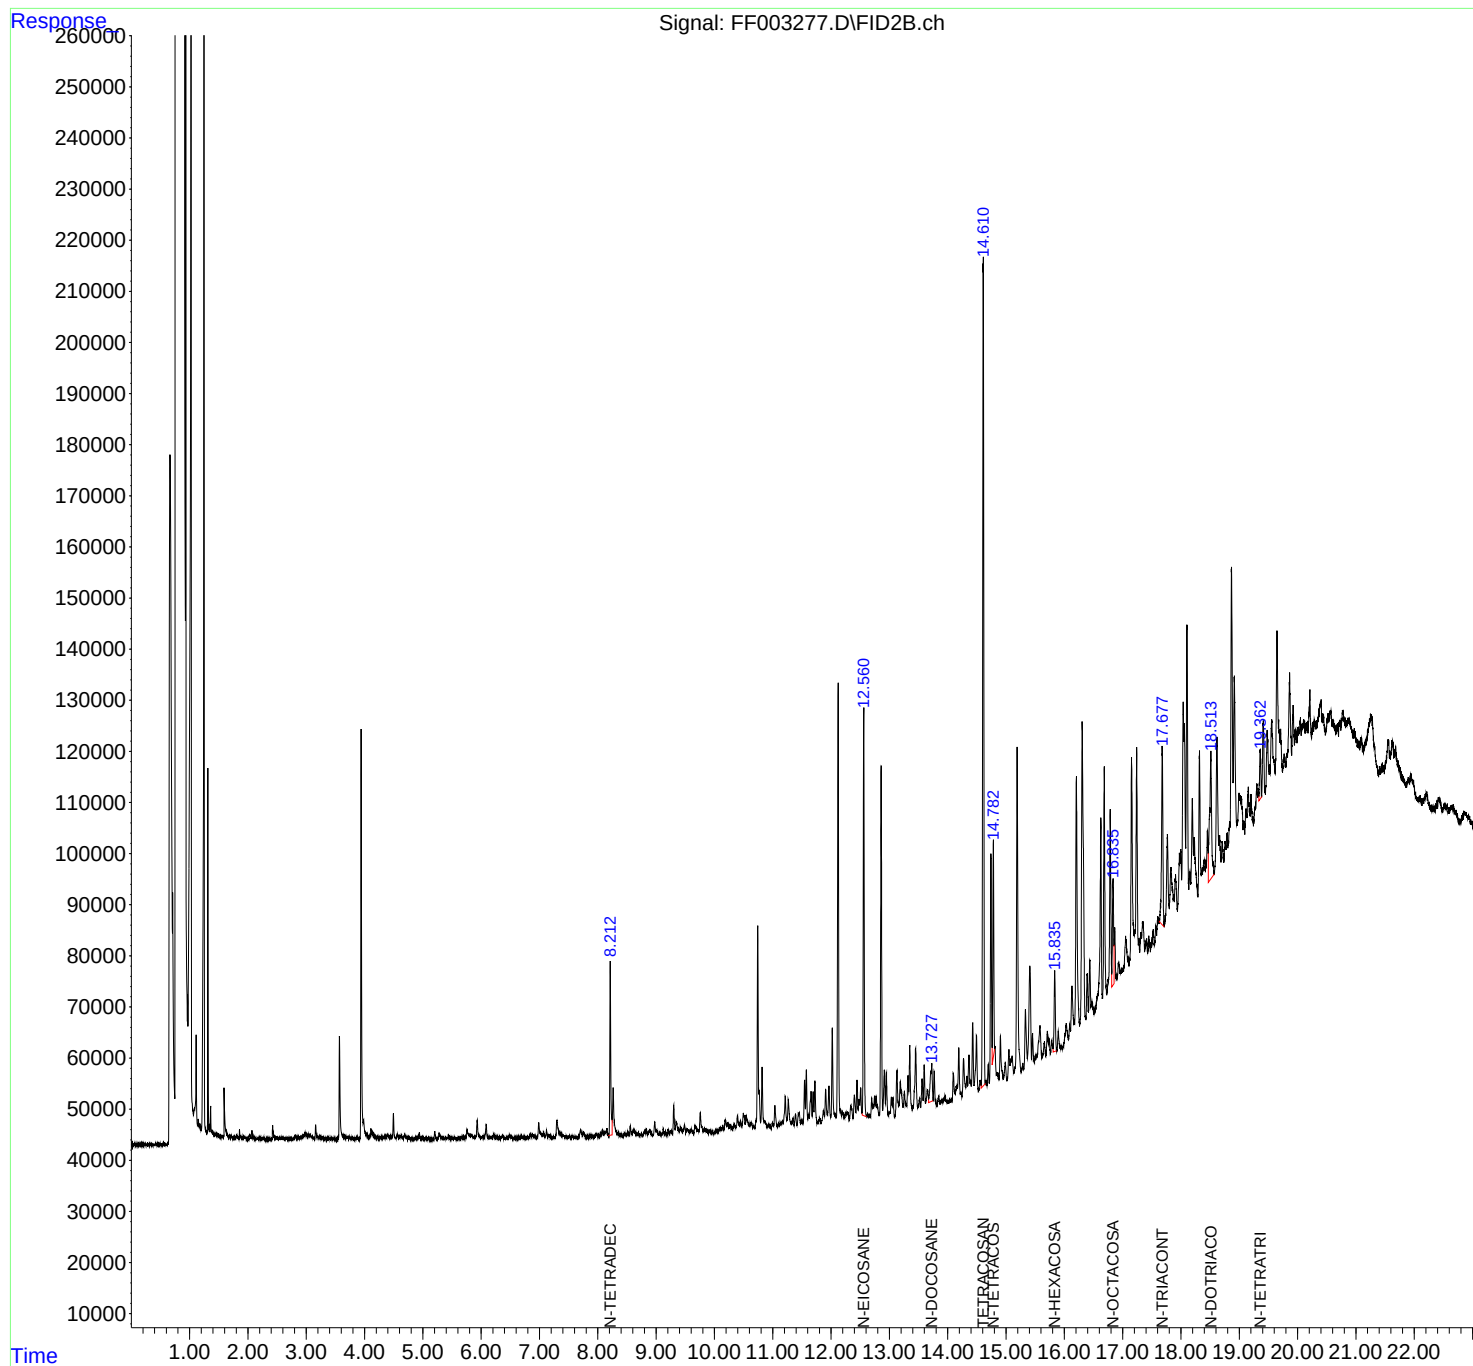


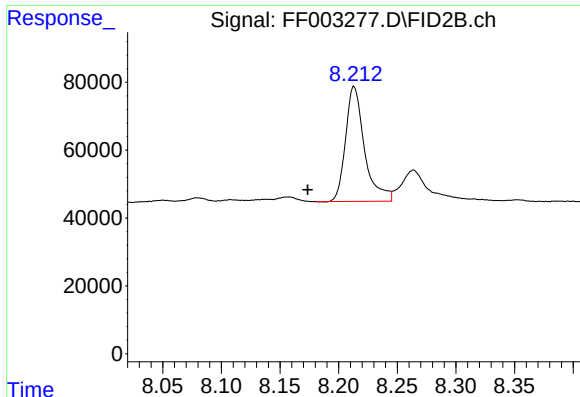

#4 N-TETRADECANE


R.T.: 8.213 min
Delta R.T.: 0.040 min
Response: 381538
Conc: 2.34 ug/ml

Instrument :
FID_F
ClientSampleId :

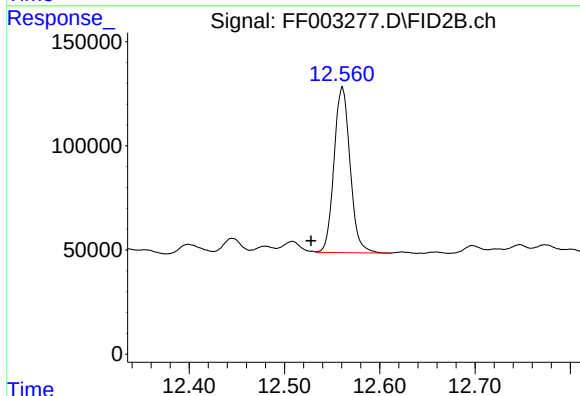


#7 N-EICOSANE

R.T.: 12.561 min
Delta R.T.: 0.033 min
Response: 930128
Conc: 5.66 ug/ml

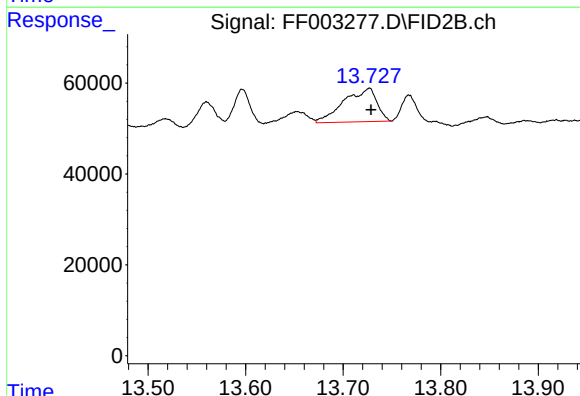


#8 N-DOCOSANE

R.T.: 13.727 min
Delta R.T.: -0.002 min
Response: 172659
Conc: 1.06 ug/ml

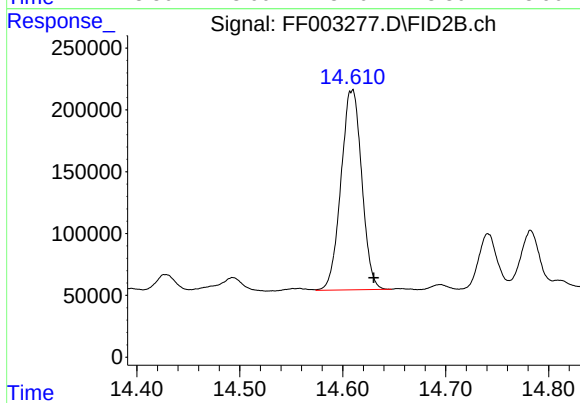

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.609 min
Delta R.T.: -0.021 min
Response: 2265096
Conc: 15.83 ug/ml

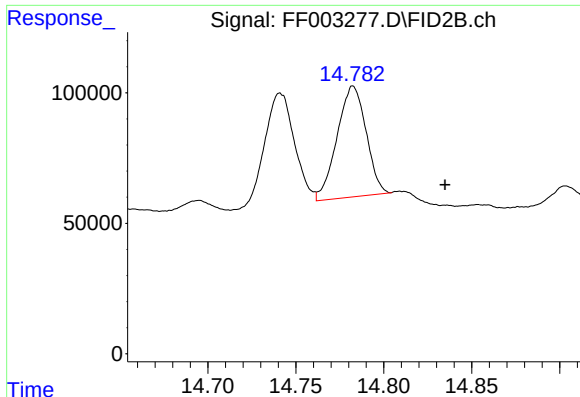

#10 N-TETRACOSANE


R.T.: 14.783 min
Delta R.T.: -0.052 min
Response: 488867
Conc: 3.05 ug/ml

Instrument :
FID_F
ClientSampleId :

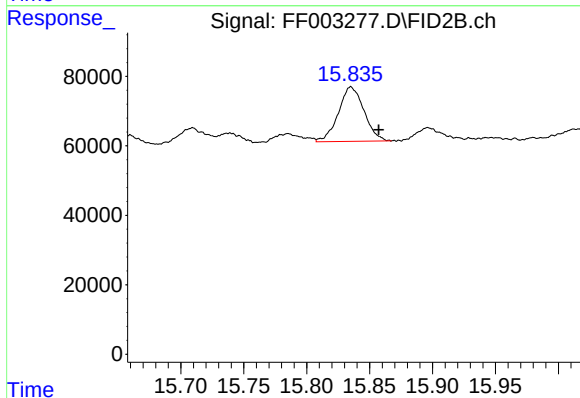


#11 N-HEXACOSANE

R.T.: 15.835 min
Delta R.T.: -0.022 min
Response: 222529
Conc: 1.41 ug/ml

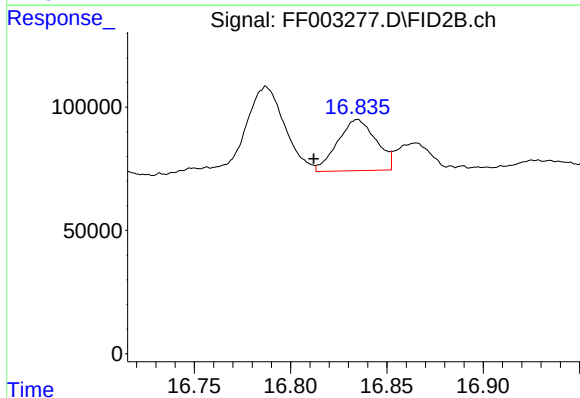


#12 N-OCTACOSANE

R.T.: 16.835 min
Delta R.T.: 0.023 min
Response: 287955
Conc: 1.83 ug/ml

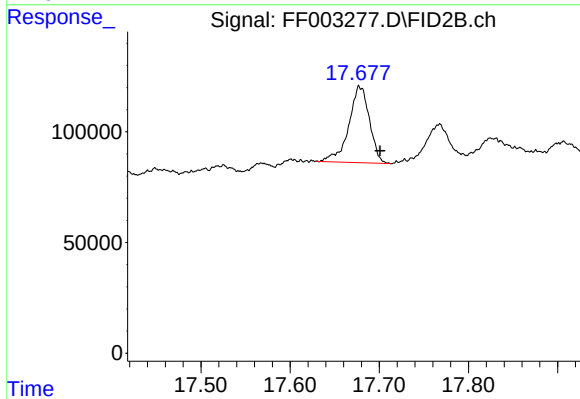

#13 N-TRIACONTANE


R.T.: 17.678 min
Delta R.T.: -0.023 min
Response: 555550
Conc: 3.54 ug/ml

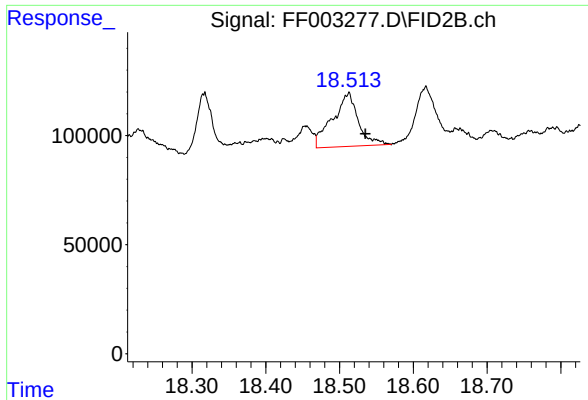

#14 N-DOTRIACONTANE

R.T.: 18.513 min
Delta R.T.: -0.023 min
Response: 593664
Conc: 4.08 ug/ml

Instrument :
FID_F
ClientSampleId :

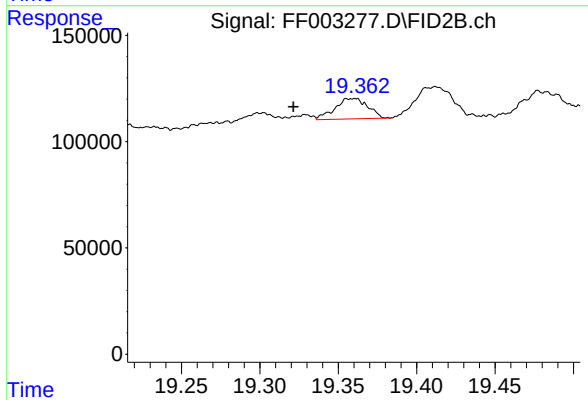

#15 N-TETRATRIACONTANE

R.T.: 19.360 min
Delta R.T.: 0.039 min
Response: 139589
Conc: 1.06 ug/ml