

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
 Data File : FF003281.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jan 2019 18:11
 Operator : AJ\SJ
 Sample : K1157-01
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 17 23:43:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.608	1612128	11.267 ug/ml
Target Compounds			
4) N-TETRADECANE	8.213	979535	5.999 ug/ml
7) N-EICOSANE	12.560	747932	4.555 ug/ml
10) N-TETRACOSANE	14.781f	413846	2.580 ug/ml
11) N-HEXACOSANE	15.834	171775	1.086 ug/ml
12) N-OCTACOSANE	16.833	306137	1.944 ug/ml
13) N-TRIACONTANE	17.676	387700	2.469 ug/ml
14) N-DOTRIACONTANE	18.505	537531	3.696 ug/ml
15) N-TETRATRIACONTANE	19.355	140156	1.060 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
Data File : FF003281.D
Signal(s) : FID2B.ch
Acq On : 17 Jan 2019 18:11
Operator : AJ\SJ
Sample : K1157-01
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 17 23:43:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

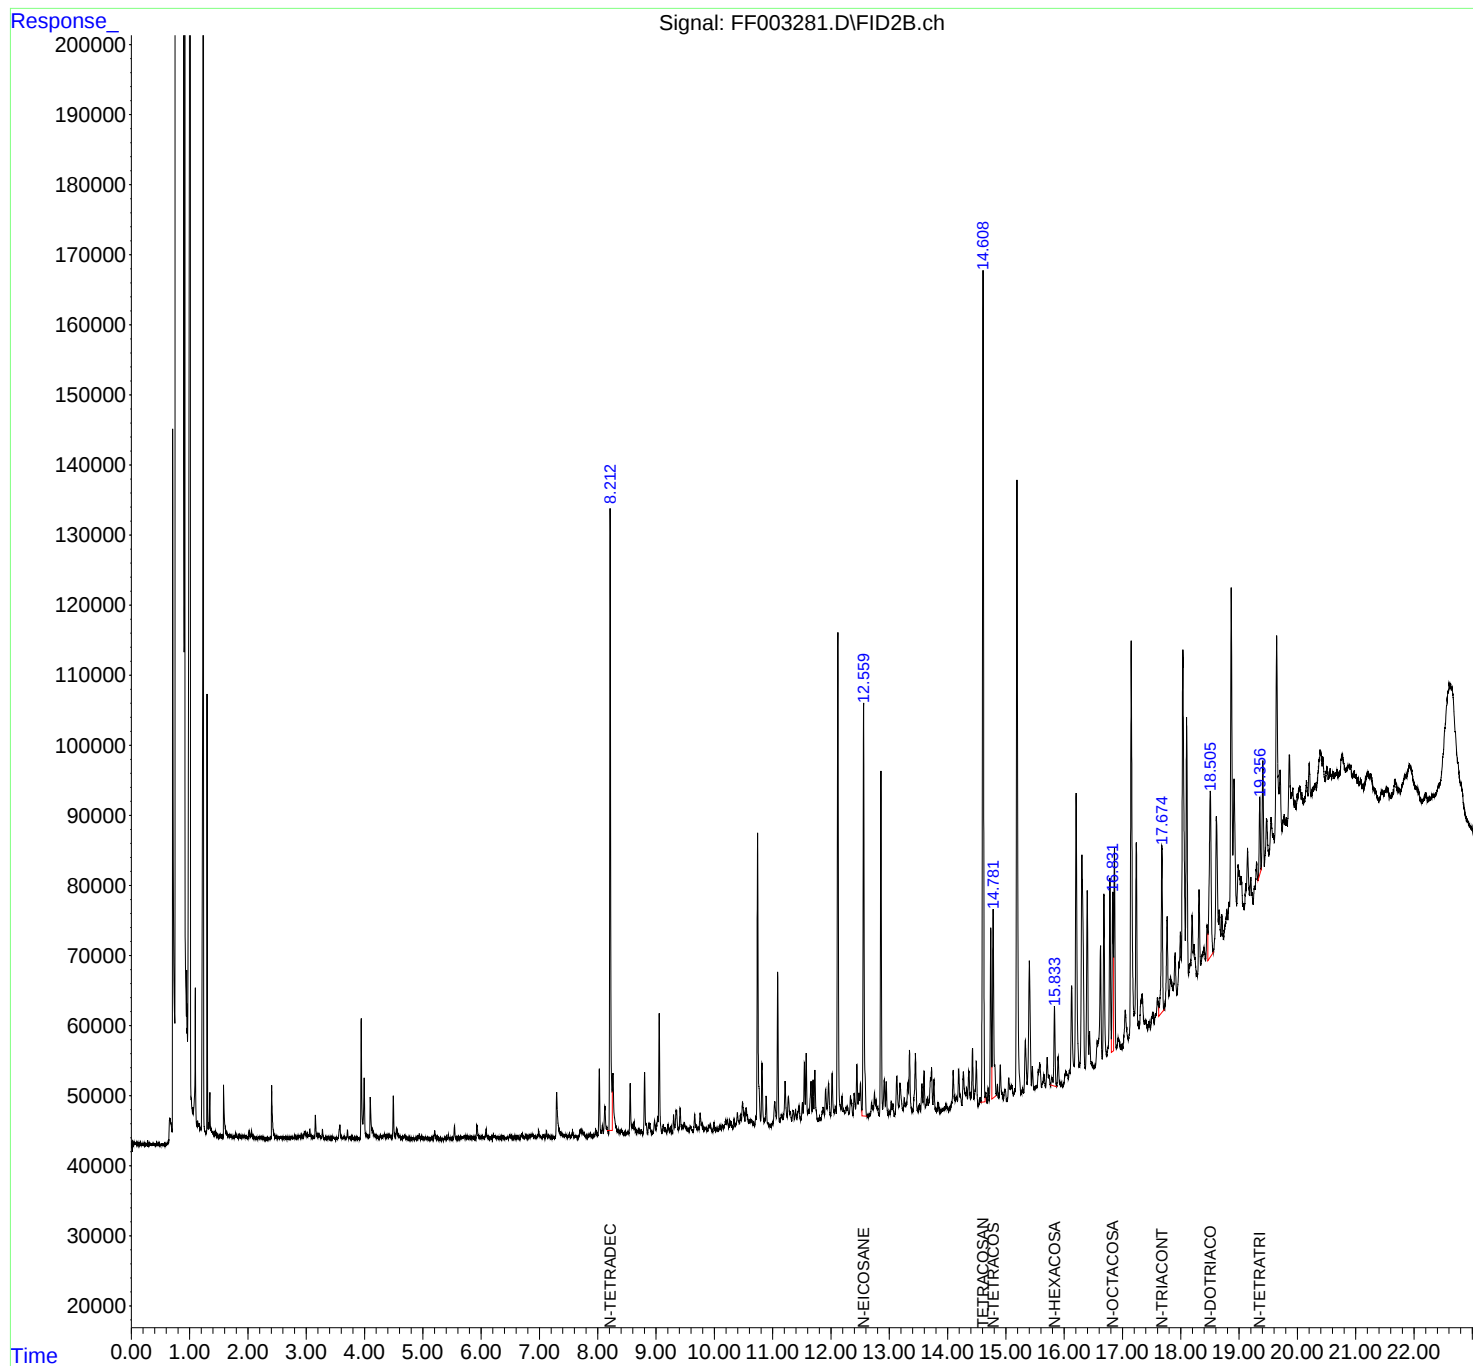


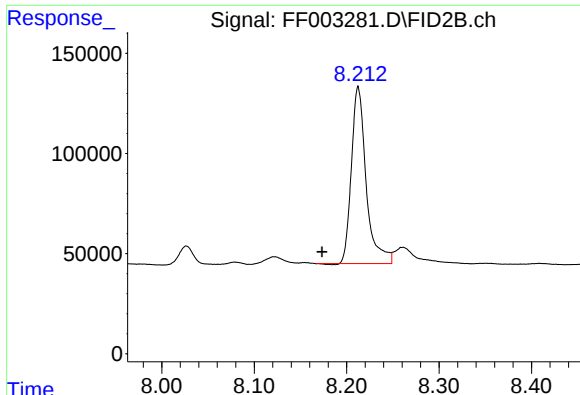

#4 N-TETRADECANE


R.T.: 8.213 min
Delta R.T.: 0.039 min
Response: 979535
Conc: 6.00 ug/ml

Instrument :
FID_F
ClientSampleId :

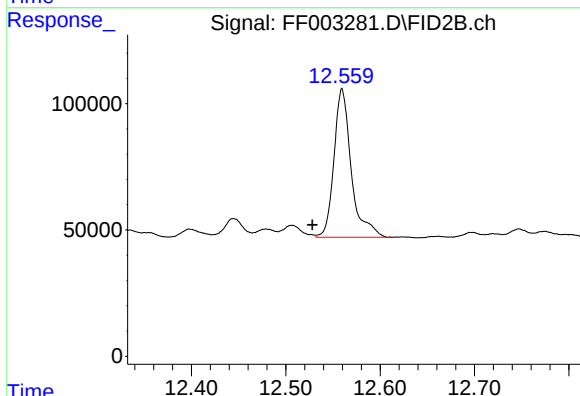


#7 N-EICOSANE

R.T.: 12.560 min
Delta R.T.: 0.032 min
Response: 747932
Conc: 4.56 ug/ml

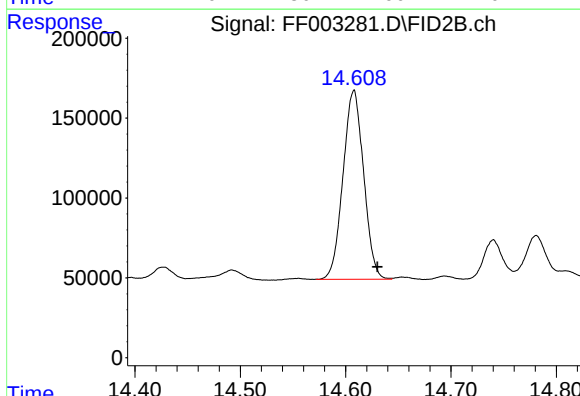


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.608 min
Delta R.T.: -0.022 min
Response: 1612128
Conc: 11.27 ug/ml

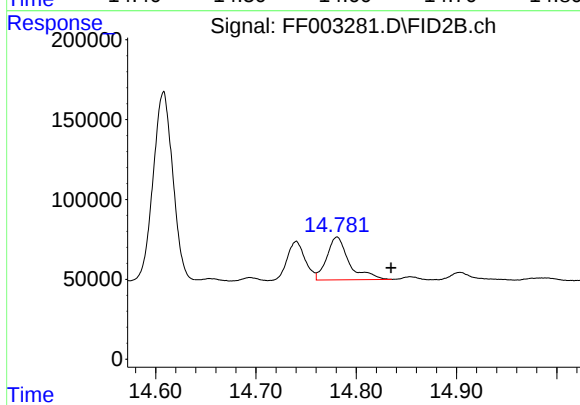

#10 N-TETRACOSANE


R.T.: 14.781 min
Delta R.T.: -0.054 min
Response: 413846
Conc: 2.58 ug/ml

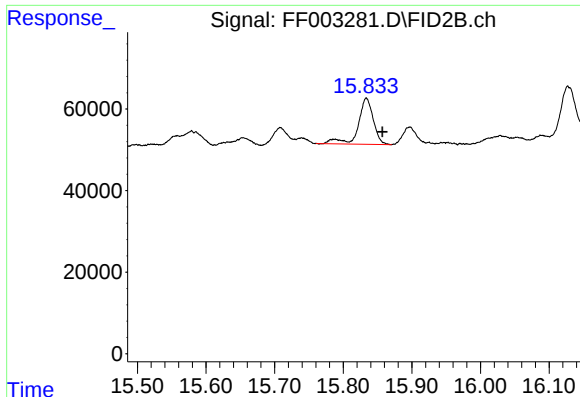

#11 N-HEXACOSANE


R.T.: 15.834 min
Delta R.T.: -0.024 min
Response: 171775
Conc: 1.09 ug/ml

Instrument :
FID_F
ClientSampleId :

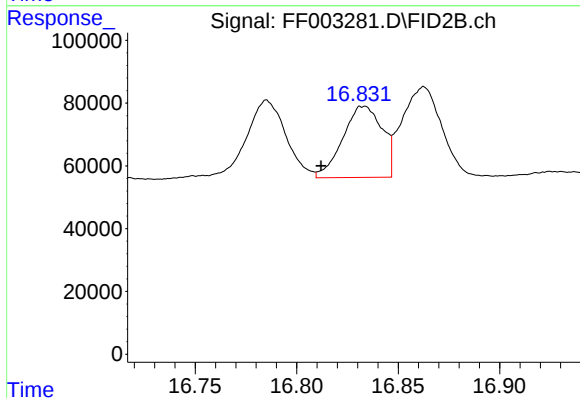


#12 N-OCTACOSANE

R.T.: 16.833 min
Delta R.T.: 0.021 min
Response: 306137
Conc: 1.94 ug/ml

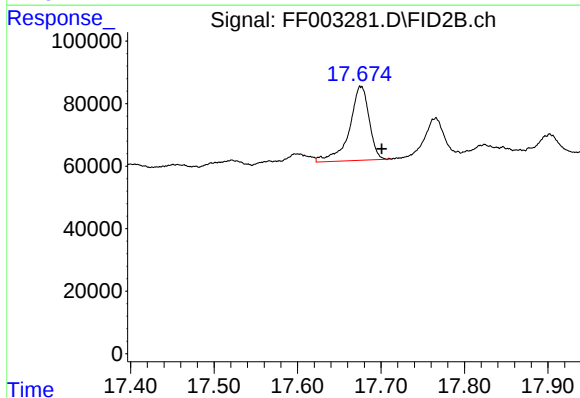


#13 N-TRIACONTANE

R.T.: 17.676 min
Delta R.T.: -0.025 min
Response: 387700
Conc: 2.47 ug/ml

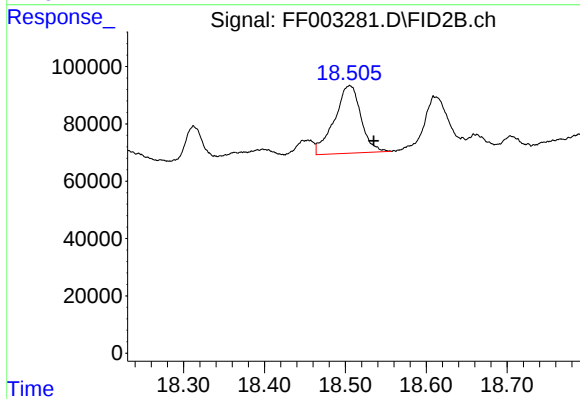

#14 N-DOTRIACONTANE

R.T.: 18.505 min
Delta R.T.: -0.030 min
Response: 537531
Conc: 3.70 ug/ml

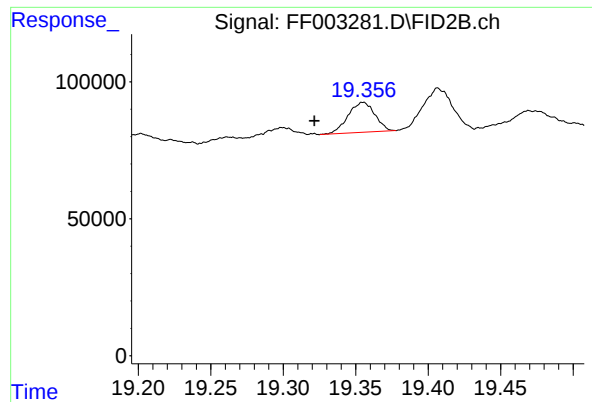

#15 N-TETRATRIACONTANE

R.T.: 19.355 min
Delta R.T.: 0.034 min
Response: 140156
Conc: 1.06 ug/ml

Instrument :
FID_F
ClientSampleId :