

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
 Data File : FF003285.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jan 2019 20:10
 Operator : AJ\SJ
 Sample : K1157-07 5X
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 17 23:43:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.606	320514	2.240 ug/ml
Target Compounds			
7) N-EICOSANE	12.559	176546	1.075 ug/ml
10) N-TETRACOSANE	14.783f	124404	0.776 ug/ml
12) N-OCTACOSANE	16.786	86273	0.548 ug/ml
13) N-TRIACONTANE	17.675	160216	1.020 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
Data File : FF003285.D
Signal(s) : FID2B.ch
Acq On : 17 Jan 2019 20:10
Operator : AJ\SJ
Sample : K1157-07 5X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 17 23:43:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

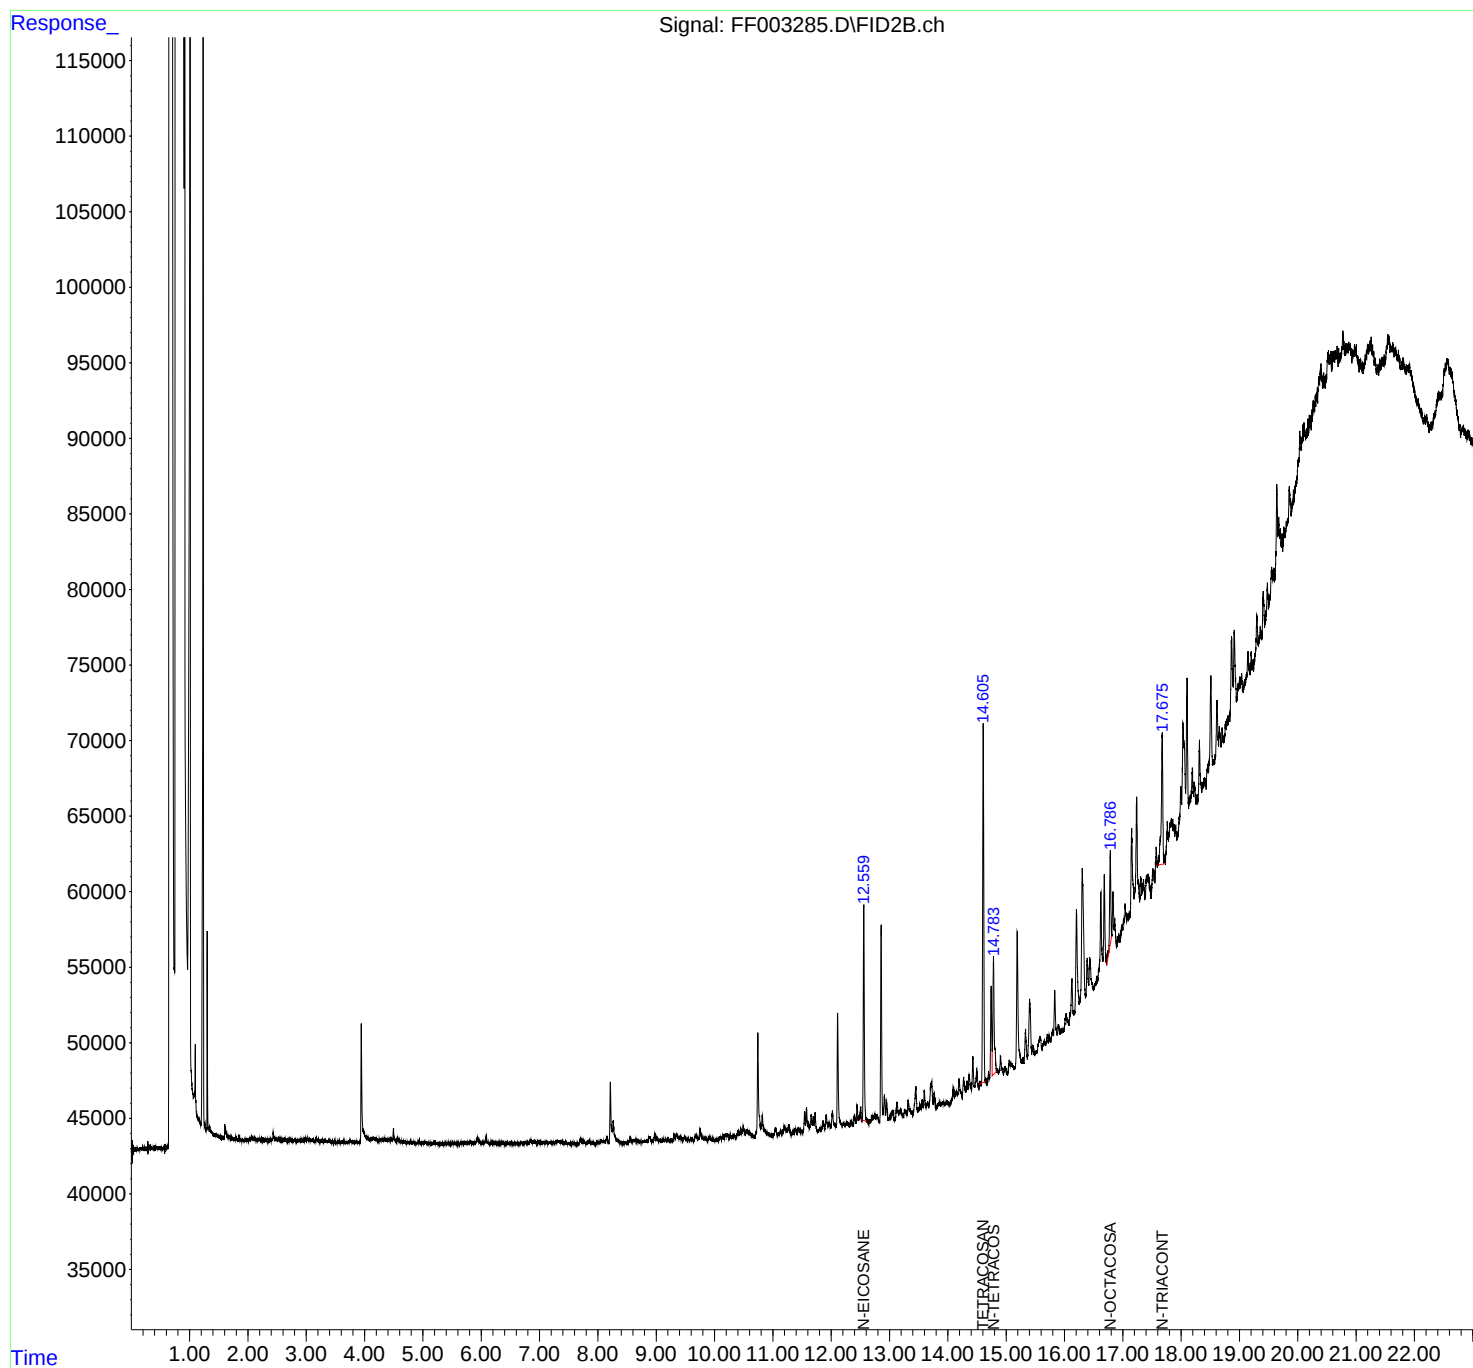


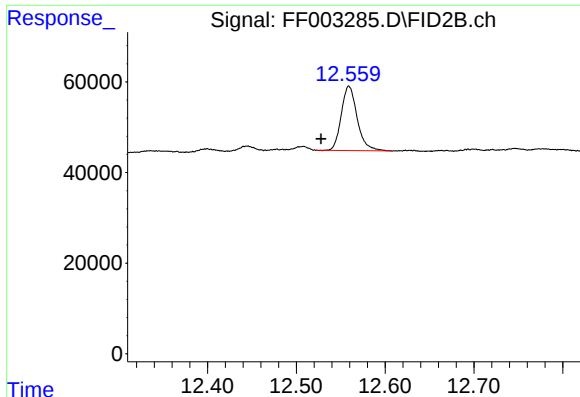

#7 N-EICOSANE


R.T.: 12.559 min
Delta R.T.: 0.031 min
Response: 176546
Conc: 1.08 ug/ml

Instrument :
FID_F
ClientSampleId :

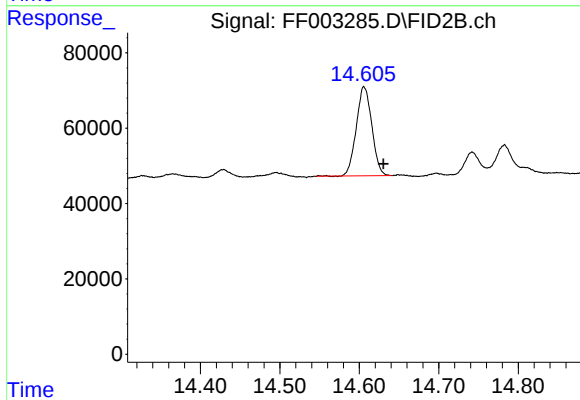


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.606 min
Delta R.T.: -0.024 min
Response: 320514
Conc: 2.24 ug/ml

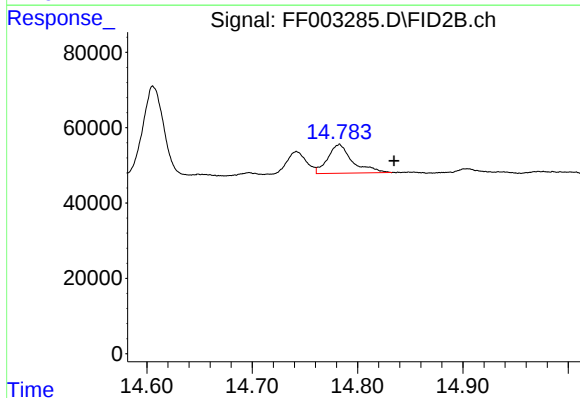


#10 N-TETRACOSANE

R.T.: 14.783 min
Delta R.T.: -0.052 min
Response: 124404
Conc: 0.78 ug/ml

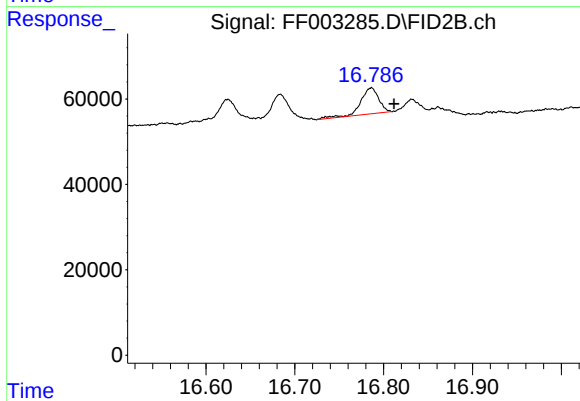

#12 N-OCTACOSANE

R.T.: 16.786 min
Delta R.T.: -0.026 min
Response: 86273
Conc: 0.55 ug/ml

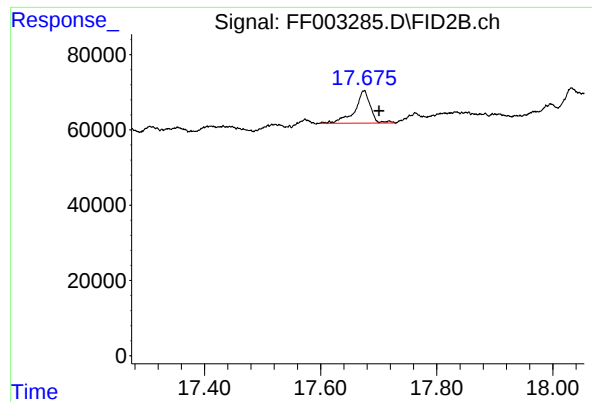

#13 N-TRIACONTANE

R.T.: 17.675 min
Delta R.T.: -0.026 min
Response: 160216
Conc: 1.02 ug/ml

Instrument :
FID_F
ClientSampleId :