

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
 Data File : FF003286.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jan 2019 20:40
 Operator : AJ\SJ
 Sample : K1157-09 2X
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 17 23:44:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.608	790541	5.525 ug/ml
Target Compounds			
4) N-TETRADECANE	8.213	398109	2.438 ug/ml
7) N-EICOSANE	12.560	1279805	7.795 ug/ml
8) N-DOCOSANE	13.725	134924	0.830 ug/ml
10) N-TETRACOSANE	14.782f	673840	4.201 ug/ml
11) N-HEXACOSANE	15.834	109304	0.691 ug/ml
12) N-OCTACOSANE	16.834	137017	0.870 ug/ml
13) N-TRIACONTANE	17.677	249472	1.589 ug/ml
14) N-DOTRIACONTANE	18.511	339792	2.337 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
Data File : FF003286.D
Signal(s) : FID2B.ch
Acq On : 17 Jan 2019 20:40
Operator : AJ\SJ
Sample : K1157-09 2X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 17 23:44:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

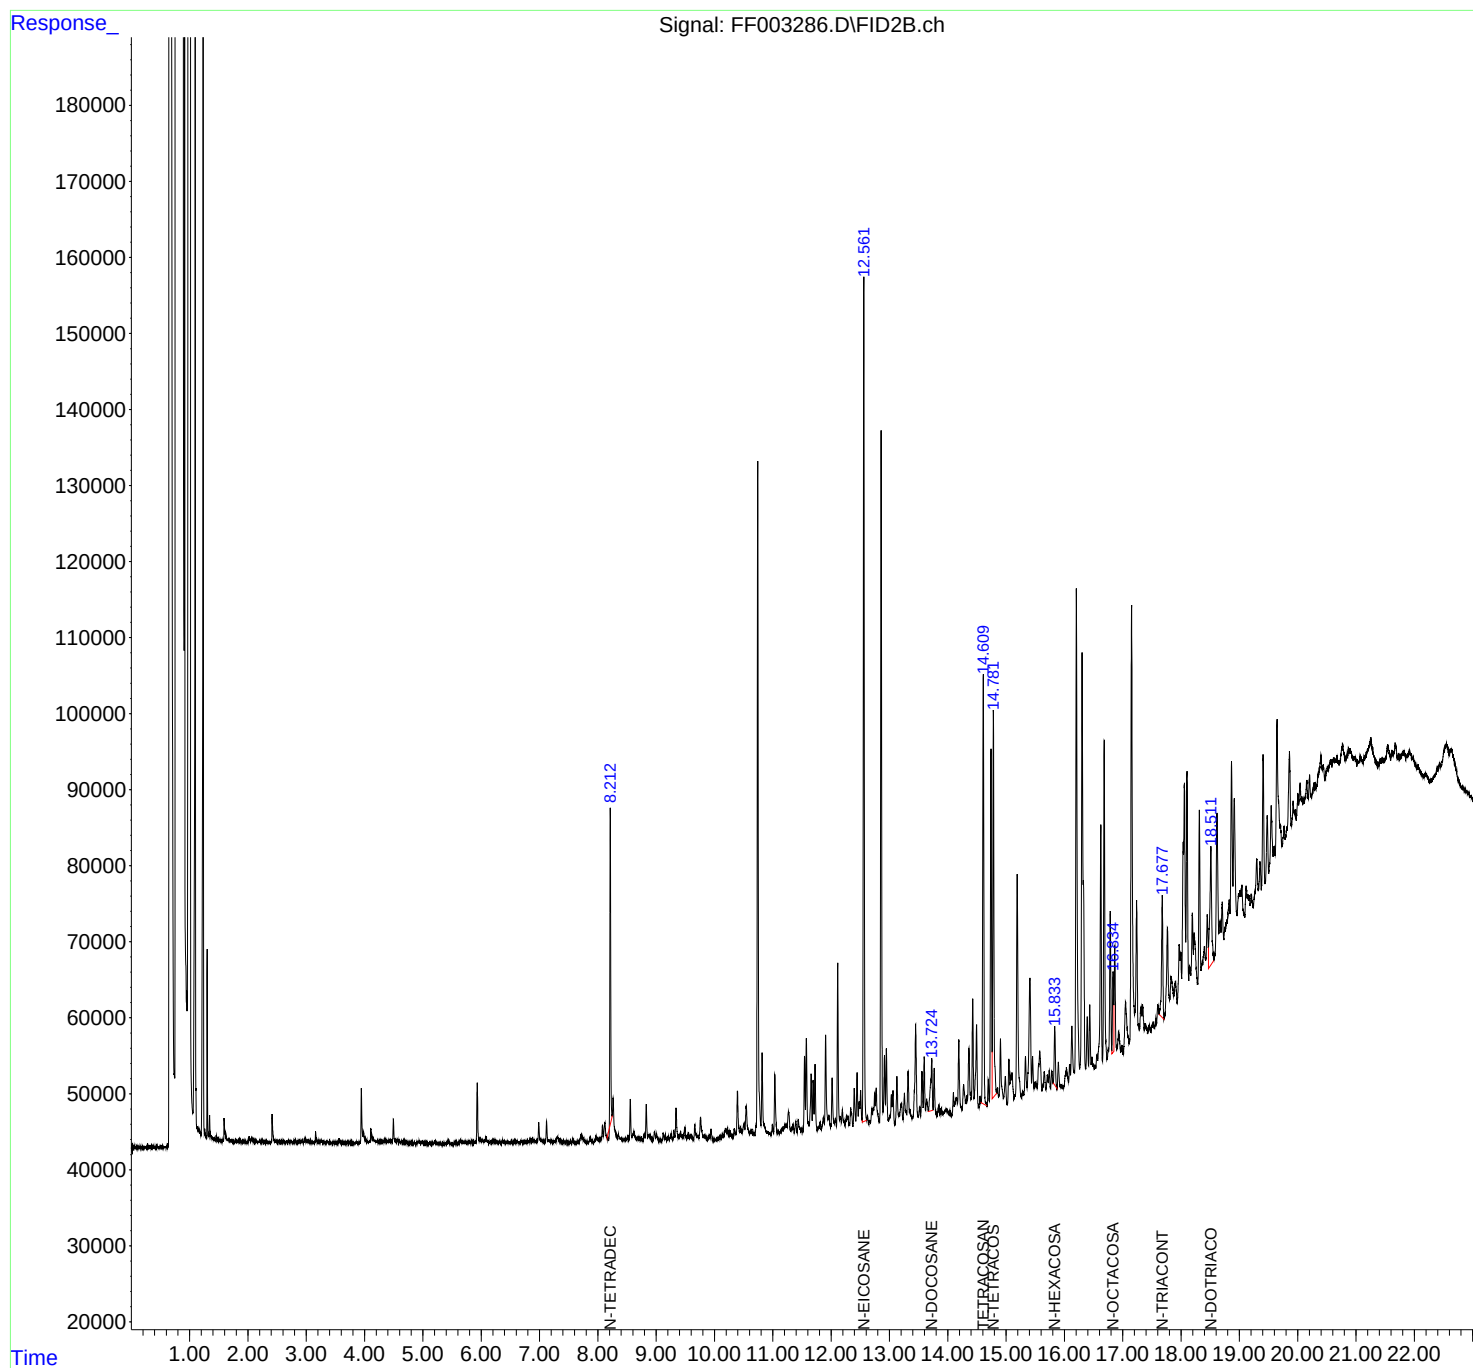


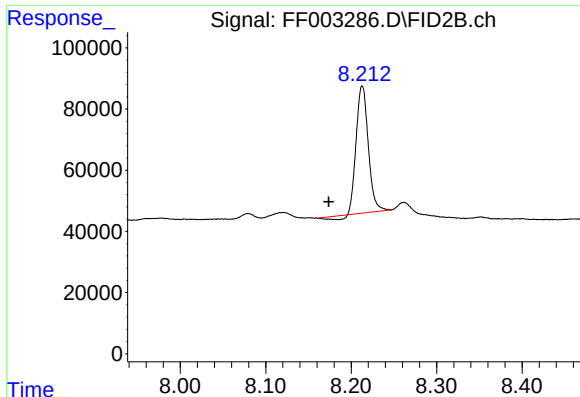

#4 N-TETRADECANE


R.T.: 8.213 min
Delta R.T.: 0.039 min
Response: 398109
Conc: 2.44 ug/ml

Instrument :
FID_F
ClientSampleId :

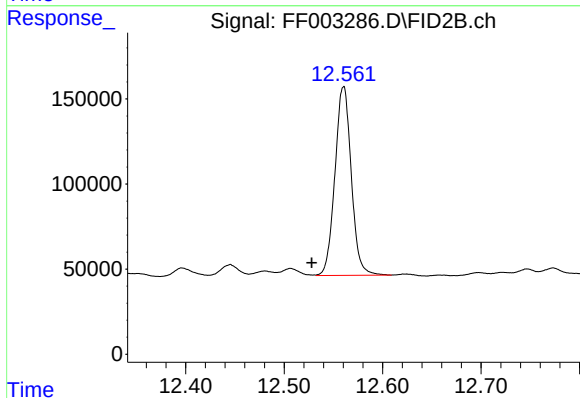


#7 N-EICOSANE

R.T.: 12.560 min
Delta R.T.: 0.032 min
Response: 1279805
Conc: 7.79 ug/ml

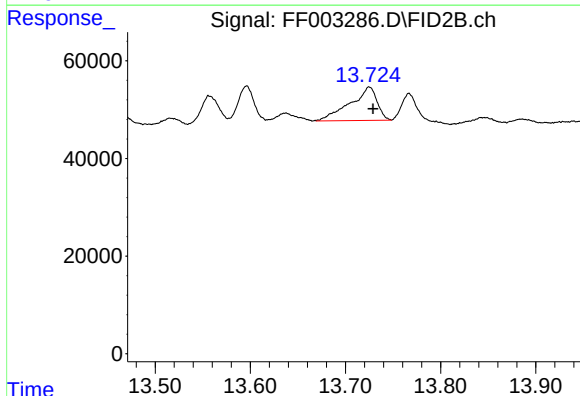


#8 N-DOCOSANE

R.T.: 13.725 min
Delta R.T.: -0.004 min
Response: 134924
Conc: 0.83 ug/ml

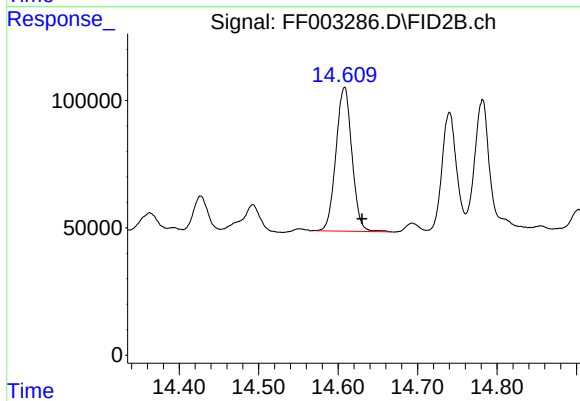

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.608 min
Delta R.T.: -0.022 min
Response: 790541
Conc: 5.52 ug/ml

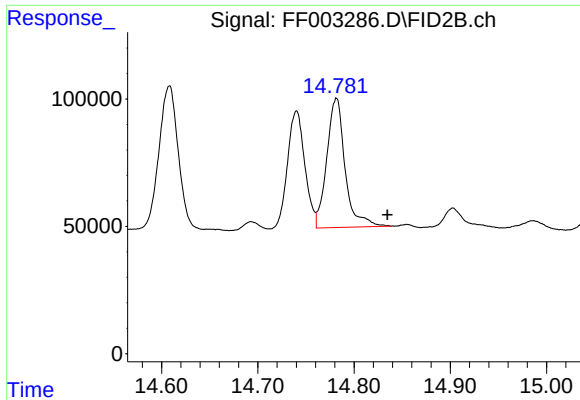

#10 N-TETRACOSANE


R.T.: 14.782 min
Delta R.T.: -0.053 min
Response: 673840
Conc: 4.20 ug/ml

Instrument :
FID_F
ClientSampleId :

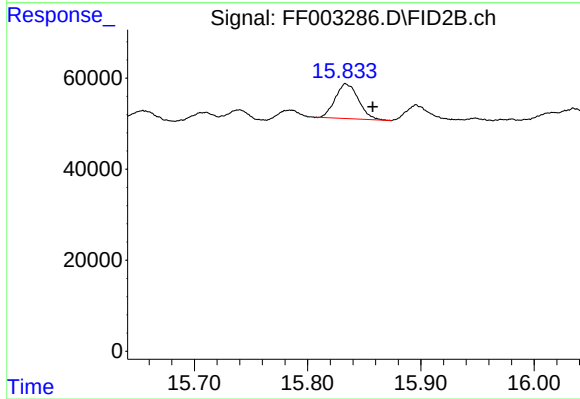


#11 N-HEXACOSANE

R.T.: 15.834 min
Delta R.T.: -0.024 min
Response: 109304
Conc: 0.69 ug/ml

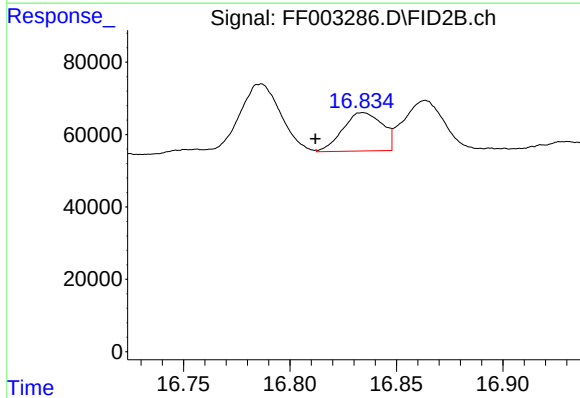


#12 N-OCTACOSANE

R.T.: 16.834 min
Delta R.T.: 0.022 min
Response: 137017
Conc: 0.87 ug/ml

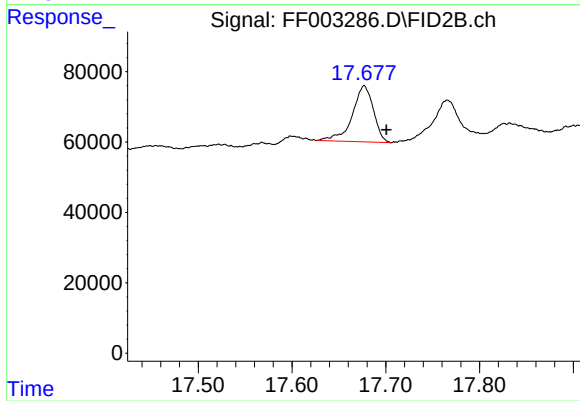

#13 N-TRIACONTANE

R.T.: 17.677 min
Delta R.T.: -0.024 min
Response: 249472
Conc: 1.59 ug/ml

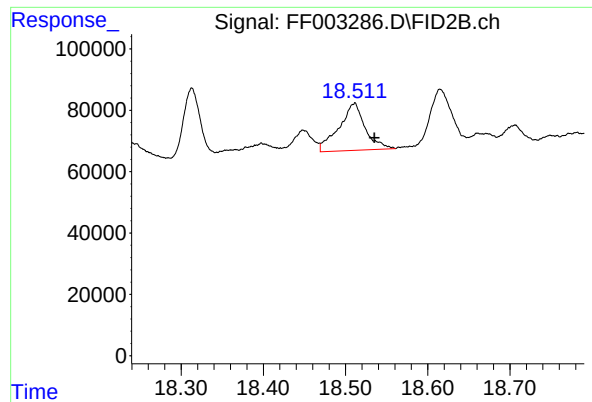

#14 N-DOTRIACONTANE

R.T.: 18.511 min
Delta R.T.: -0.024 min
Response: 339792
Conc: 2.34 ug/ml

Instrument :
FID_F
ClientSampleId :