

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
 Data File : FF003287.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jan 2019 21:10
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 17 23:44:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.608	2164096	15.124 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.675	174198	1.110 ug/ml
14) N-DOTRIACONTANE	18.511	228739	1.573 ug/ml
15) N-TETRATRIACONTANE	19.297	115358	0.873 ug/ml
17) N-OCTATRIACONTANE	20.775	173983	1.665 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011719\
Data File : FF003287.D
Signal(s) : FID2B.ch
Acq On : 17 Jan 2019 21:10
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 17 23:44:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

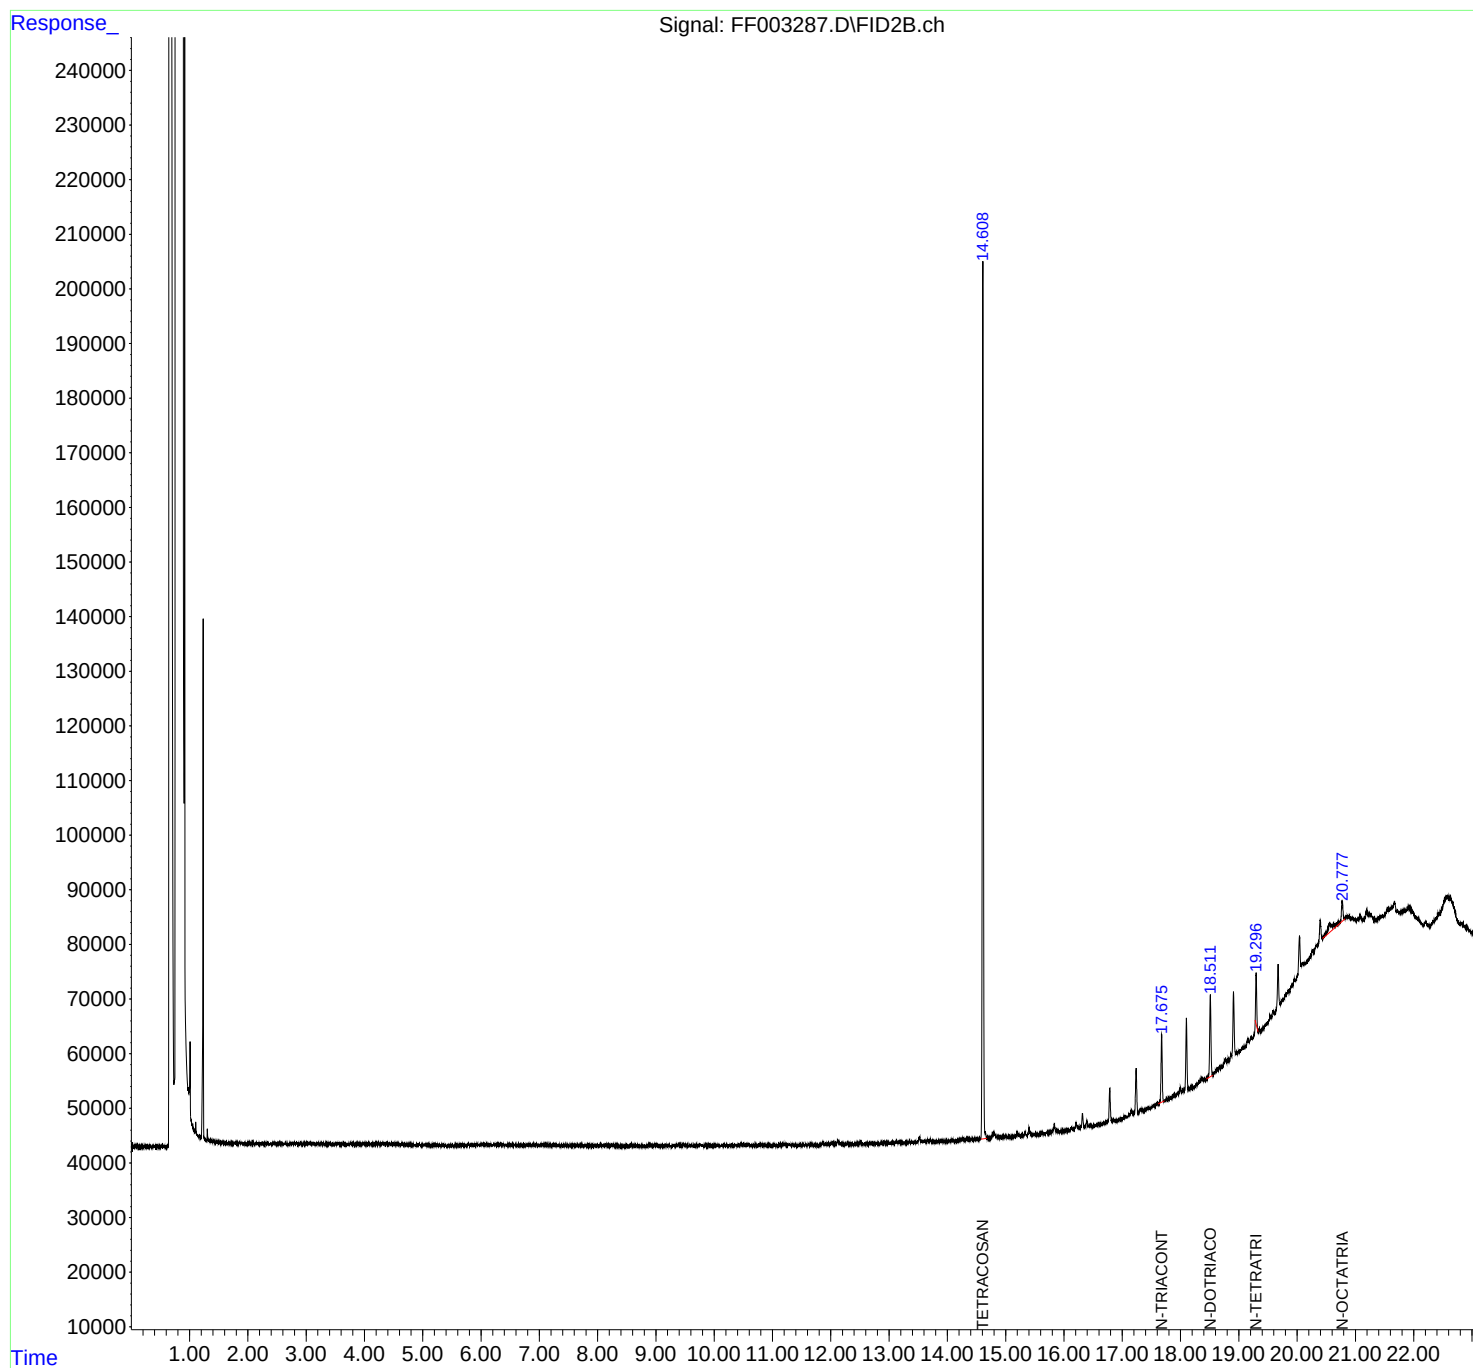


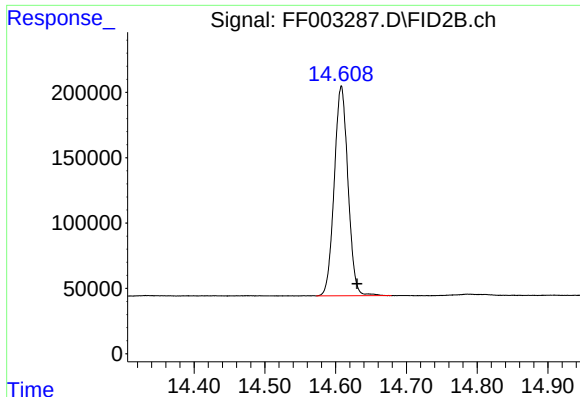

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.608 min
Delta R.T.: -0.022 min
Response: 2164096
Conc: 15.12 ug/ml

Instrument :
FID_F
ClientSampleId :

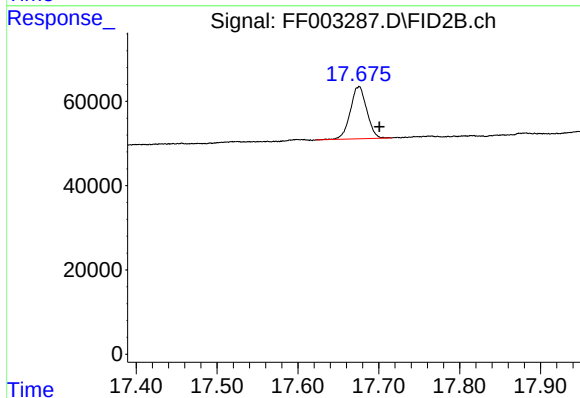


#13 N-TRIACONTANE

R.T.: 17.675 min
Delta R.T.: -0.025 min
Response: 174198
Conc: 1.11 ug/ml

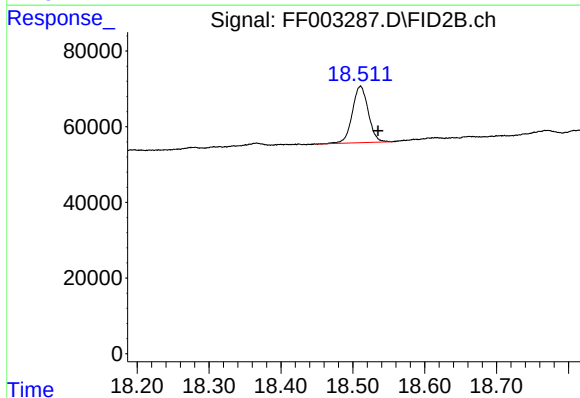


#14 N-DOTRIACONTANE

R.T.: 18.511 min
Delta R.T.: -0.025 min
Response: 228739
Conc: 1.57 ug/ml

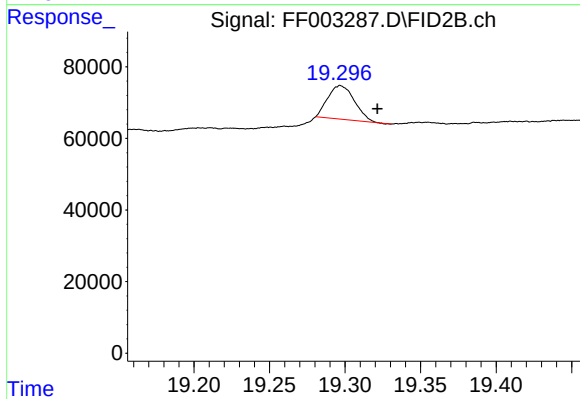

#15 N-TETRATRIACONTANE

R.T.: 19.297 min
Delta R.T.: -0.025 min
Response: 115358
Conc: 0.87 ug/ml

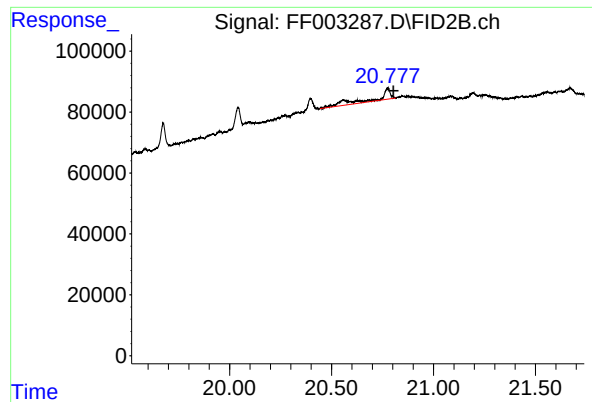

#17 N-OCTATRIACONTANE

R.T.: 20.775 min
Delta R.T.: -0.029 min
Response: 173983
Conc: 1.67 ug/ml

Instrument :
FID_F
ClientSampleId :