

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011720\
 Data File : FF006224.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jan 2020 16:26
 Operator : DD\AJ
 Sample : L1155-05
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 17 21:55:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.633	1175980	10.853 ug/ml
Target Compounds			
4) N-TETRADECANE	8.259f	277888	2.202 ug/ml
10) N-TETRACOSANE	14.824	168223	1.350 ug/ml
11) N-HEXACOSANE	15.855	204844	1.666 ug/ml
12) N-OCTACOSANE	16.802	442872	3.643 ug/ml
13) N-TRIACONTANE	17.686	434488	3.624 ug/ml
14) N-DOTRIACONTANE	18.515	1635117	14.149 ug/ml
15) N-TETRATRIACONTANE	19.298	102266	0.908 ug/ml
16) N-HEXATRIACONTANE	20.022	1112836	10.408 ug/ml
17) N-OCTATRIACONTANE	20.732	496900	5.371 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011720\
Data File : FF006224.D
Signal(s) : FID2B.ch
Acq On : 17 Jan 2020 16:26
Operator : DD\AJ
Sample : L1155-05
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 17 21:55:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

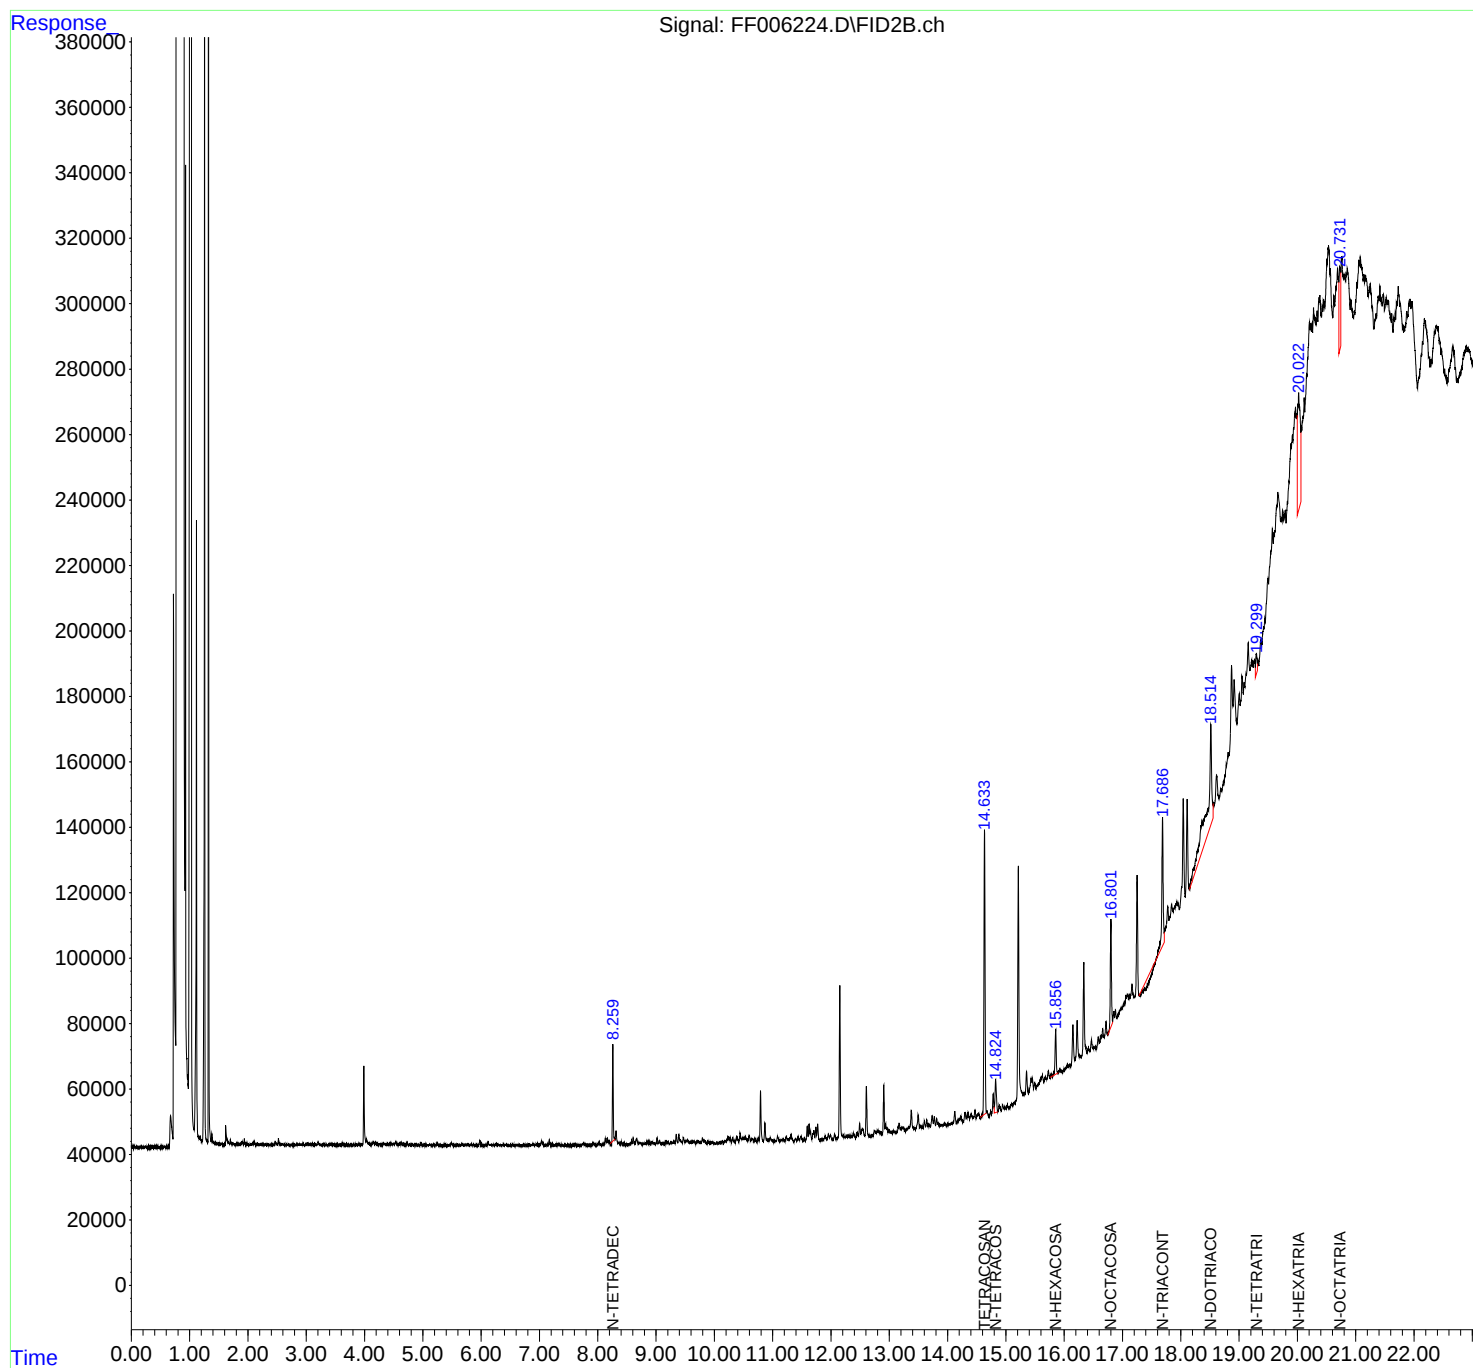

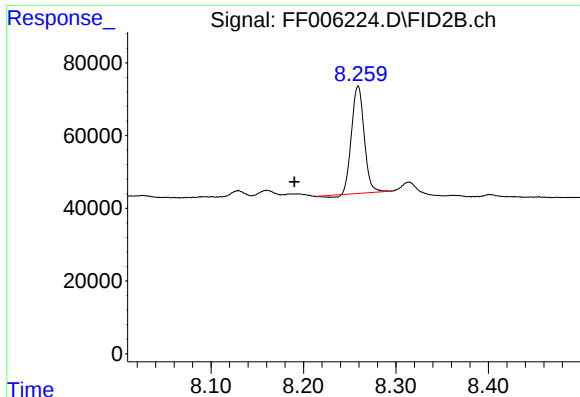


#4 N-TETRADECANE

R.T.: 8.259 min
Delta R.T.: 0.069 min
Response: 277888
Conc: 2.20 ug/ml

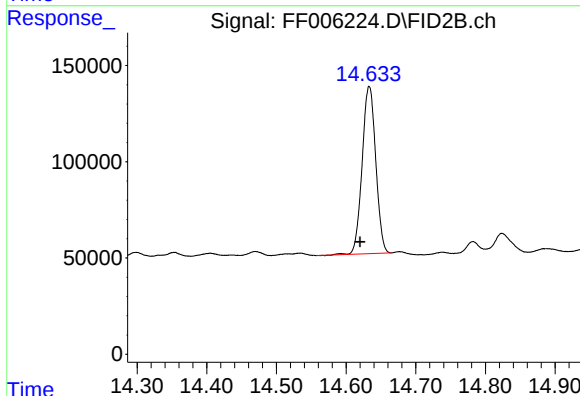


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.633 min
Delta R.T.: 0.013 min
Response: 1175980
Conc: 10.85 ug/ml

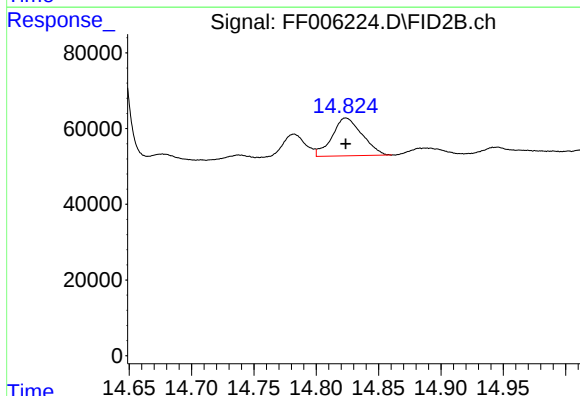


#10 N-TETRACOSANE

R.T.: 14.824 min
Delta R.T.: 0.000 min
Response: 168223
Conc: 1.35 ug/ml

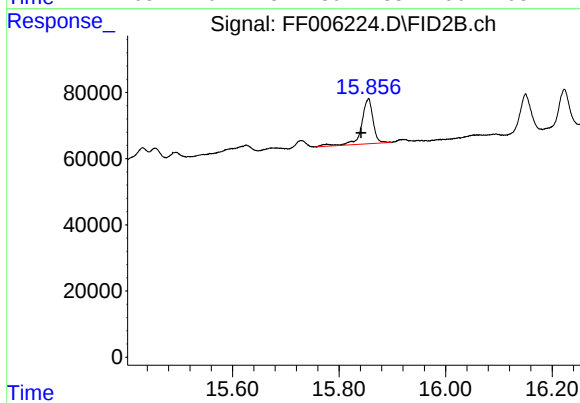


#11 N-HEXACOSANE

R.T.: 15.855 min
Delta R.T.: 0.014 min
Response: 204844
Conc: 1.67 ug/ml

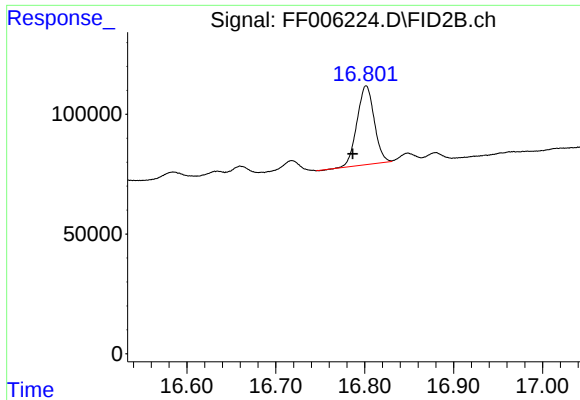


#12 N-OCTACOSANE

R.T.: 16.802 min
Delta R.T.: 0.015 min
Response: 442872
Conc: 3.64 ug/ml

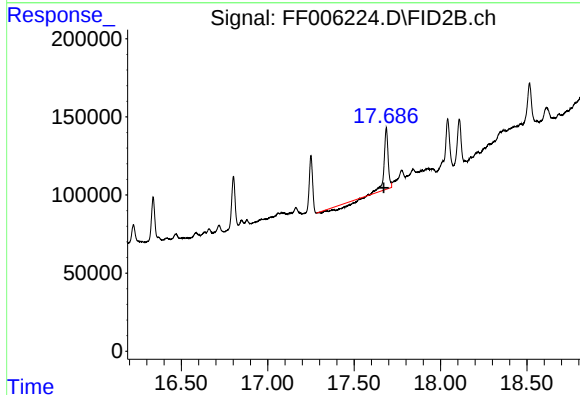


#13 N-TRIACONTANE

R.T.: 17.686 min
Delta R.T.: 0.015 min
Response: 434488
Conc: 3.62 ug/ml

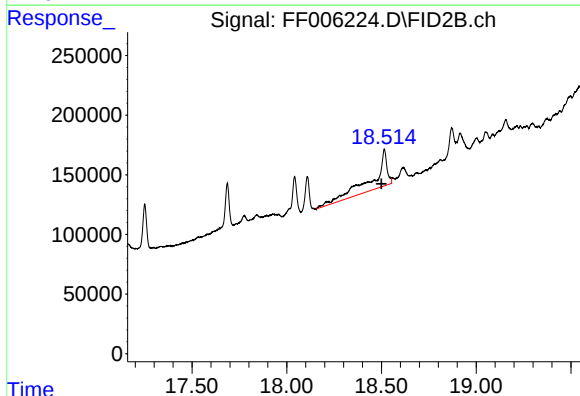


#14 N-DOTRIACONTANE

R.T.: 18.515 min
Delta R.T.: 0.014 min
Response: 1635117
Conc: 14.15 ug/ml

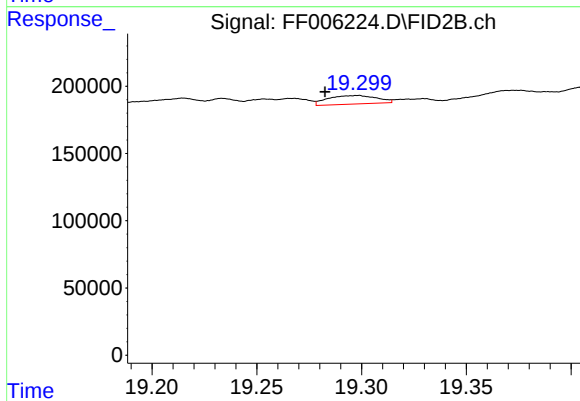


#15 N-TETRATRIACONTANE

R.T.: 19.298 min
Delta R.T.: 0.015 min
Response: 102266
Conc: 0.91 ug/ml

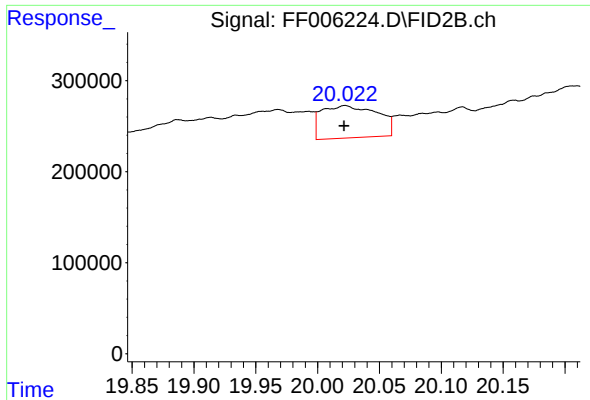

#16 N-HEXATRIACONTANE

R.T.: 20.022 min
Delta R.T.: 0.000 min
Response: 1112836
Conc: 10.41 ug/ml

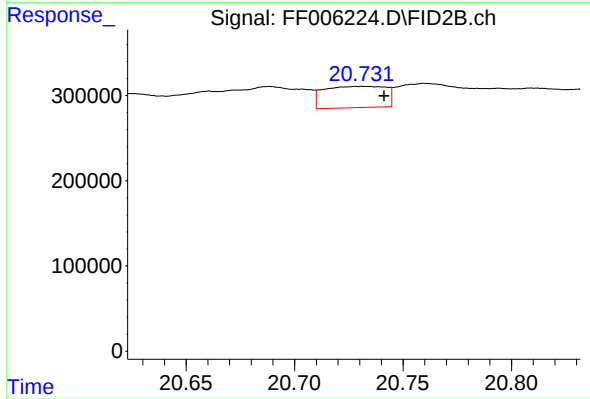

#17 N-OCTATRIACONTANE

R.T.: 20.732 min
Delta R.T.: -0.010 min
Response: 496900
Conc: 5.37 ug/ml