

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011722\
Data File : FF009674.D
Signal(s) : FID2B.ch
Acq On : 17 Jan 2022 18:05
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 18 02:54:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
12) N-OCTACOSANE	16.614	73498	0.506 ug/ml
13) N-TRIACONTANE	17.501	120441	0.842 ug/ml
14) N-DOTRIACONTANE	18.331	104294	0.766 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011722\
Data File : FF009674.D
Signal(s) : FID2B.ch
Acq On : 17 Jan 2022 18:05
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 18 02:54:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

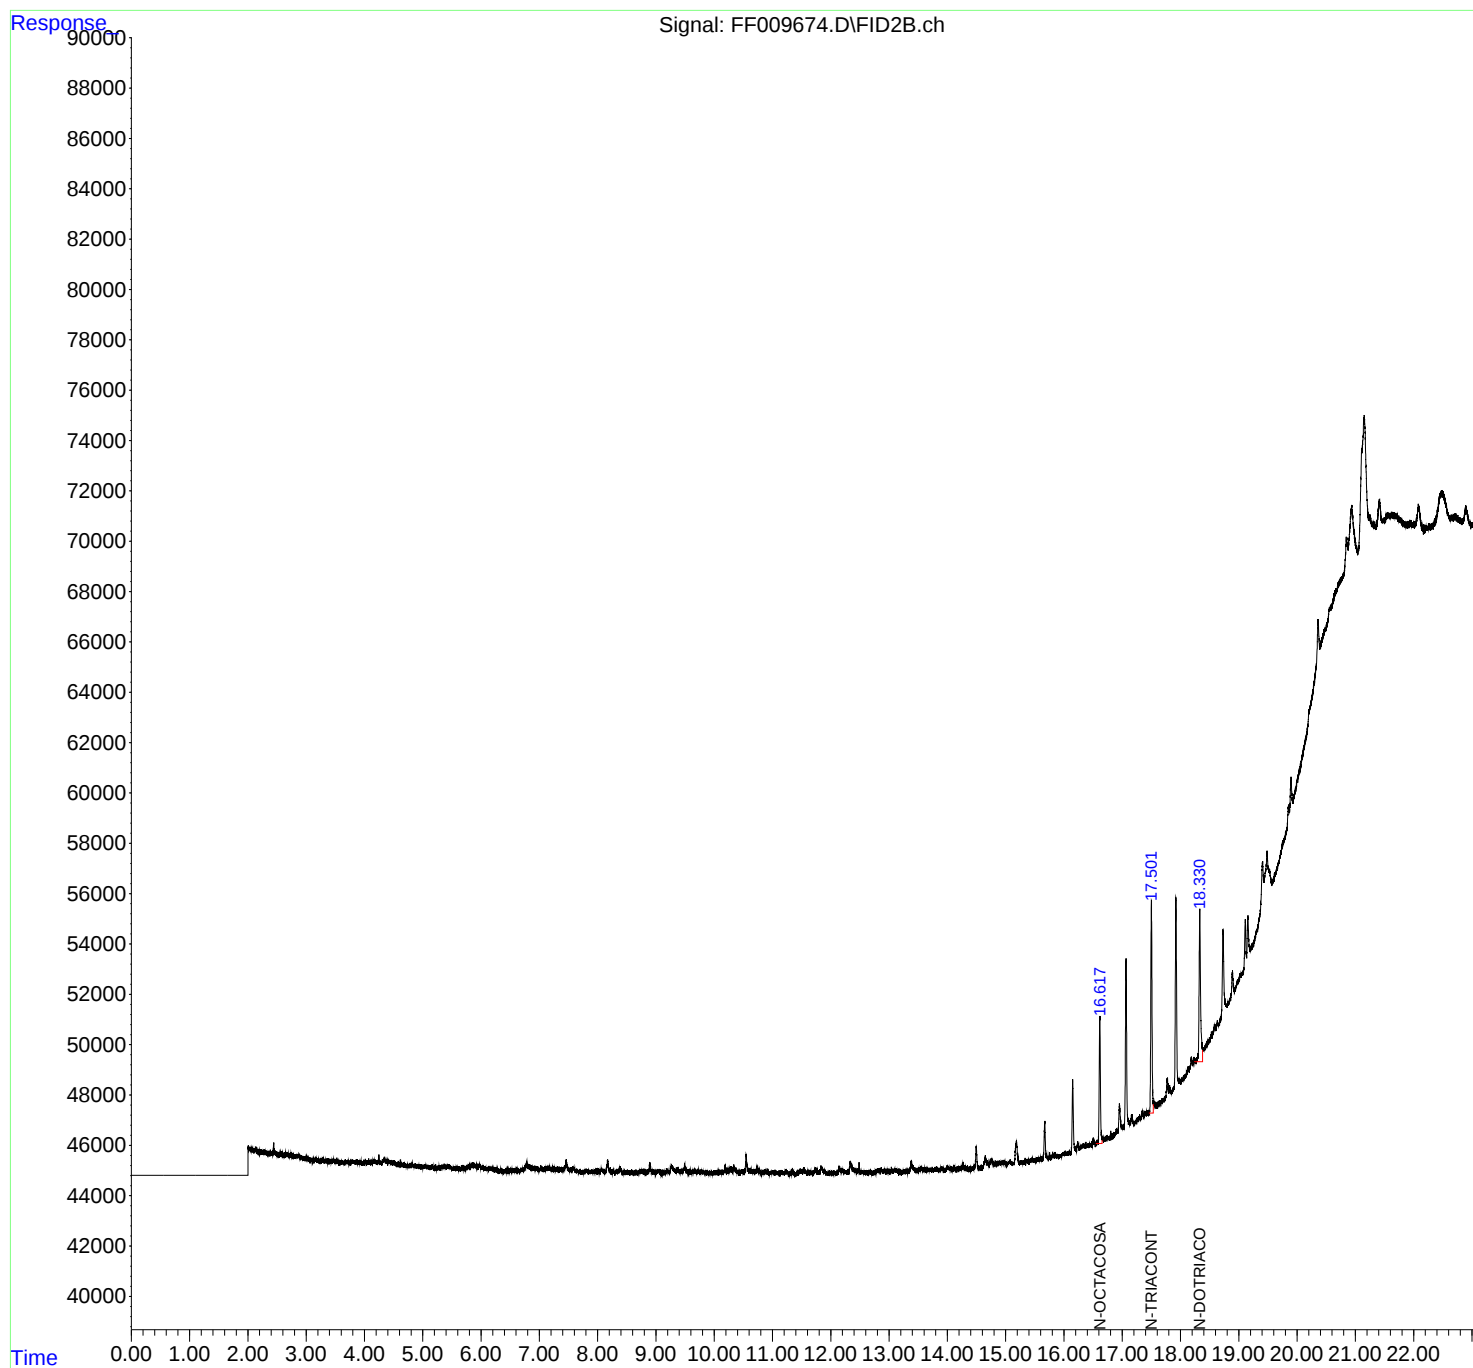


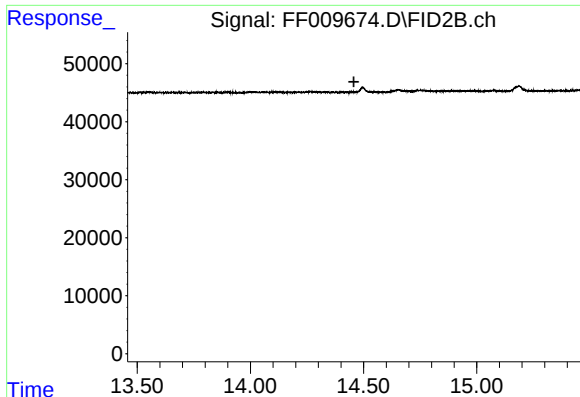

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.457 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

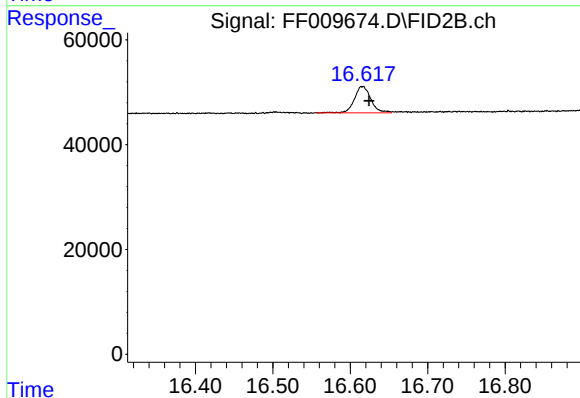


#12 N-OCTACOSANE

R.T.: 16.614 min
Delta R.T.: -0.010 min
Response: 73498
Conc: 0.51 ug/ml

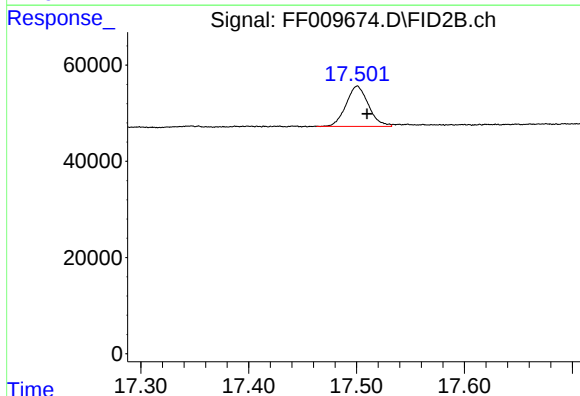

#13 N-TRIACONTANE

R.T.: 17.501 min
Delta R.T.: -0.009 min
Response: 120441
Conc: 0.84 ug/ml

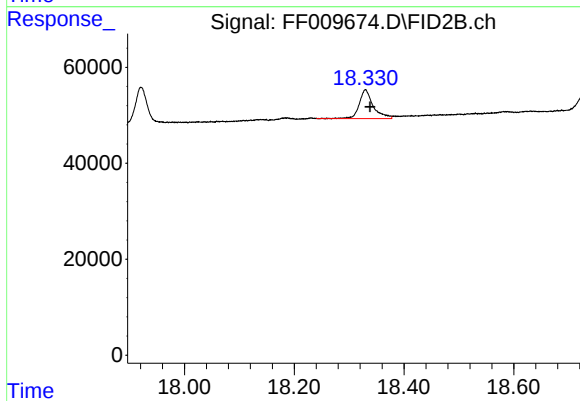

#14 N-DOTRIACONTANE

R.T.: 18.331 min
Delta R.T.: -0.008 min
Response: 104294
Conc: 0.77 ug/ml