

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011725\
 Data File : FF015249.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jan 2025 12:14
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 17 22:12:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011425.M
 Quant Title :
 QLast Update : Tue Jan 14 11:12:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.732	2625198	19.191 ug/ml
12) N-OCTACOSANE	17.192	2533625	18.488 ug/ml
13) N-TRIACONTANE	18.080	56195	0.422 ug/ml
14) N-DOTRIACONTANE	18.913	93677	0.737 ug/ml
15) N-TETRATRIACONTANE	19.696	60721	0.548 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011725\
Data File : FF015249.D
Signal(s) : FID2B.ch
Acq On : 17 Jan 2025 12:14
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 17 22:12:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011425.M
Quant Title :
QLast Update : Tue Jan 14 11:12:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

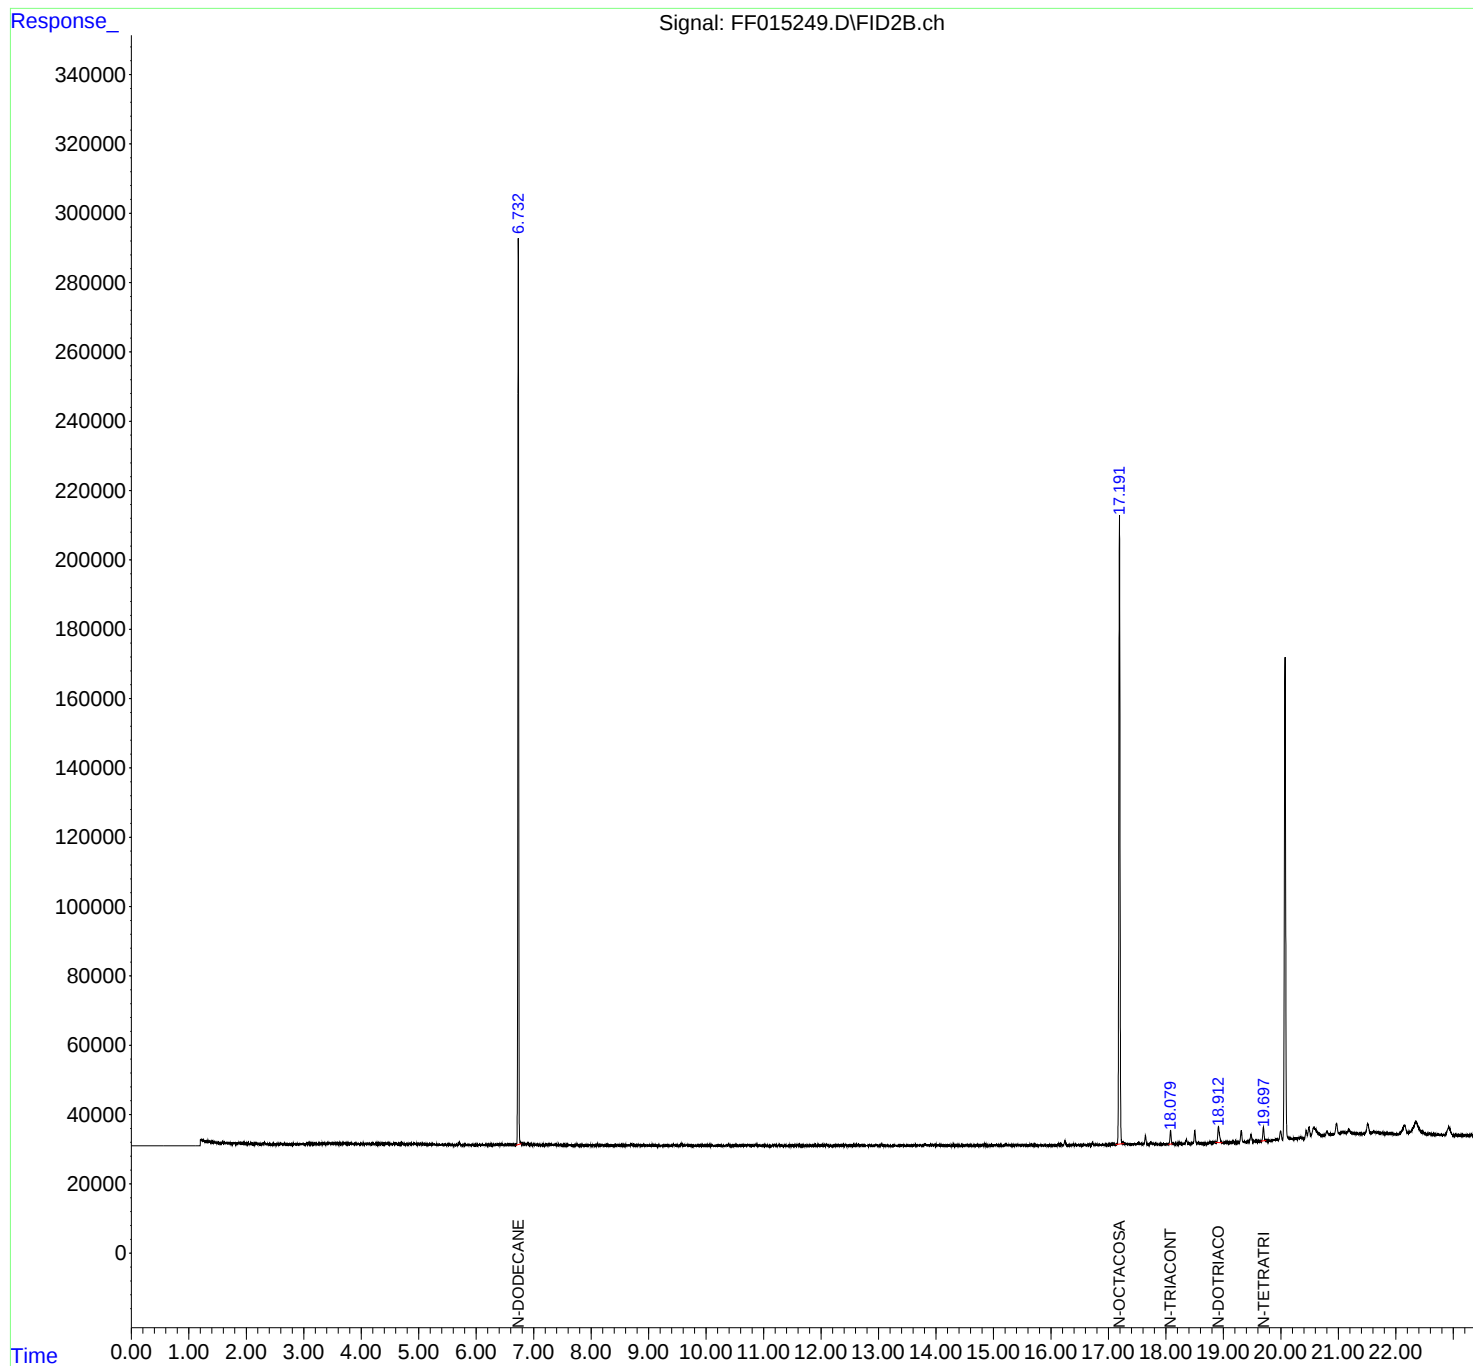


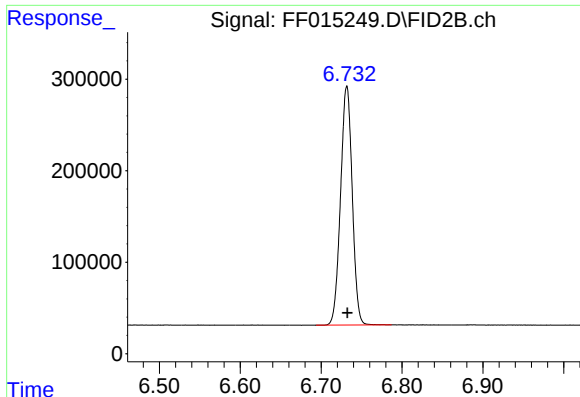

#3 N-DODECANE


R.T.: 6.732 min
Delta R.T.: 0.000 min
Response: 2625198
Conc: 19.19 ug/ml

Instrument :
FID_F
ClientSampleId :

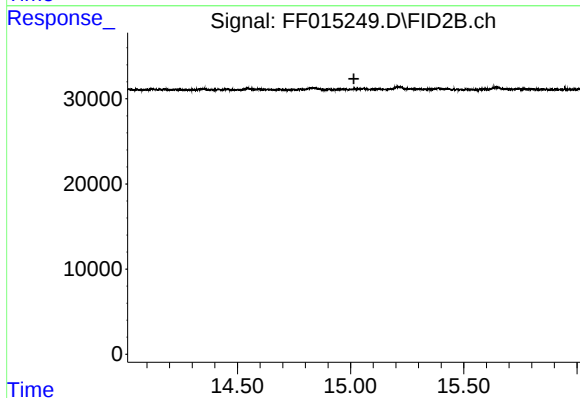


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.015 min
Response: 0
Conc: N.D.

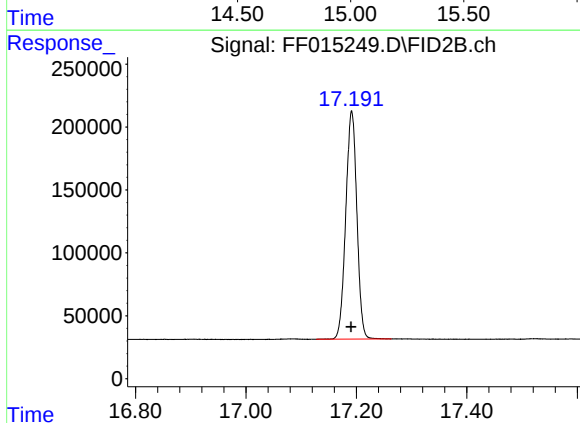


#12 N-OCTACOSANE

R.T.: 17.192 min
Delta R.T.: 0.001 min
Response: 2533625
Conc: 18.49 ug/ml

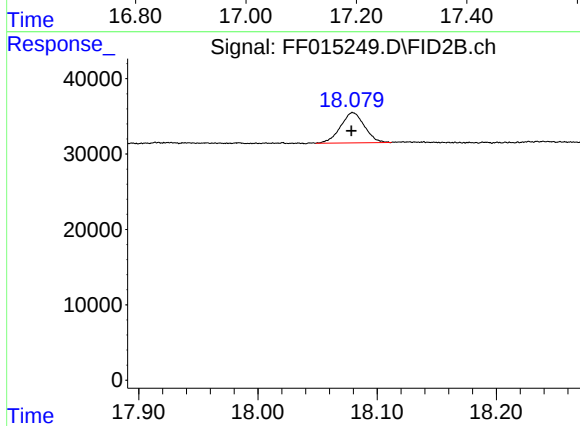

#13 N-TRIACONTANE


R.T.: 18.080 min
Delta R.T.: 0.001 min
Response: 56195
Conc: 0.42 ug/ml

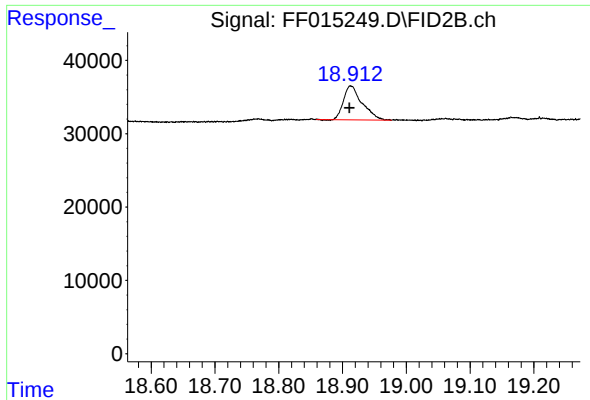

#14 N-DOTRIACONTANE

R.T.: 18.913 min
Delta R.T.: 0.002 min
Response: 93677
Conc: 0.74 ug/ml

Instrument :
FID_F
ClientSampleId :

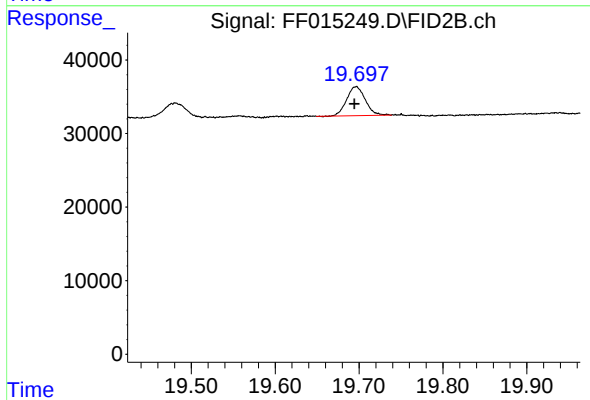

#15 N-TETRATRIACONTANE

R.T.: 19.696 min
Delta R.T.: 0.002 min
Response: 60721
Conc: 0.55 ug/ml