

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
 Data File : FF003292.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jan 2019 09:47
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 18 20:53:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.361	3770678	23.245 ug/ml
12) N-OCTACOSANE	16.789	3509276	22.280 ug/ml
13) N-TRIACONTANE	17.677	403605	2.571 ug/ml
14) N-DOTRIACONTANE	18.513	448146	3.082 ug/ml
15) N-TETRATRIACONTANE	19.299	257874	1.951 ug/ml
16) N-HEXATRIACONTANE	20.044	108114	0.916 ug/ml
17) N-OCTATRIACONTANE	20.778	129069	1.235 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
Data File : FF003292.D
Signal(s) : FID2B.ch
Acq On : 18 Jan 2019 09:47
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 18 20:53:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

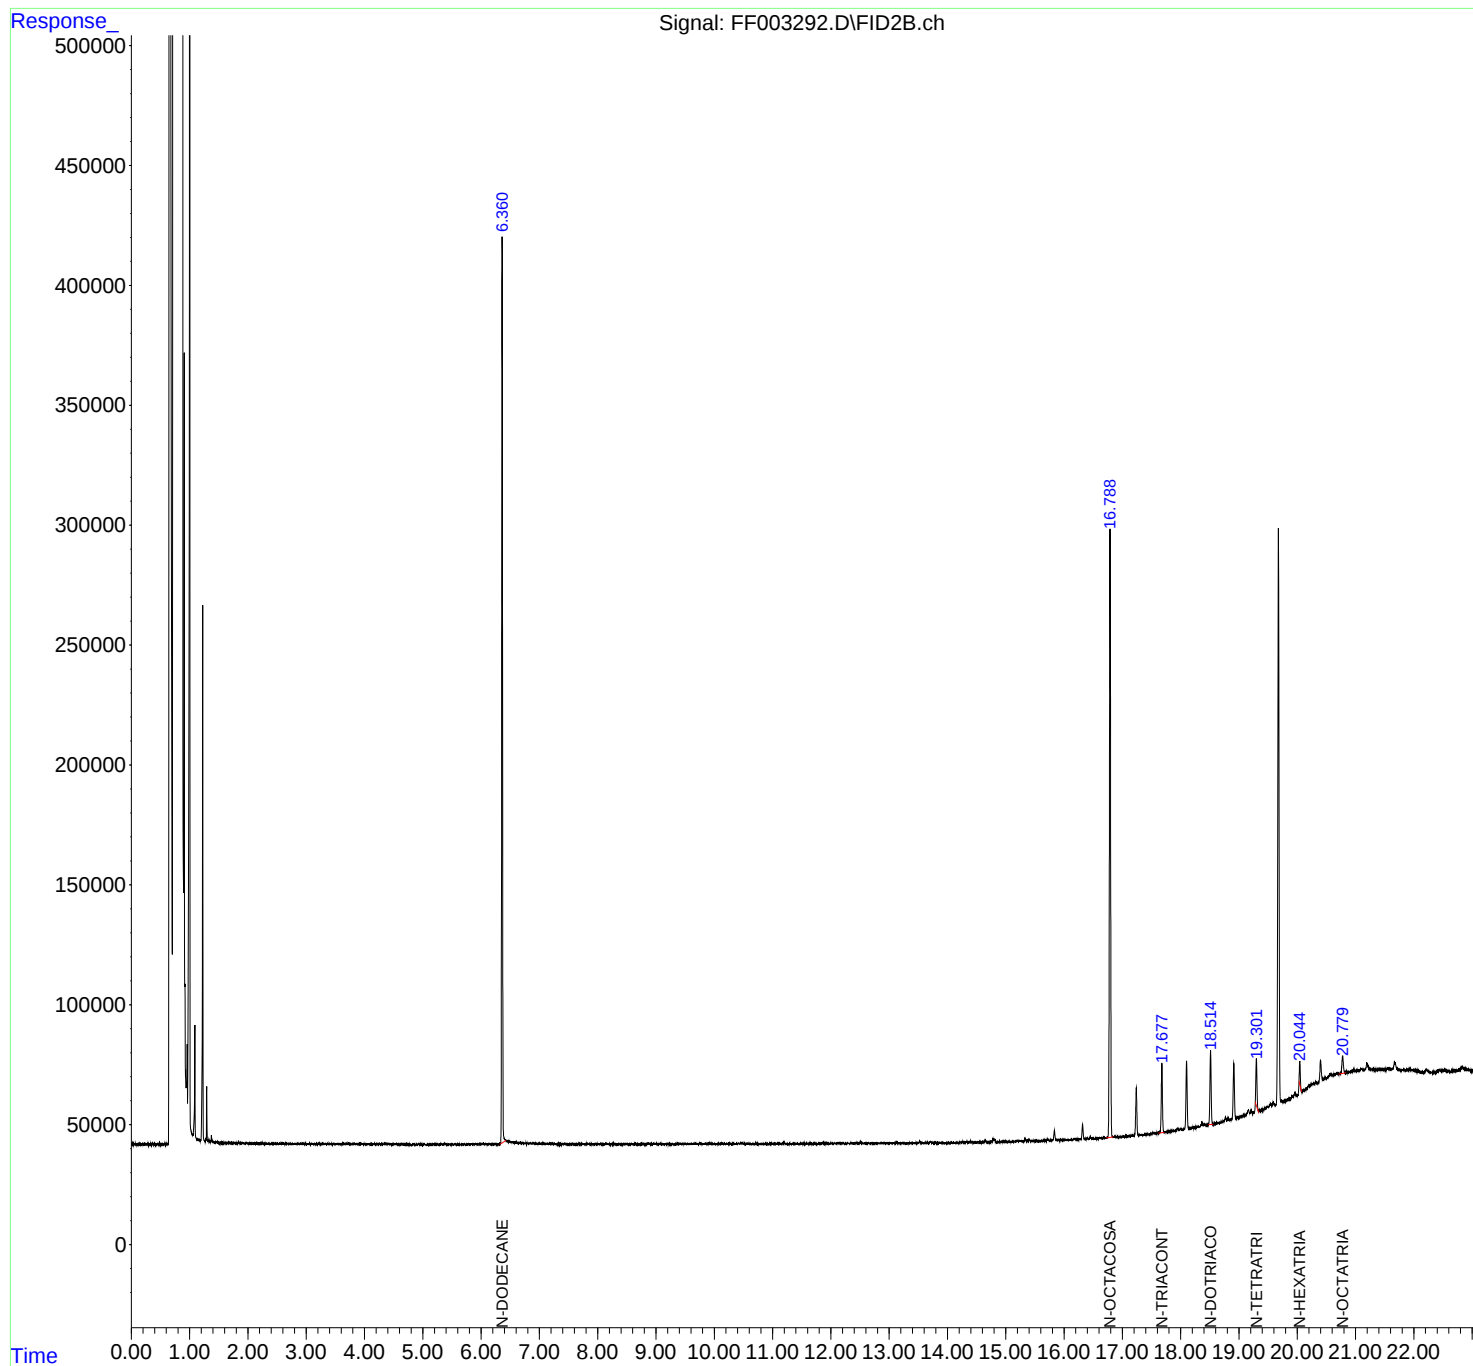


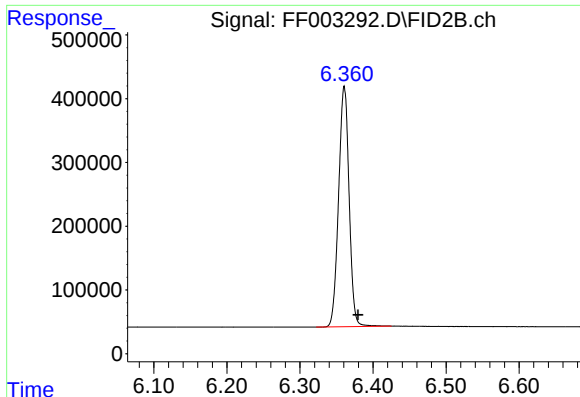

#3 N-DODECANE


R.T.: 6.361 min
Delta R.T.: -0.019 min
Response: 3770678
Conc: 23.24 ug/ml

Instrument :
FID_F
ClientSampleId :

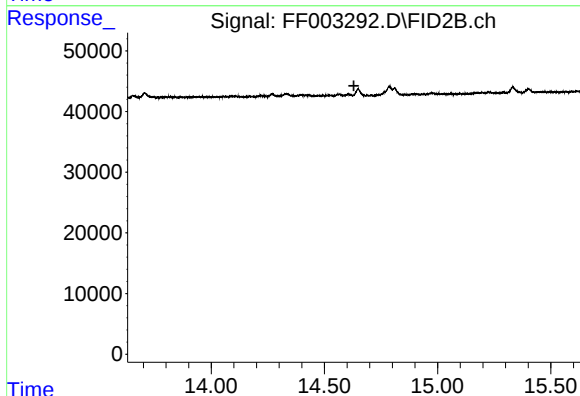


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.630 min
Response: 0
Conc: N.D.

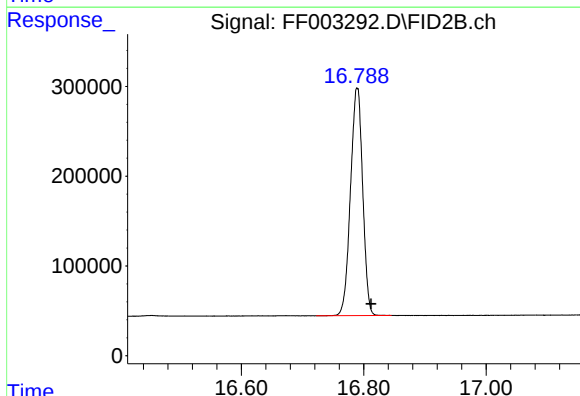


#12 N-OCTACOSANE

R.T.: 16.789 min
Delta R.T.: -0.023 min
Response: 3509276
Conc: 22.28 ug/ml

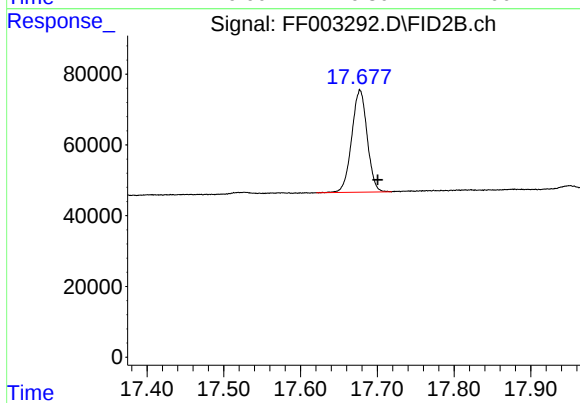

#13 N-TRIACONTANE


R.T.: 17.677 min
Delta R.T.: -0.023 min
Response: 403605
Conc: 2.57 ug/ml

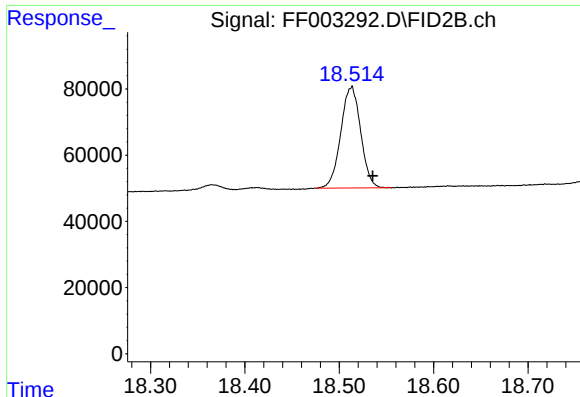

#14 N-DOTRIACONTANE


R.T.: 18.513 min
Delta R.T.: -0.022 min
Response: 448146
Conc: 3.08 ug/ml

Instrument :
FID_F
ClientSampleId :

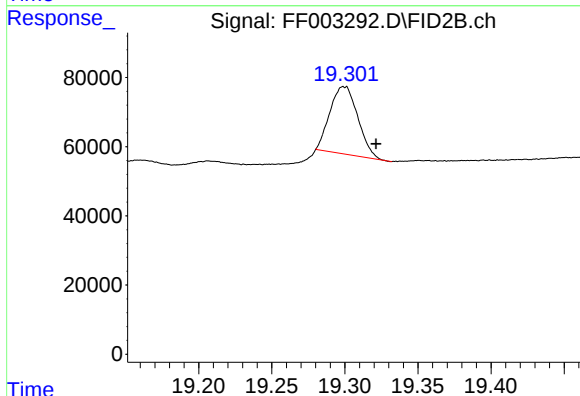


#15 N-TETRATRIACONTANE

R.T.: 19.299 min
Delta R.T.: -0.022 min
Response: 257874
Conc: 1.95 ug/ml

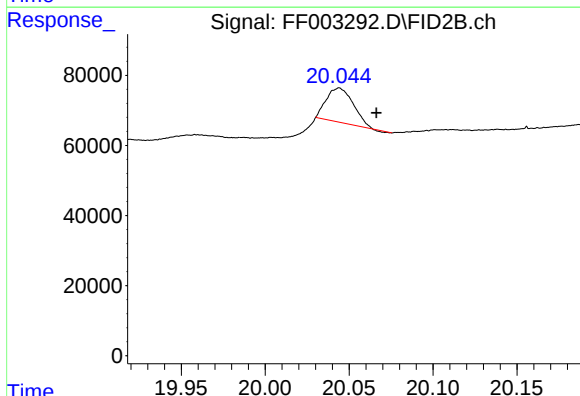

#16 N-HEXATRIACONTANE

R.T.: 20.044 min
Delta R.T.: -0.022 min
Response: 108114
Conc: 0.92 ug/ml

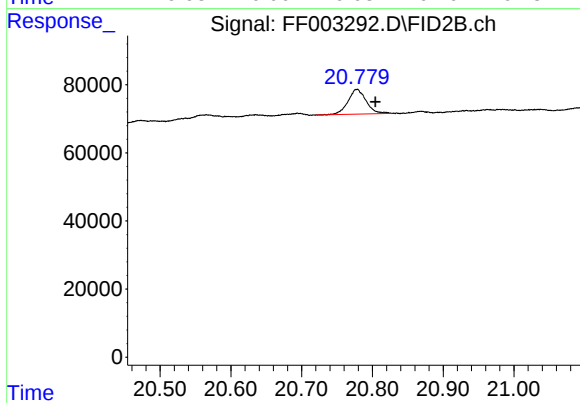

#17 N-OCTATRIACONTANE

R.T.: 20.778 min
Delta R.T.: -0.026 min
Response: 129069
Conc: 1.24 ug/ml