

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
 Data File : FF003293.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jan 2019 10:30
 Operator : AJ\SJ
 Sample : K1157-13RE
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 WC-07-011519RE

Integration File: autoint1.e
 Quant Time: Jan 18 20:53:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.607	821583	5.742 ug/ml
Target Compounds			
4) N-TETRADECANE	8.208	104358	0.639 ug/ml
7) N-EICOSANE	12.558	170944	1.041 ug/ml
10) N-TETRACOSANE	14.782f	159988	0.998 ug/ml
11) N-HEXACOSANE	15.834	150992	0.955 ug/ml
12) N-OCTACOSANE	16.788	367665	2.334 ug/ml
13) N-TRIACONTANE	17.679	494527	3.150 ug/ml
14) N-DOTRIACONTANE	18.513	422561	2.906 ug/ml
15) N-TETRATRIACONTANE	19.361	77355	0.585 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
Data File : FF003293.D
Signal(s) : FID2B.ch
Acq On : 18 Jan 2019 10:30
Operator : AJ\SJ
Sample : K1157-13RE
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WC-07-011519RE

Integration File: autoint1.e
Quant Time: Jan 18 20:53:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

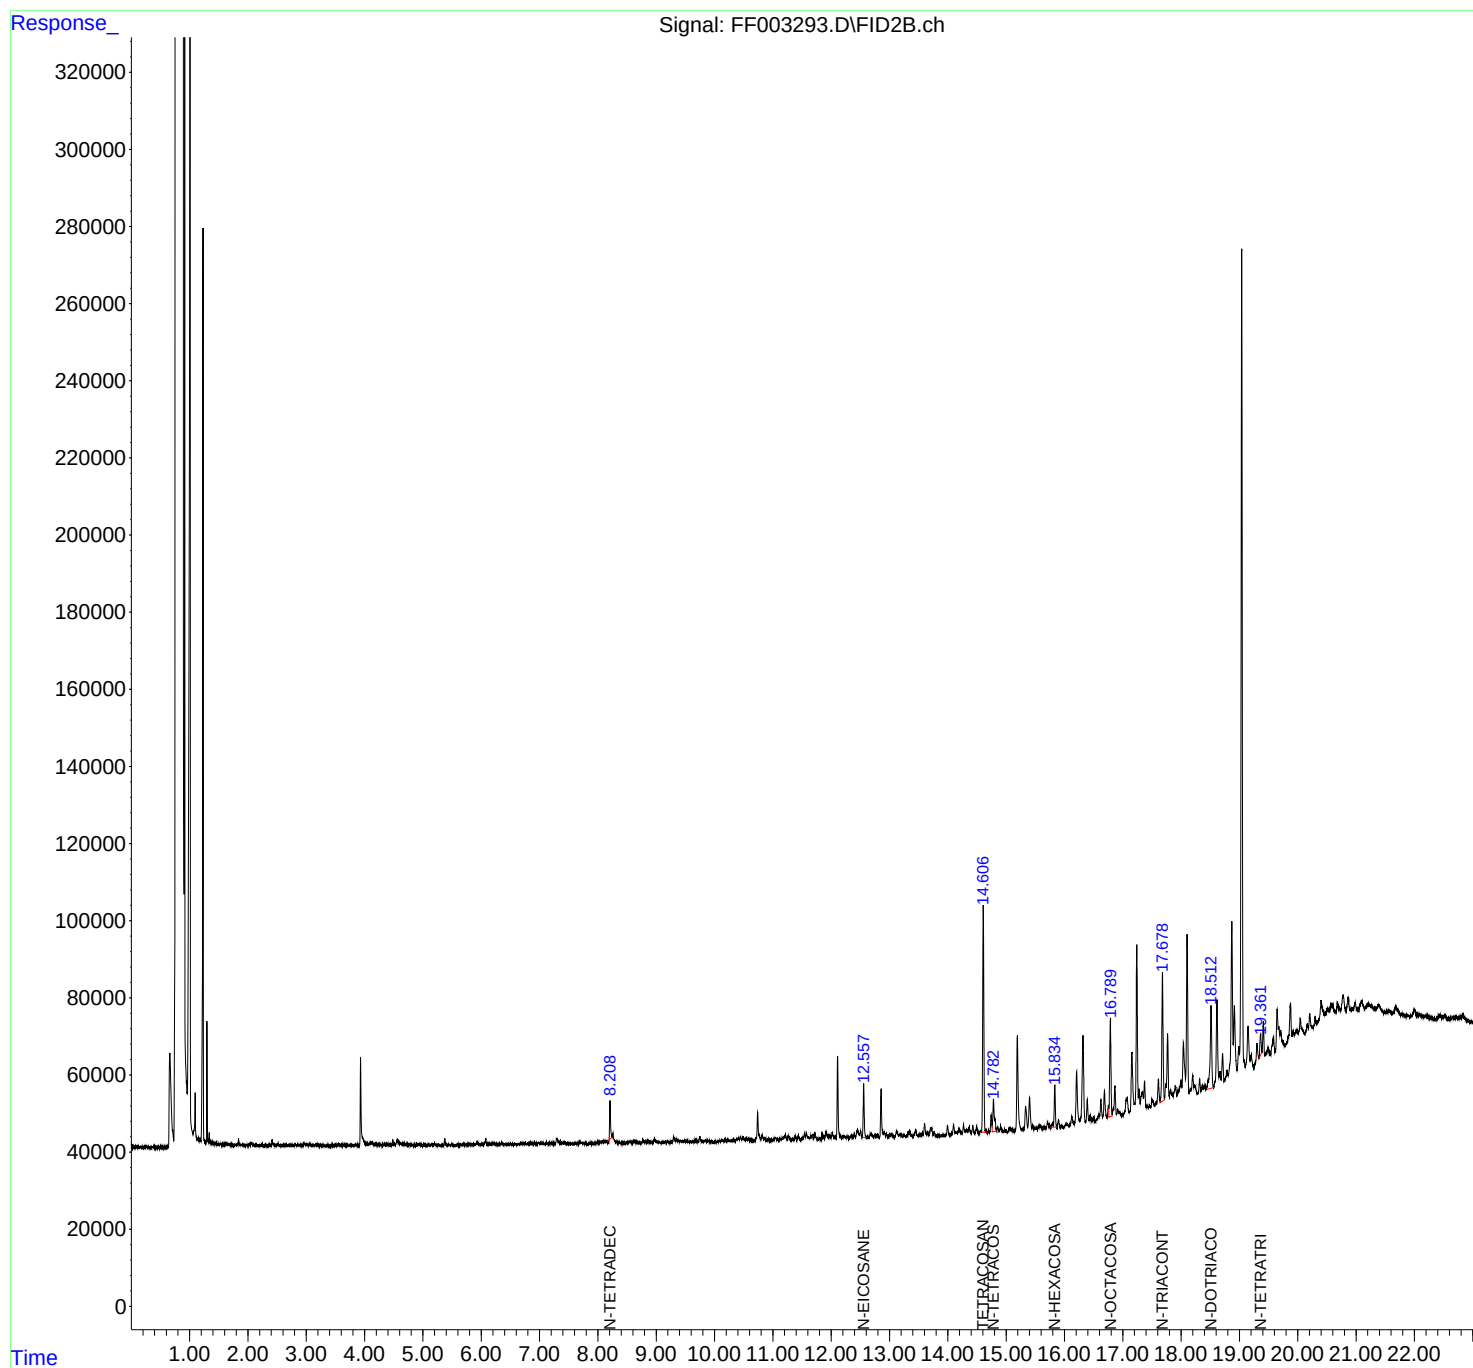


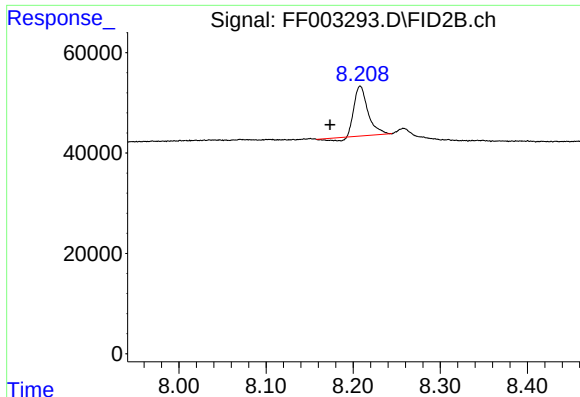

#4 N-TETRADECANE


R.T.: 8.208 min
Delta R.T.: 0.035 min
Response: 104358
Conc: 0.64 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-07-011519RE

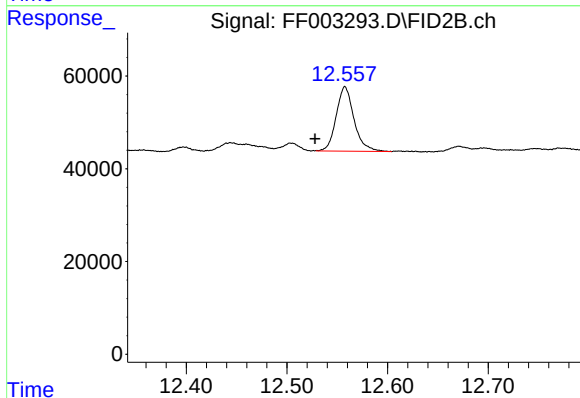


#7 N-EICOSANE

R.T.: 12.558 min
Delta R.T.: 0.030 min
Response: 170944
Conc: 1.04 ug/ml

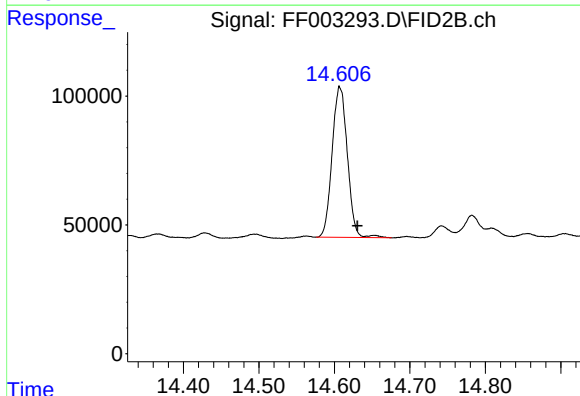


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.607 min
Delta R.T.: -0.023 min
Response: 821583
Conc: 5.74 ug/ml

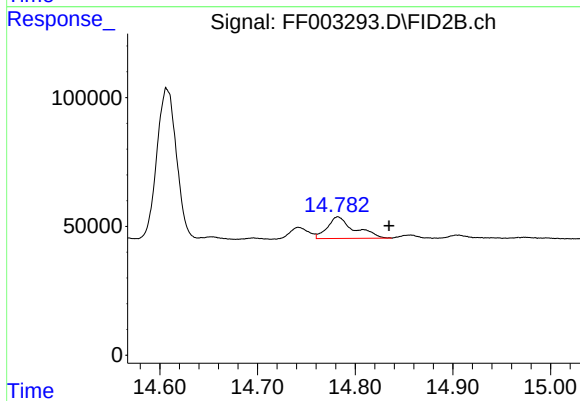

#10 N-TETRACOSANE


R.T.: 14.782 min
Delta R.T.: -0.052 min
Response: 159988
Conc: 1.00 ug/ml

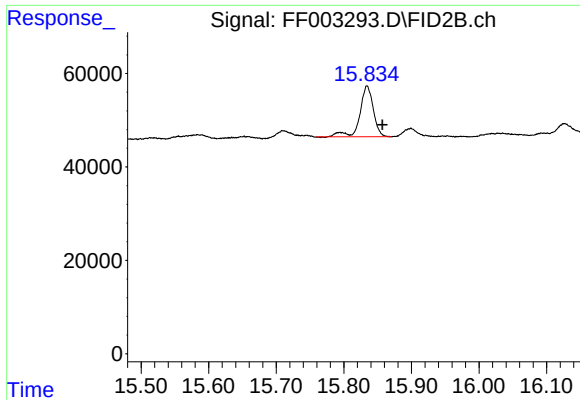

#11 N-HEXACOSANE


R.T.: 15.834 min
Delta R.T.: -0.023 min
Response: 150992
Conc: 0.95 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-07-011519RE

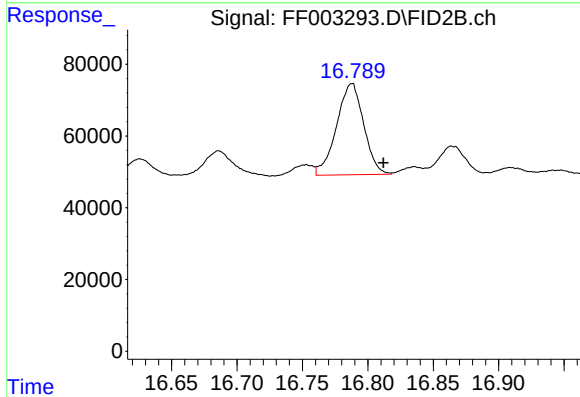


#12 N-OCTACOSANE

R.T.: 16.788 min
Delta R.T.: -0.024 min
Response: 367665
Conc: 2.33 ug/ml

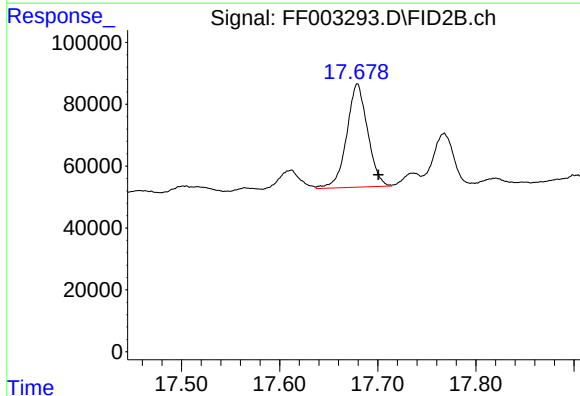


#13 N-TRIACONTANE

R.T.: 17.679 min
Delta R.T.: -0.022 min
Response: 494527
Conc: 3.15 ug/ml

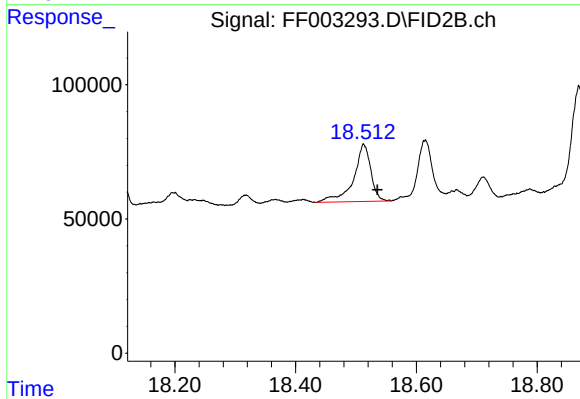

#14 N-DOTRIACONTANE

R.T.: 18.513 min
Delta R.T.: -0.023 min
Response: 422561
Conc: 2.91 ug/ml

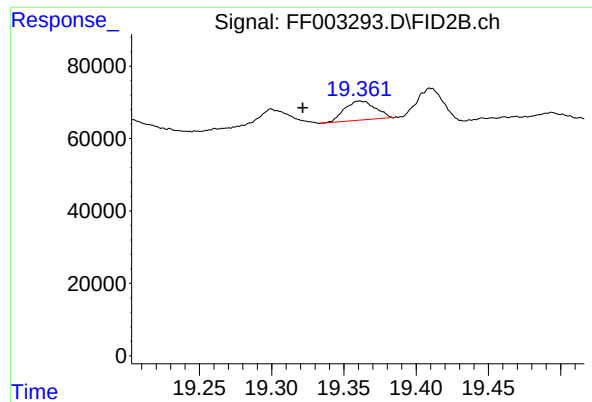

#15 N-TETRATRIACONTANE

R.T.: 19.361 min
Delta R.T.: 0.039 min
Response: 77355
Conc: 0.59 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-07-011519RE