

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
 Data File : FF003295.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jan 2019 11:29
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 18 20:53:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.606	2345071	16.389 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.787	92784	0.589 ug/ml
13) N-TRIACONTANE	17.676	201950	1.286 ug/ml
14) N-DOTRIACONTANE	18.511	249908	1.719 ug/ml
15) N-TETRATRIACONTANE	19.300	135971	1.028 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
Data File : FF003295.D
Signal(s) : FID2B.ch
Acq On : 18 Jan 2019 11:29
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 18 20:53:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

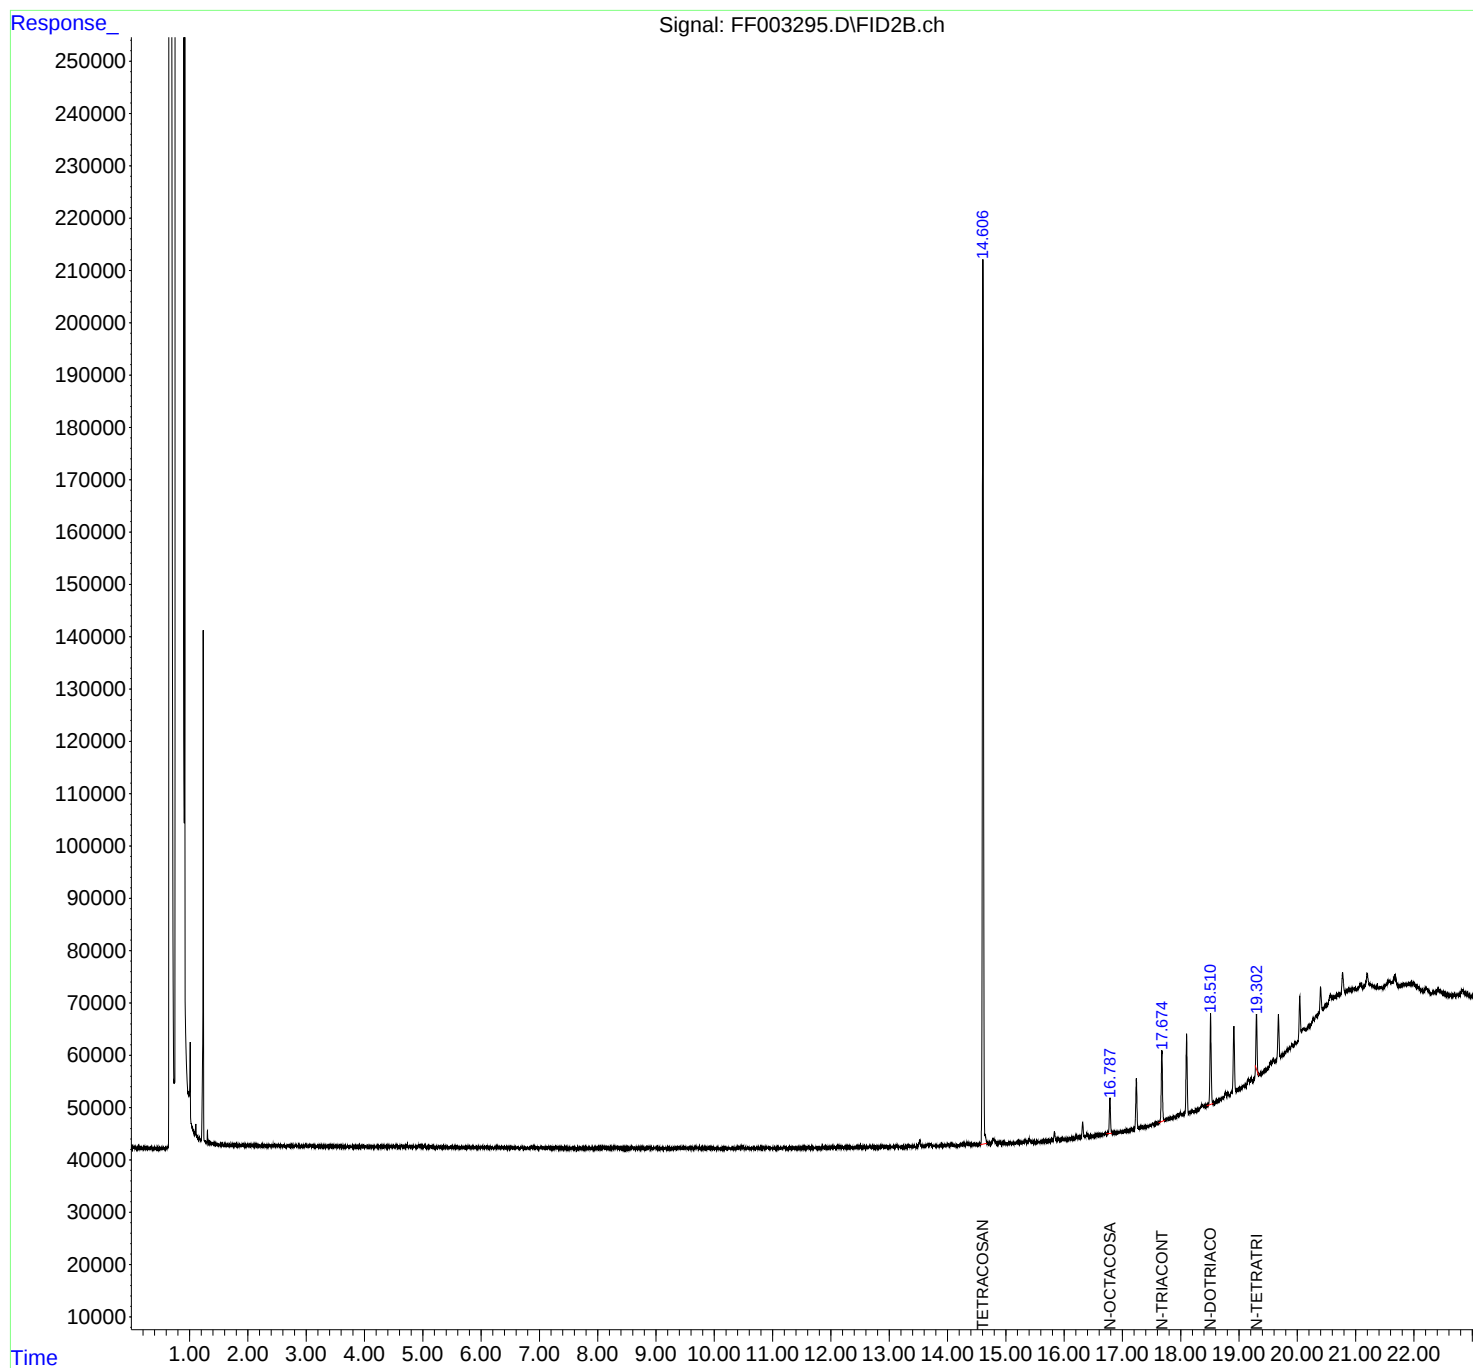


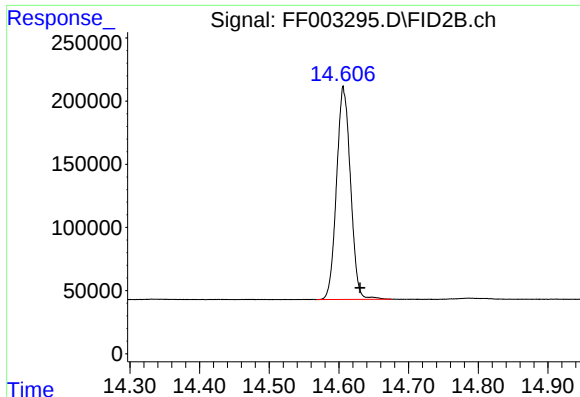

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.606 min
Delta R.T.: -0.024 min
Response: 2345071
Conc: 16.39 ug/ml

Instrument :
FID_F
ClientSampleId :

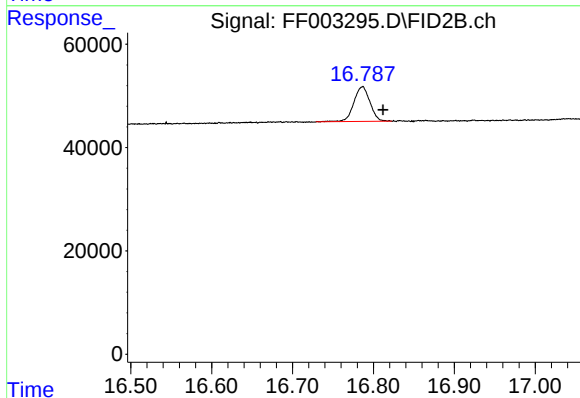


#12 N-OCTACOSANE

R.T.: 16.787 min
Delta R.T.: -0.025 min
Response: 92784
Conc: 0.59 ug/ml

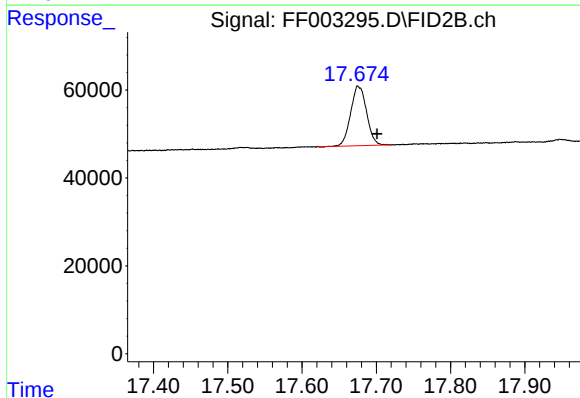


#13 N-TRIACONTANE

R.T.: 17.676 min
Delta R.T.: -0.025 min
Response: 201950
Conc: 1.29 ug/ml

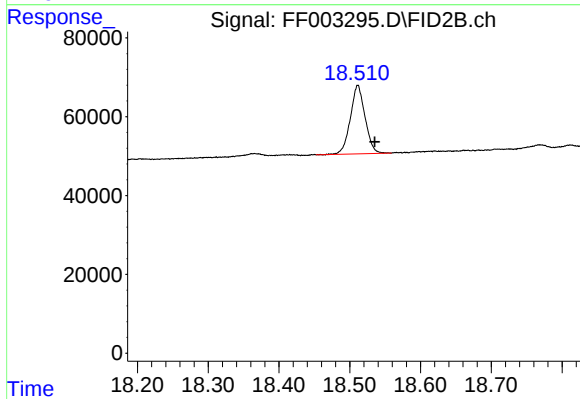

#14 N-DOTRIACONTANE

R.T.: 18.511 min
Delta R.T.: -0.024 min
Response: 249908
Conc: 1.72 ug/ml

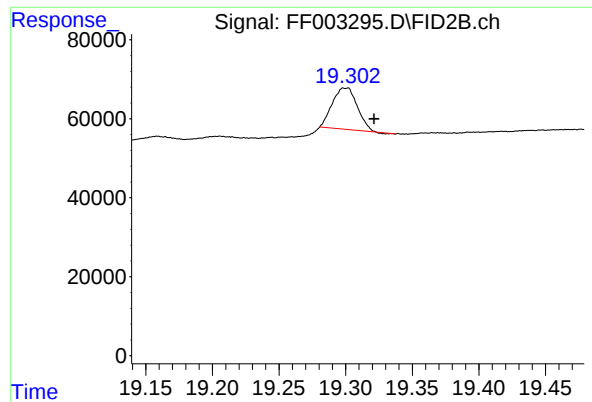

#15 N-TETRATRIACONTANE

R.T.: 19.300 min

Delta R.T.: -0.021 min

Response: 135971

Conc: 1.03 ug/ml

Instrument :
FID_F
ClientSampleId :