

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
 Data File : FF003297.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jan 2019 12:29
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 18 20:54:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.607	2498272	17.460 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.787	107247	0.681 ug/ml
13) N-TRIACONTANE	17.677	224564	1.430 ug/ml
14) N-DOTRIACONTANE	18.512	277860	1.911 ug/ml
15) N-TETRATRIACONTANE	19.298	159287	1.205 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
Data File : FF003297.D
Signal(s) : FID2B.ch
Acq On : 18 Jan 2019 12:29
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 18 20:54:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

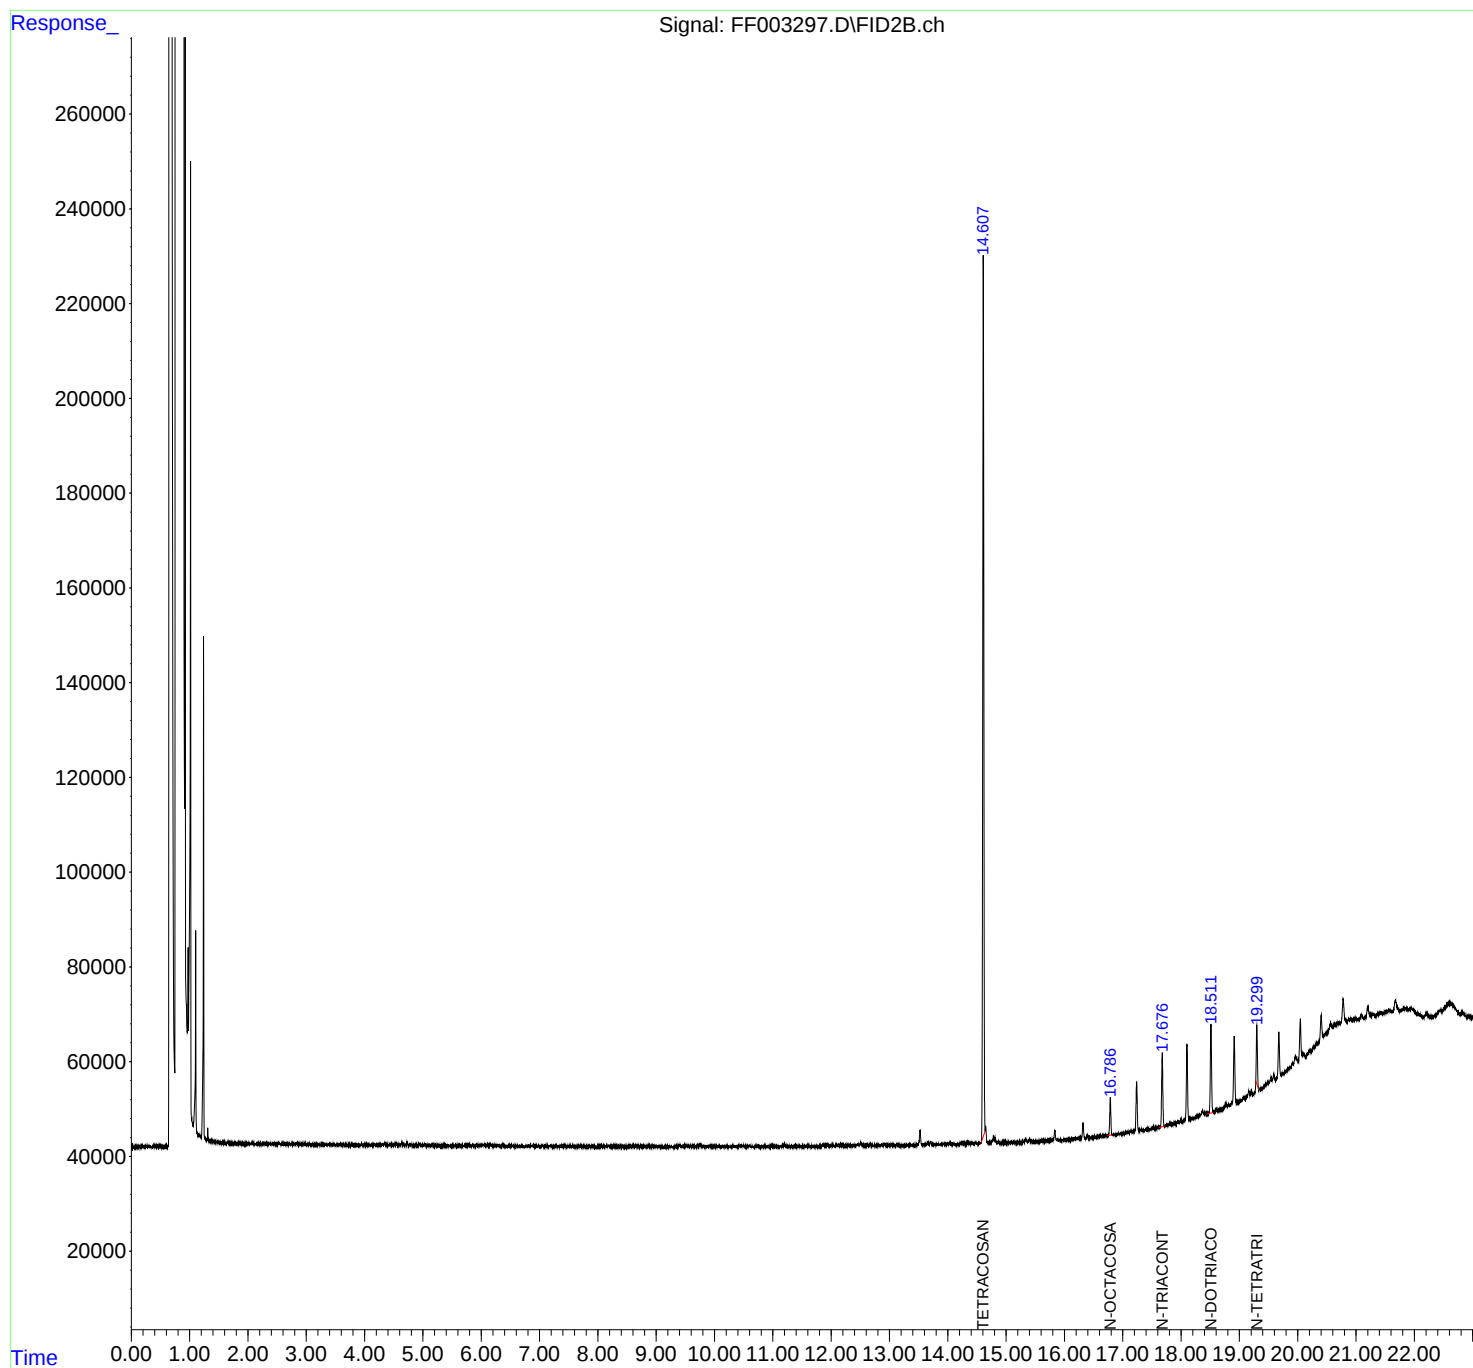


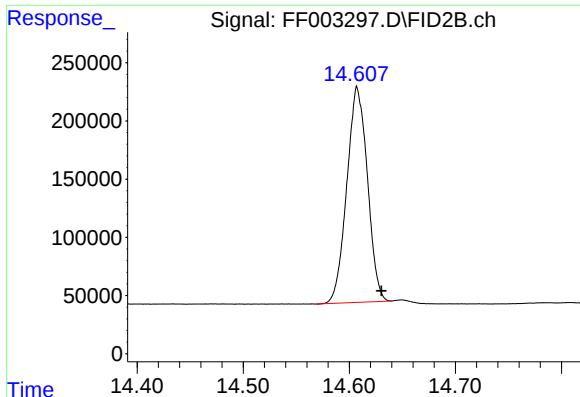

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.607 min
Delta R.T.: -0.023 min
Response: 2498272
Conc: 17.46 ug/ml

Instrument :
FID_F
ClientSampleId :

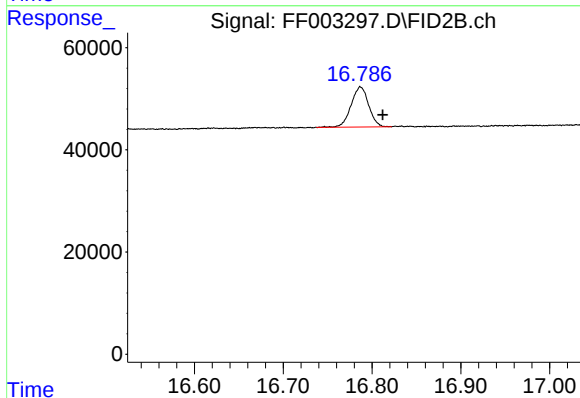


#12 N-OCTACOSANE

R.T.: 16.787 min
Delta R.T.: -0.025 min
Response: 107247
Conc: 0.68 ug/ml

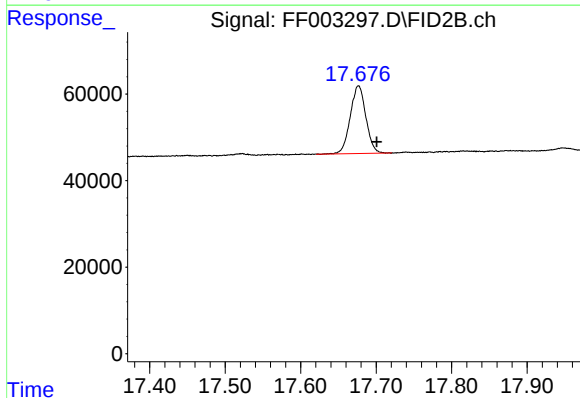


#13 N-TRIACONTANE

R.T.: 17.677 min
Delta R.T.: -0.024 min
Response: 224564
Conc: 1.43 ug/ml

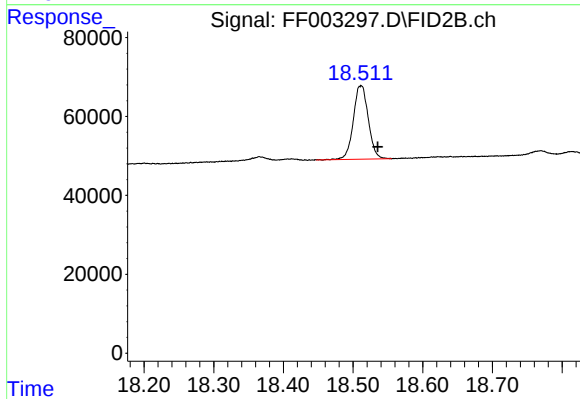

#14 N-DOTRIACONTANE

R.T.: 18.512 min
Delta R.T.: -0.024 min
Response: 277860
Conc: 1.91 ug/ml

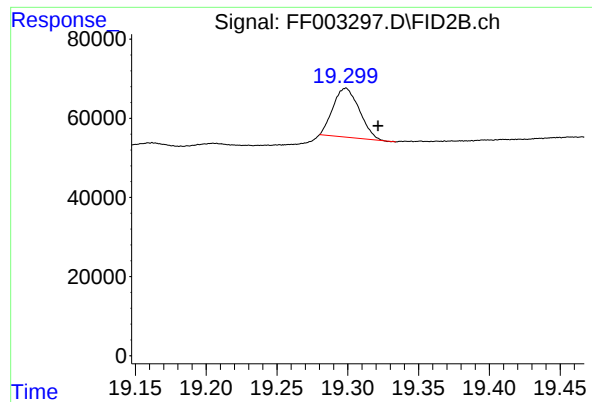

#15 N-TETRATRIACONTANE

R.T.: 19.298 min

Delta R.T.: -0.023 min

Response: 159287

Conc: 1.20 ug/ml

Instrument :
FID_F
ClientSampleId :