

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
Data File : FF003299.D
Signal(s) : FID2B.ch
Acq On : 18 Jan 2019 13:29
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 18 20:54:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.365	3874256	23.883 ug/ml
12)	N-OCTACOSANE	16.788	3577431	22.713 ug/ml
13)	N-TRIACONTANE	17.677	448824	2.859 ug/ml
14)	N-DOTRIACONTANE	18.511	508295	3.495 ug/ml
15)	N-TETRATRIACONTANE	19.298	271288	2.052 ug/ml
16)	N-HEXATRIACONTANE	20.042	94040	0.797 ug/ml
17)	N-OCTATRIACONTANE	20.777	142357	1.362 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
Data File : FF003299.D
Signal(s) : FID2B.ch
Acq On : 18 Jan 2019 13:29
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 18 20:54:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

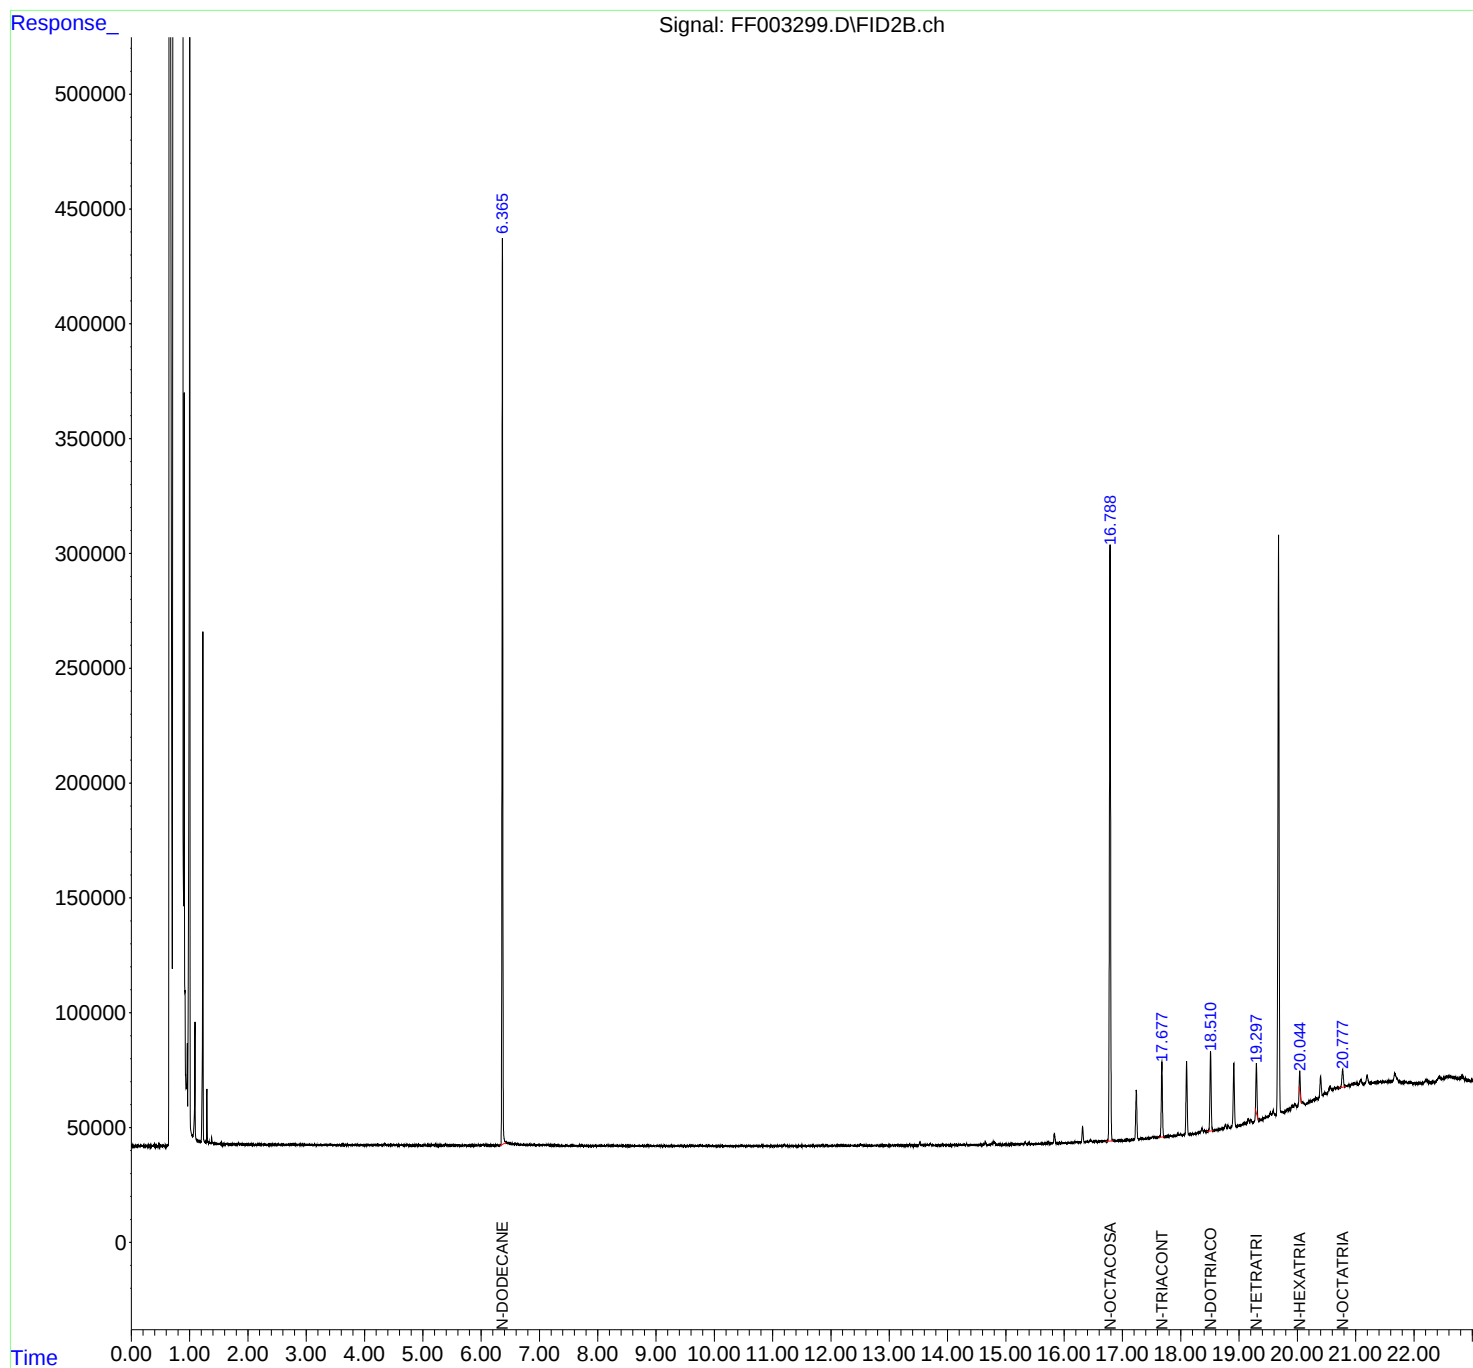


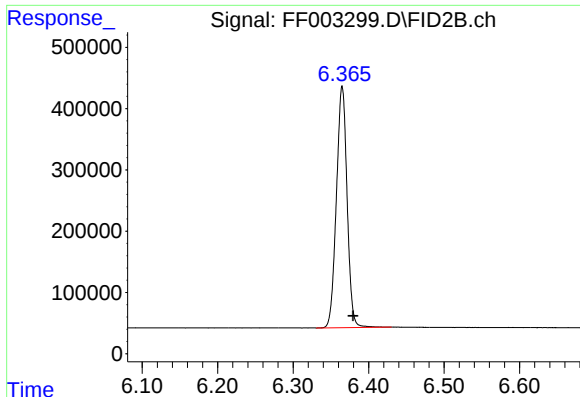

#3 N-DODECANE


R.T.: 6.365 min
Delta R.T.: -0.015 min
Response: 3874256
Conc: 23.88 ug/ml

Instrument :
FID_F
ClientSampleId :

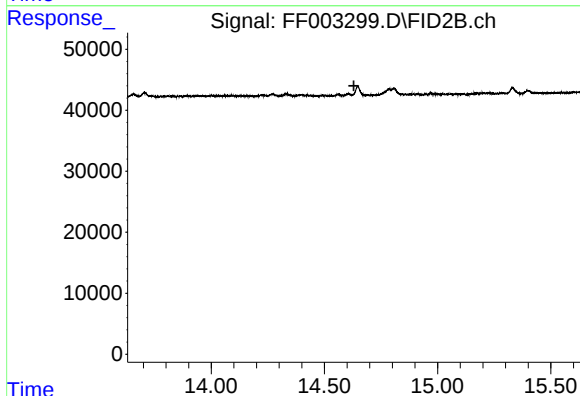


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.630 min
Response: 0
Conc: N.D.

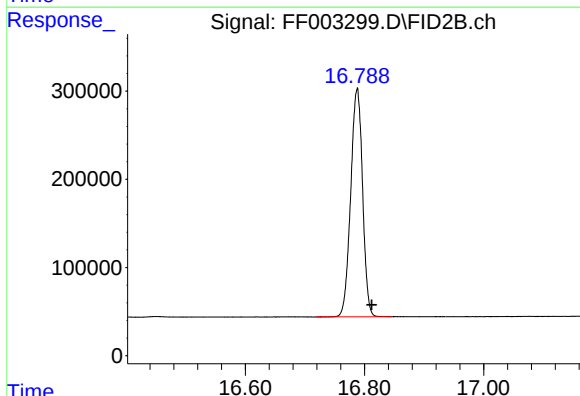


#12 N-OCTACOSANE

R.T.: 16.788 min
Delta R.T.: -0.024 min
Response: 3577431
Conc: 22.71 ug/ml

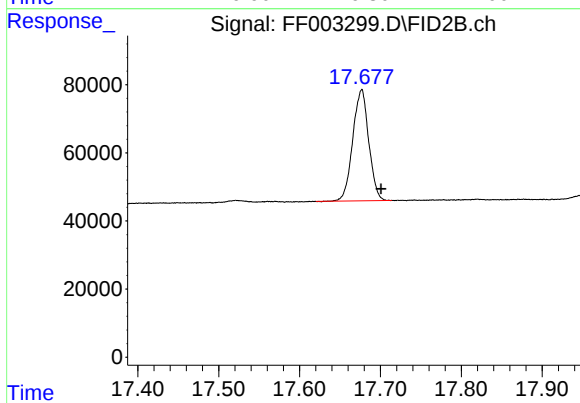

#13 N-TRIACONTANE


R.T.: 17.677 min
Delta R.T.: -0.024 min
Response: 448824
Conc: 2.86 ug/ml

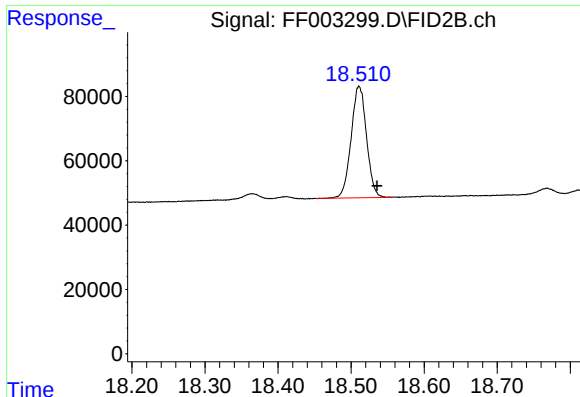

#14 N-DOTRIACONTANE


R.T.: 18.511 min
Delta R.T.: -0.024 min
Response: 508295
Conc: 3.50 ug/ml

Instrument :
FID_F
ClientSampleId :

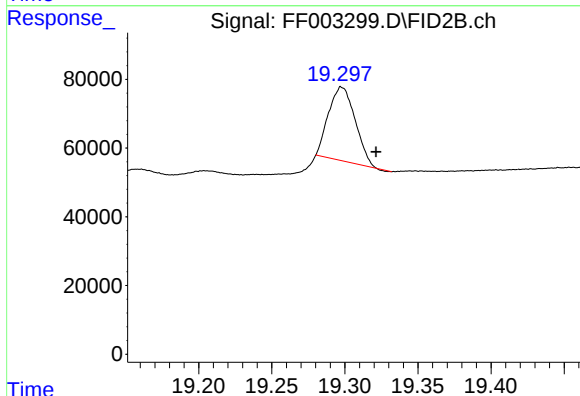


#15 N-TETRATRIACONTANE

R.T.: 19.298 min
Delta R.T.: -0.024 min
Response: 271288
Conc: 2.05 ug/ml

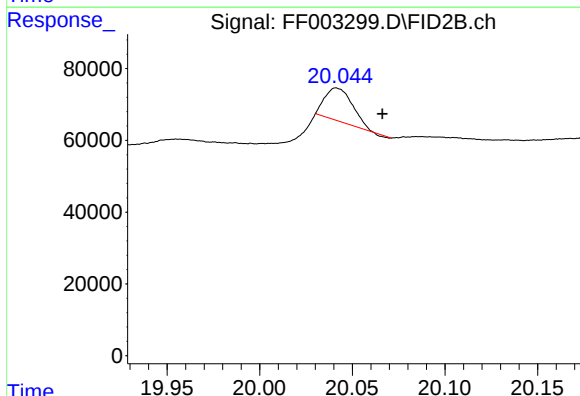

#16 N-HEXATRIACONTANE

R.T.: 20.042 min
Delta R.T.: -0.025 min
Response: 94040
Conc: 0.80 ug/ml

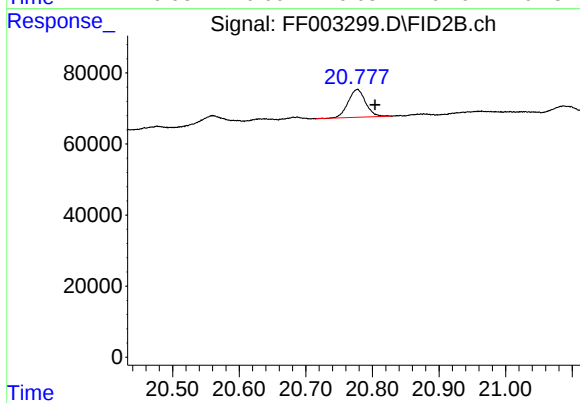

#17 N-OCTATRIACONTANE

R.T.: 20.777 min
Delta R.T.: -0.027 min
Response: 142357
Conc: 1.36 ug/ml