

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
 Data File : FF003302.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jan 2019 14:58
 Operator : AJ\SJ
 Sample : K1173-01
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 18 20:55:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Tue Jan 15 08:58:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.606	1832912	12.810 ug/ml
Target Compounds			
4) N-TETRADECANE	8.212	1115970	6.834 ug/ml
5) N-HEXADECANE	9.773	145828	0.888 ug/ml
8) N-DOCOSANE	13.704	138840	0.854 ug/ml
10) N-TETRACOSANE	14.810	331650	2.068 ug/ml
11) N-HEXACOSANE	15.832	423710	2.679 ug/ml
12) N-OCTACOSANE	16.786	528106	3.353 ug/ml
13) N-TRIACONTANE	17.676	533823	3.400 ug/ml
14) N-DOTRIACONTANE	18.511	344523	2.369 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF011819\
Data File : FF003302.D
Signal(s) : FID2B.ch
Acq On : 18 Jan 2019 14:58
Operator : AJ\SJ
Sample : K1173-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 18 20:55:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Tue Jan 15 08:58:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

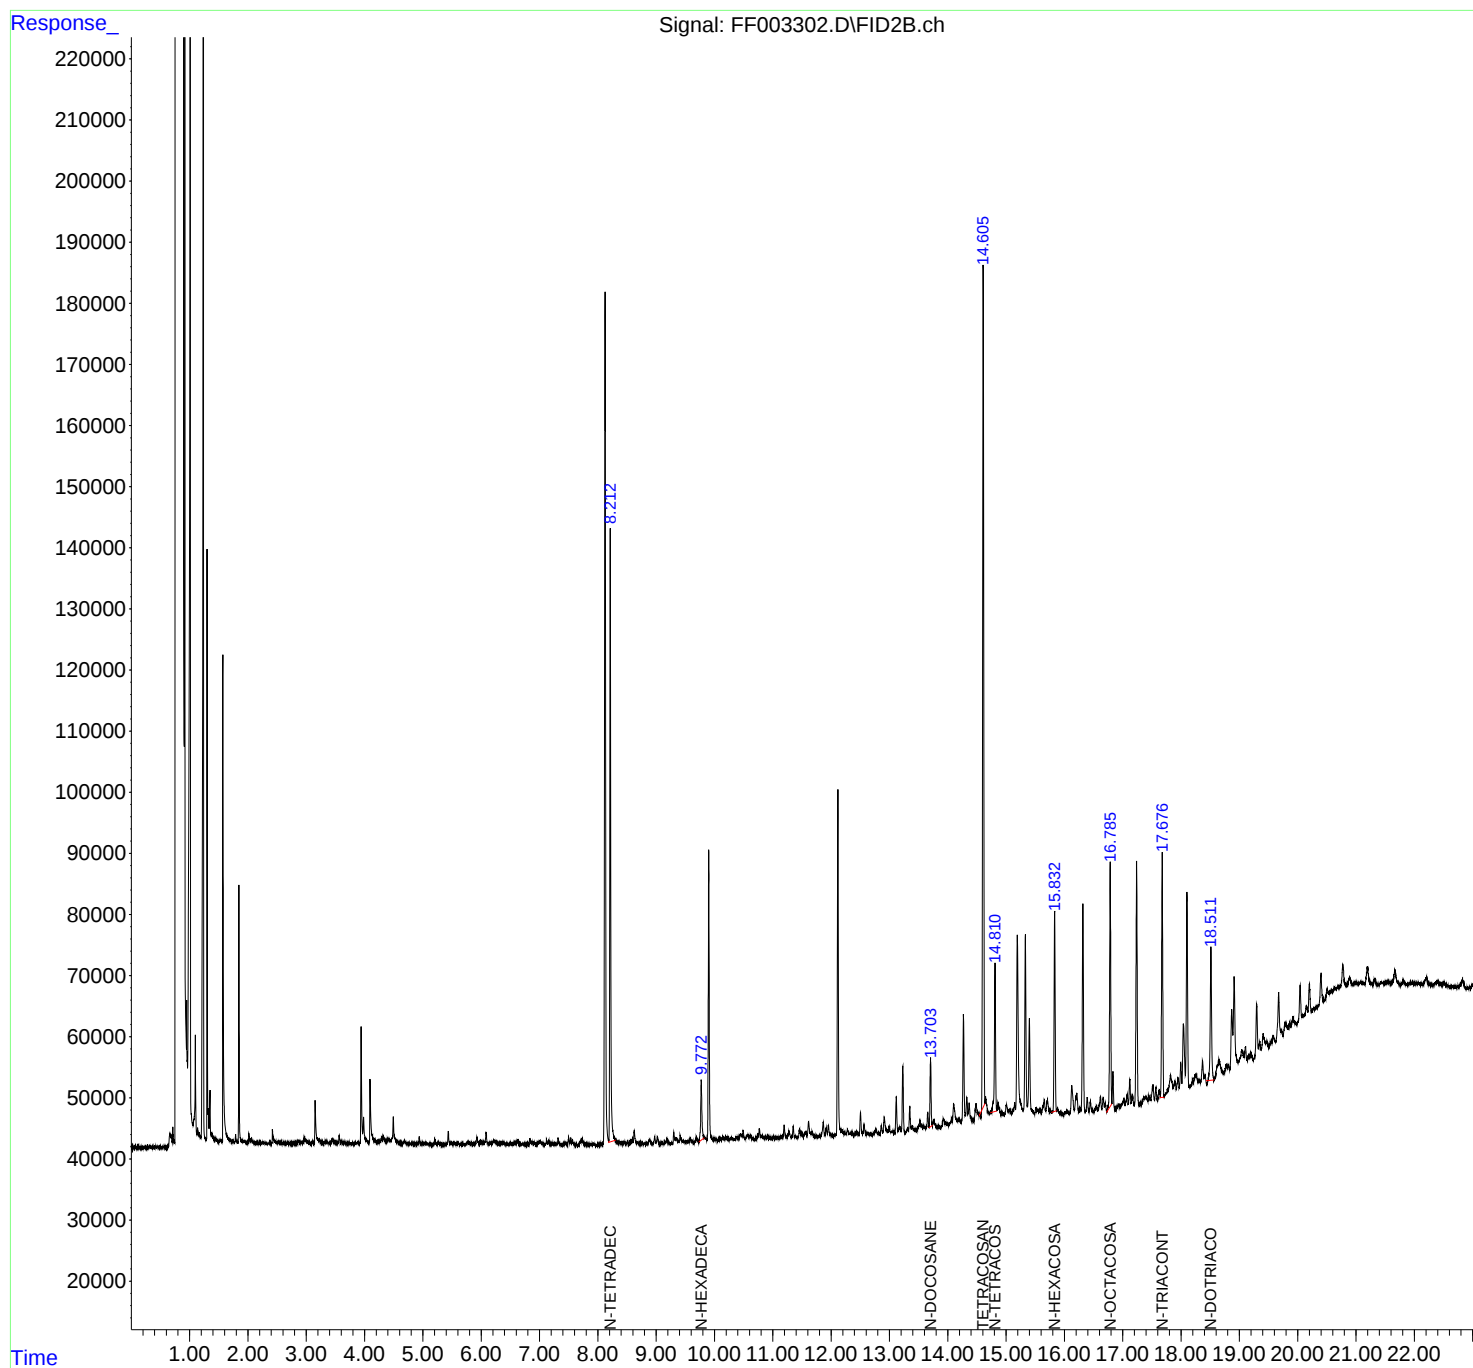


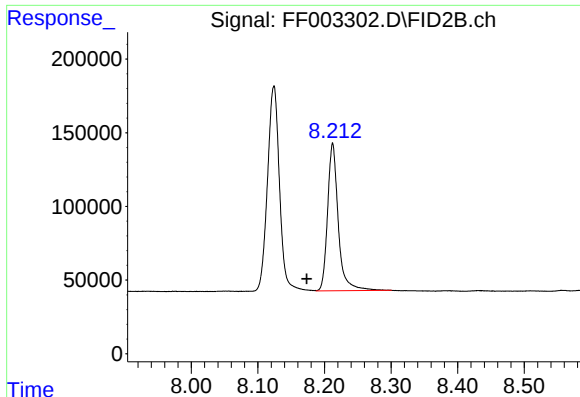

#4 N-TETRADECANE


R.T.: 8.212 min
Delta R.T.: 0.039 min
Response: 1115970
Conc: 6.83 ug/ml

Instrument :
FID_F
ClientSampleId :

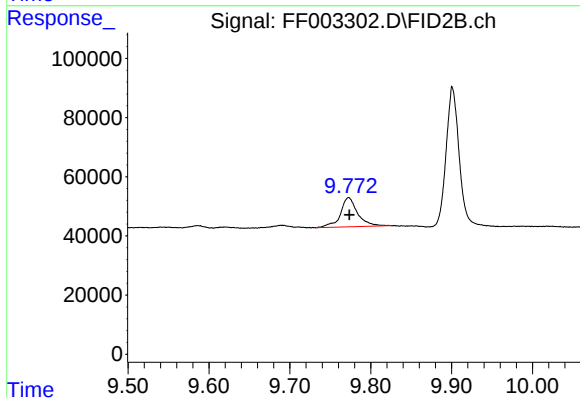


#5 N-HEXADECANE

R.T.: 9.773 min
Delta R.T.: 0.000 min
Response: 145828
Conc: 0.89 ug/ml

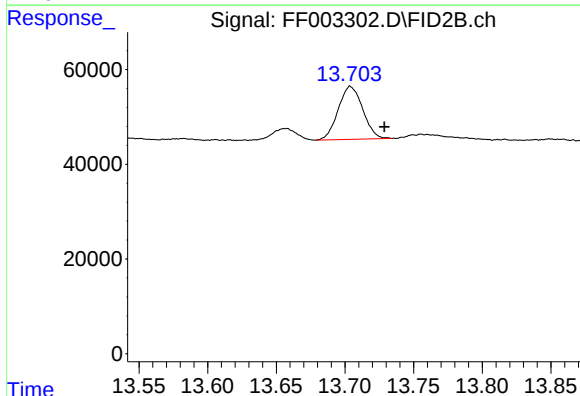


#8 N-DOCOSANE

R.T.: 13.704 min
Delta R.T.: -0.025 min
Response: 138840
Conc: 0.85 ug/ml

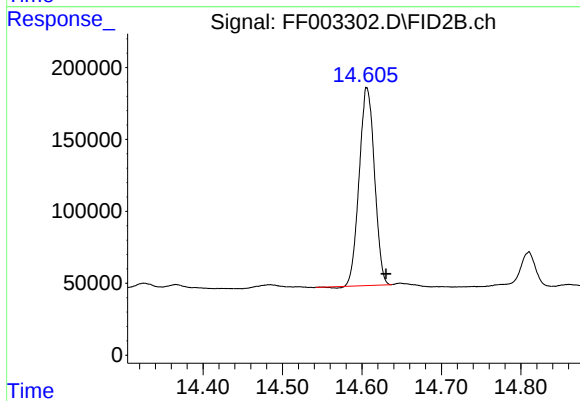

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.606 min
Delta R.T.: -0.024 min
Response: 1832912
Conc: 12.81 ug/ml

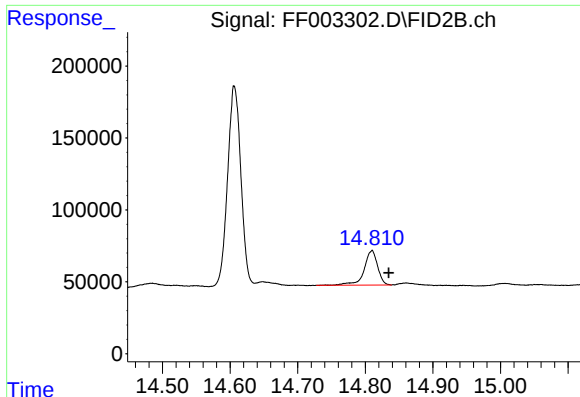

#10 N-TETRACOSANE


R.T.: 14.810 min
Delta R.T.: -0.025 min
Response: 331650
Conc: 2.07 ug/ml

Instrument :
FID_F
ClientSampleId :

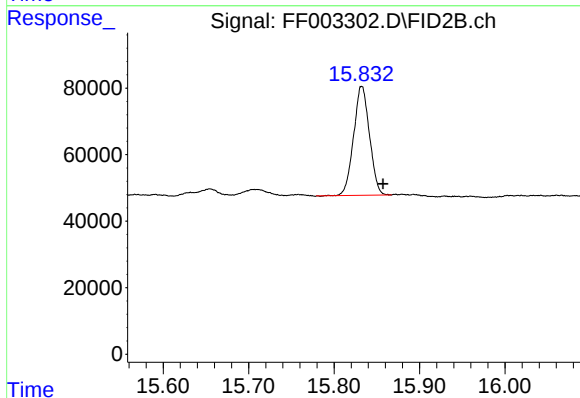


#11 N-HEXACOSANE

R.T.: 15.832 min
Delta R.T.: -0.025 min
Response: 423710
Conc: 2.68 ug/ml

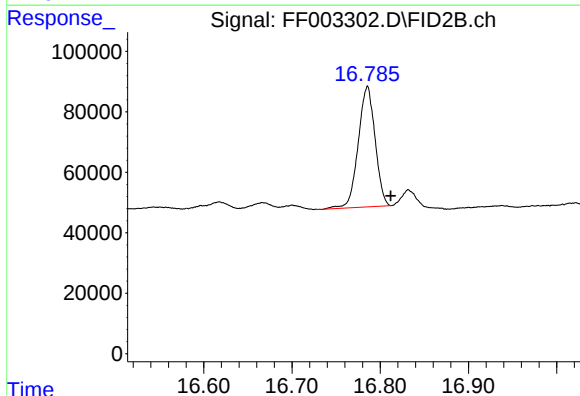


#12 N-OCTACOSANE

R.T.: 16.786 min
Delta R.T.: -0.026 min
Response: 528106
Conc: 3.35 ug/ml

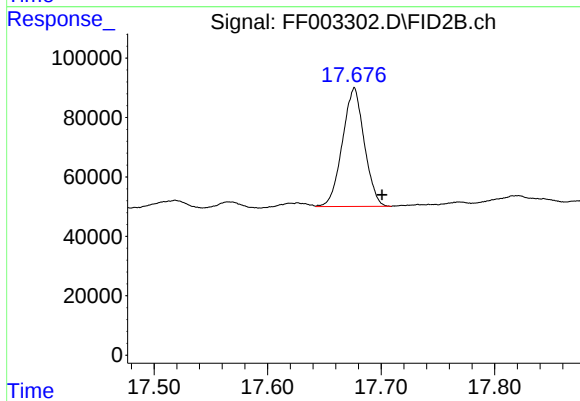

#13 N-TRIACONTANE

R.T.: 17.676 min
Delta R.T.: -0.024 min
Response: 533823
Conc: 3.40 ug/ml

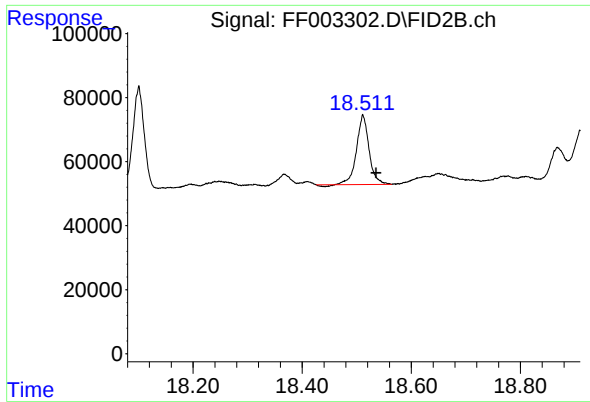

#14 N-DOTRIACONTANE

R.T.: 18.511 min
Delta R.T.: -0.024 min
Response: 344523
Conc: 2.37 ug/ml

Instrument :
FID_F
ClientSampleId :